

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030519\
 Data File : P0054228.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Mar 2019 16:43
 Operator : SM/SJ
 Sample : K1700-01RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 NB-21841-21842RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 23:41:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 05 06:51:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.033	3.119	34860913	4106817	6.269	13.071 #
2) SA Decachlor...	9.354	7.688	13995969	3817503	9.426	11.936 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030519\
Data File : P0054228.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Mar 2019 16:43
Operator : SM/SJ
Sample : K1700-01RE
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
NB-21841-21842RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 23:41:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030419.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 05 06:51:55 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

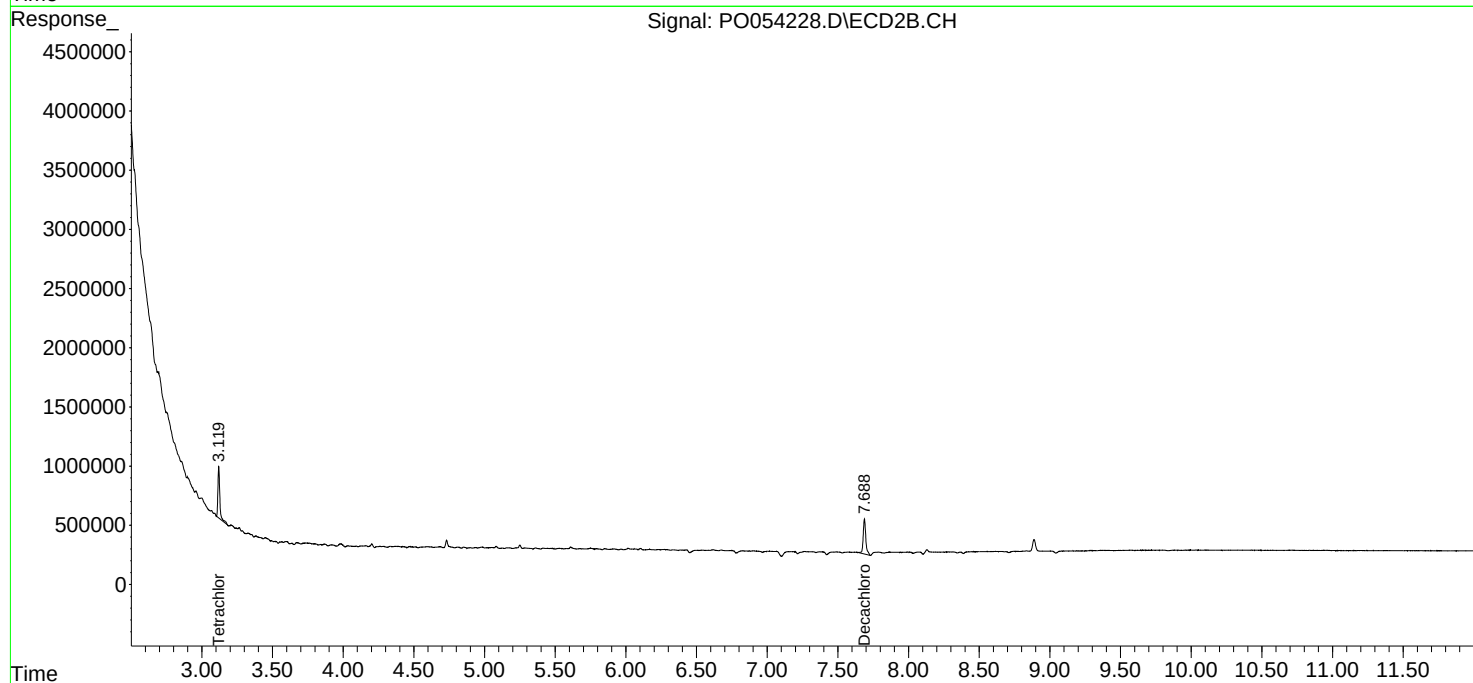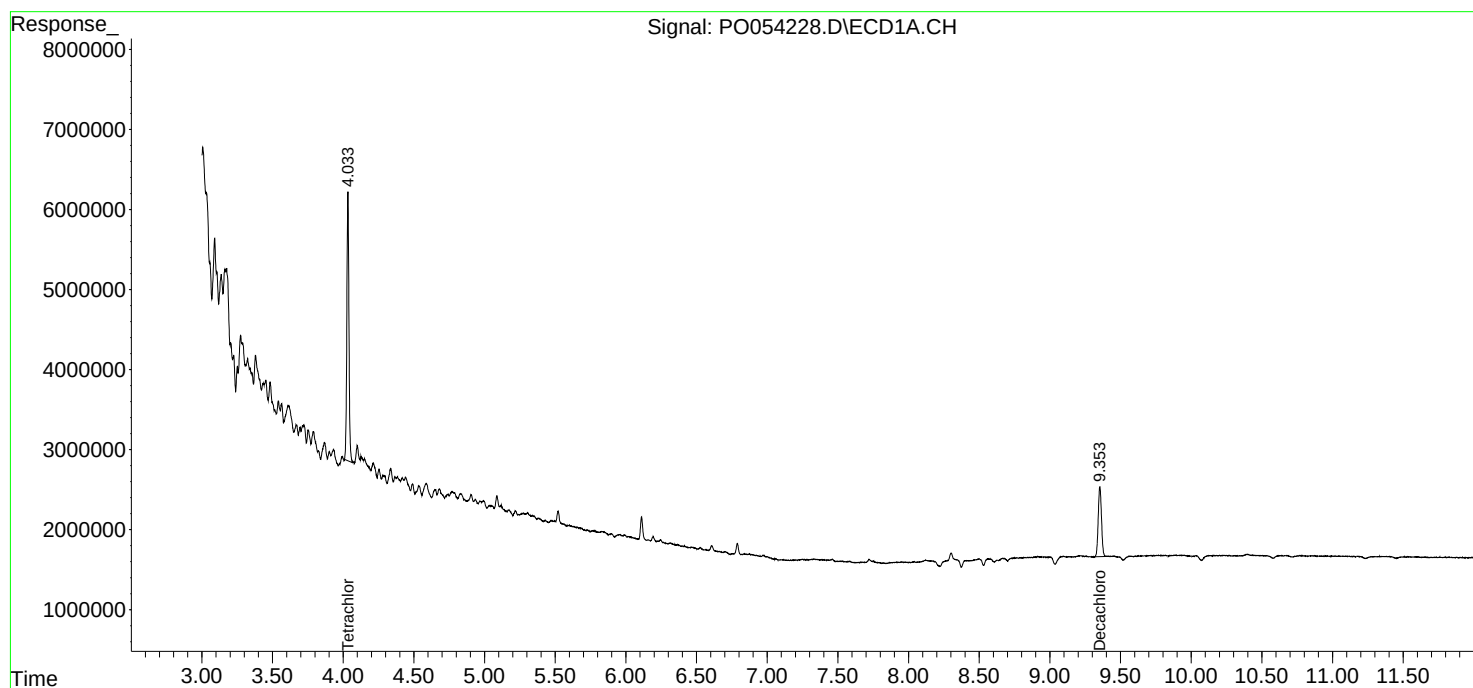


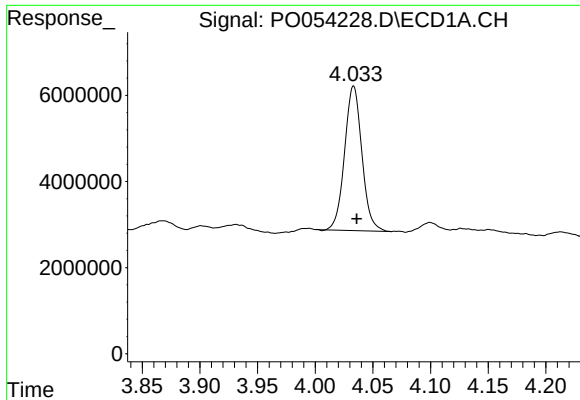

#1 Tetrachloro-m-xylene


R.T.: 4.033 min
Delta R.T.: -0.003 min
Response: 34860913
Conc: 6.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
NB-21841-21842RE

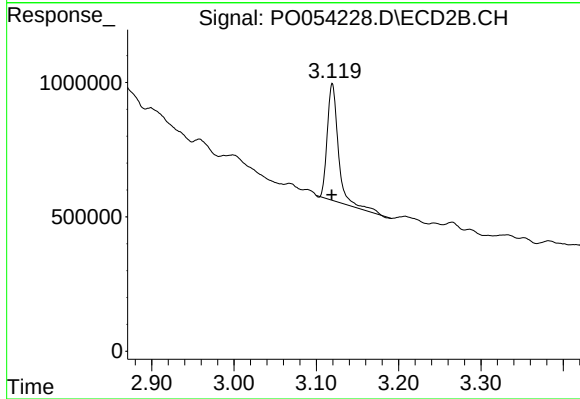


#1 Tetrachloro-m-xylene

R.T.: 3.119 min
Delta R.T.: 0.000 min
Response: 4106817
Conc: 13.07 ng/ml

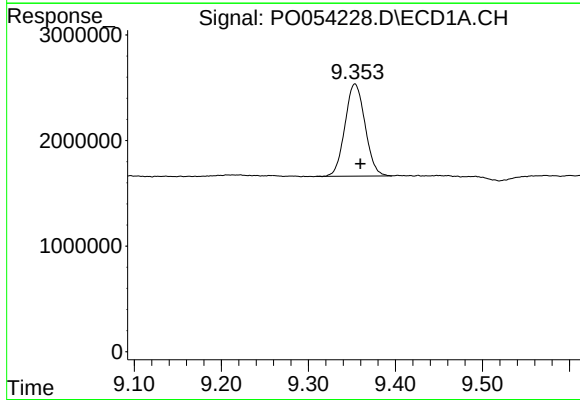

#2 Decachlorobiphenyl

R.T.: 9.354 min
Delta R.T.: -0.006 min
Response: 13995969
Conc: 9.43 ng/ml

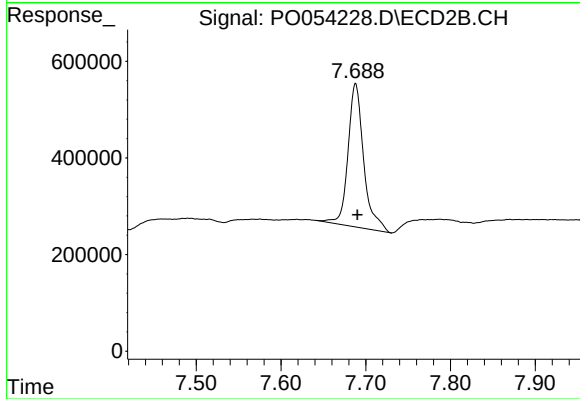

#2 Decachlorobiphenyl

R.T.: 7.688 min
Delta R.T.: -0.002 min
Response: 3817503
Conc: 11.94 ng/ml