

Data Path : P:\HPCHEM1\ECD_P\Data\PP030618\
 Data File : PP024241.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Mar 2018 15:23
 Operator : UA/AJ
 Sample : J1724-15
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SP-25

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 01:32:09 2018
 Quant Method : P:\HPCHEM1\ECD_P\methods\PP020618.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 06 02:07:55 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.575	11.365	114.0E6	159.1E6	222.500	262.344
Target Compounds							
2) T	3,5-DICHL...	0.000	9.457	0	2923312	N.D.	3.505 #
3) T	4-Nitroph...	0.000	10.528	0	6321873	N.D.	13.622 #
5) T	DICAMBA	11.939	0.000	2109138	0	0.981	N.D. #
6) T	MCPD	12.256	11.830	5587736	4637691	3.811	2.882
7) T	MCPA	12.541	12.340	-1940899	19145269	N.D.	8.222
8) T	DICHLORPROP	13.057	12.733	21007298	2897847	39.548	4.936 #
9) T	2,4-D	0.000	13.324	0	1101250	N.D.	1.434 #
10) T	Pentachlo...	13.826	13.820	524.2E6	553.1E6	64.484	64.238
11) T	2,4,5-TP ...	14.770	14.435	22287304	2287701	6.728	0.639 #
12) T	2,4,5-T	0.000	15.064	0	37491558	N.D.	12.170 #
13) T	2,4-DB	15.856	15.638	54720305	21507839	139.174	49.751 #
14) T	DINOSEB	17.328	16.108	19637828	301.1E6	8.556	122.411 #
15) T	Picloram	0.000	17.397	0	40890337	N.D.	8.209 #
16) T	DCPA	0.000	17.271	0	29023503	N.D.	6.671 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_P\Data\PP030618\
Data File : PP024241.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Mar 2018 15:23
Operator : UA/AJ
Sample : J1724-15
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SP-25

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 01:32:09 2018
Quant Method : P:\HPCHEM1\ECD_P\methods\PP020618.M
Quant Title : 8080.M
QLast Update : Tue Feb 06 02:07:55 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

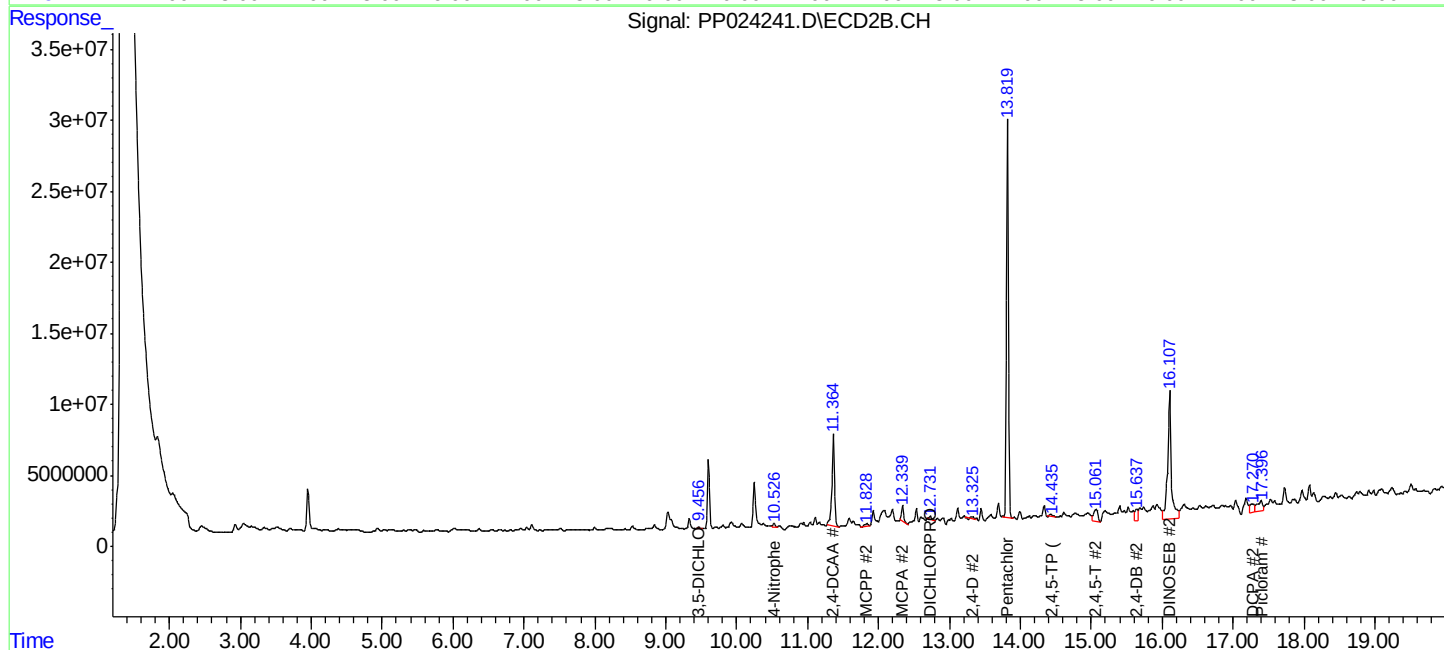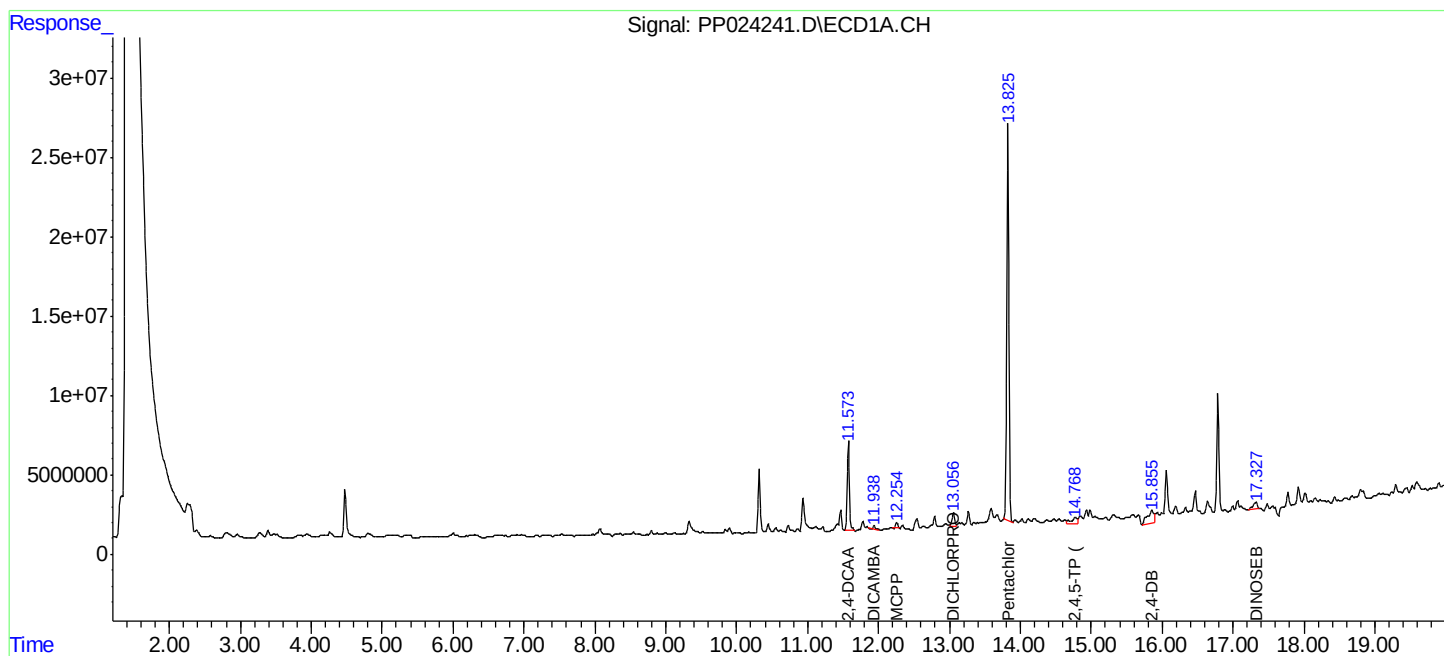


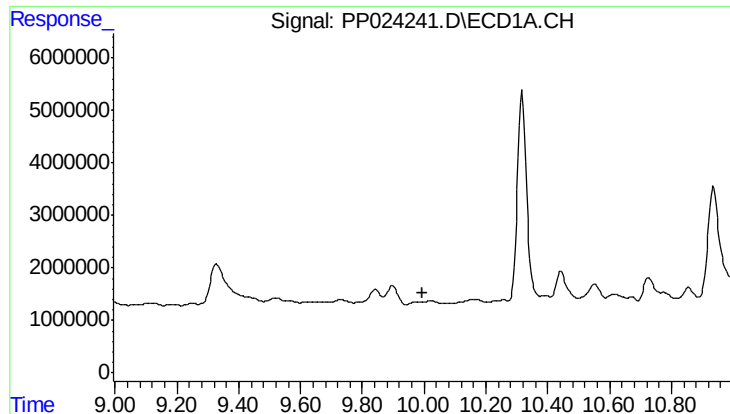

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.994 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SP-25

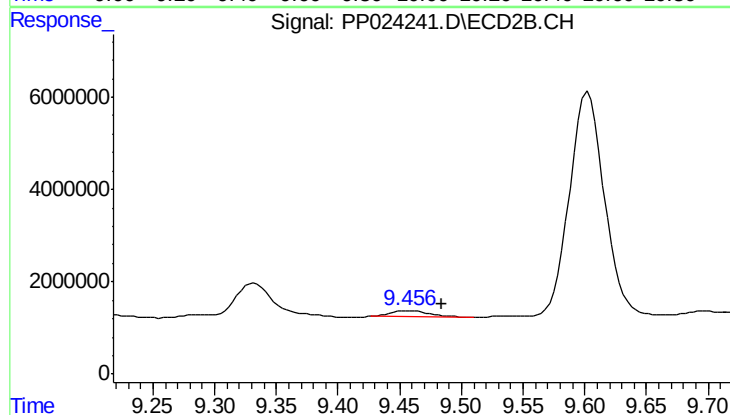


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.457 min
Delta R.T.: -0.027 min
Response: 2923312
Conc: 3.50 ng/ml

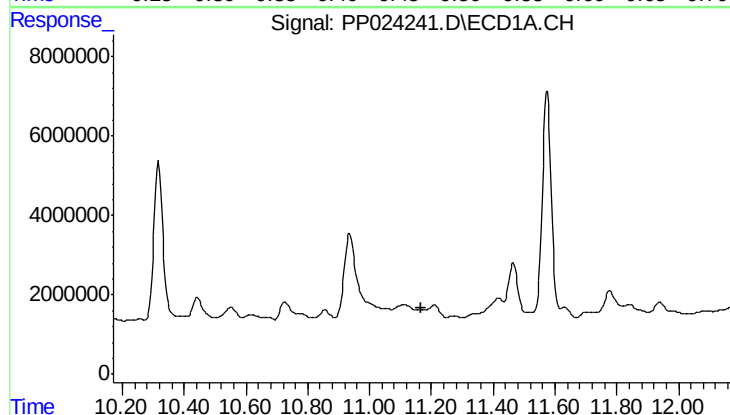


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 11.169 min
Response: 0
Conc: N.D.

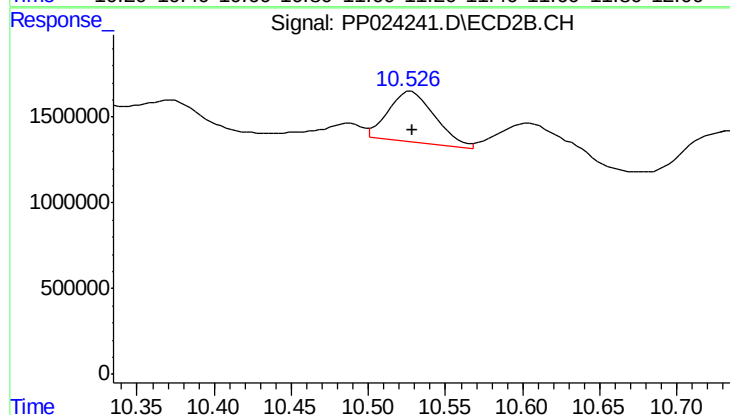

#3 4-Nitrophenol


R.T.: 10.528 min
Delta R.T.: 0.000 min
Response: 6321873
Conc: 13.62 ng/ml

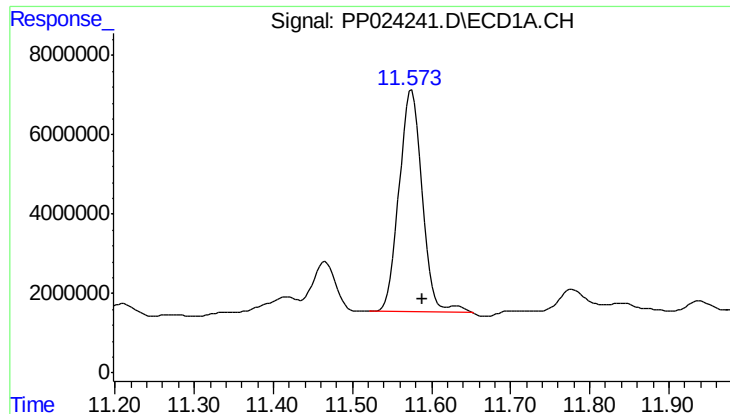

#4 2,4-DCAA


R.T.: 11.575 min
Delta R.T.: -0.014 min
Response: 114024819
Conc: 222.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-25

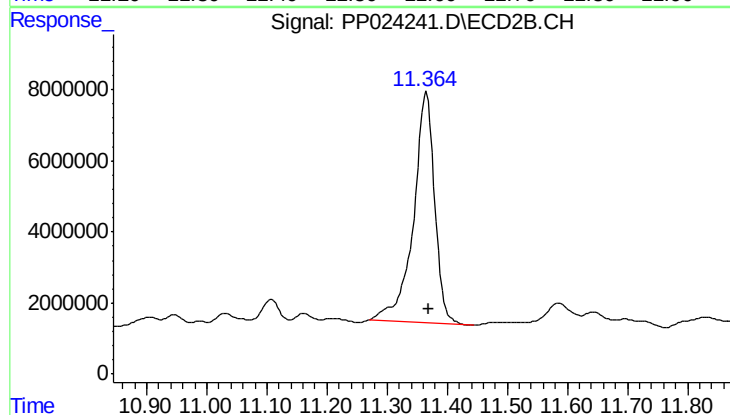


#4 2,4-DCAA

R.T.: 11.365 min
Delta R.T.: -0.003 min
Response: 159090409
Conc: 262.34 ng/ml

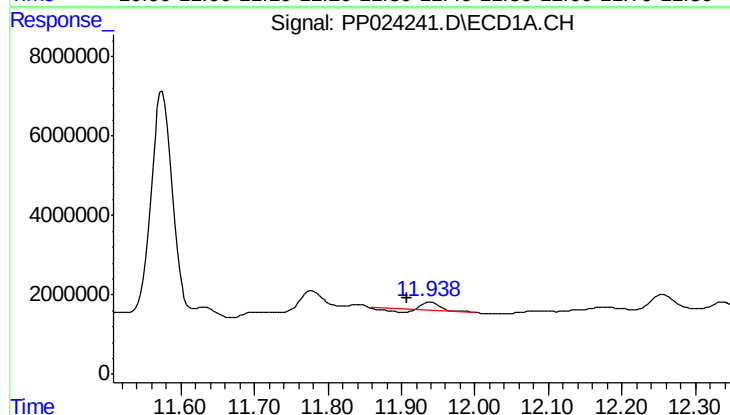


#5 DICAMBA

R.T.: 11.939 min
Delta R.T.: 0.031 min
Response: 2109138
Conc: 0.98 ng/ml

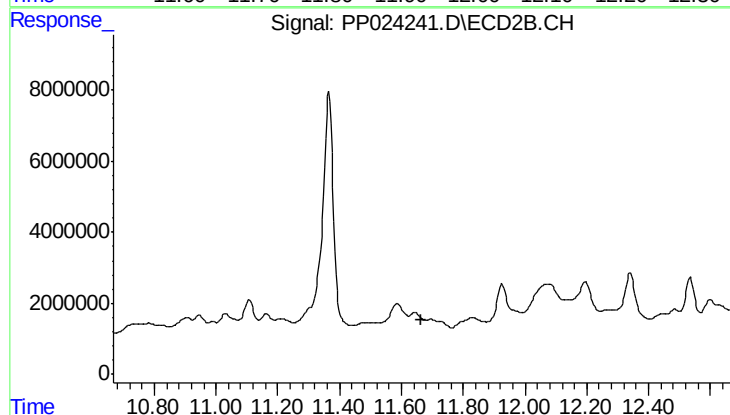

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.666 min
Response: 0
Conc: N.D.

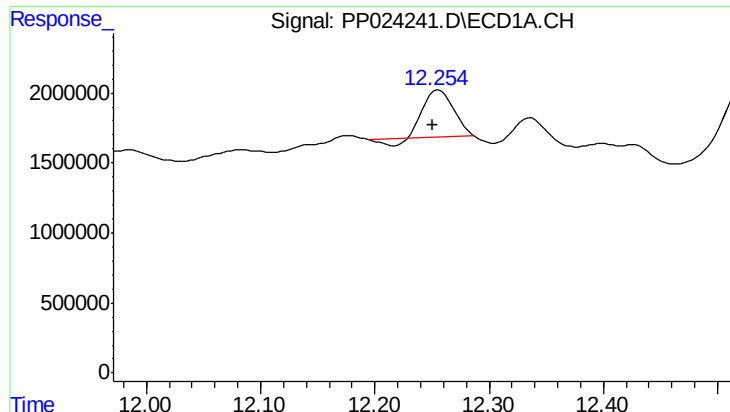

#6 MCPP


R.T.: 12.256 min
Delta R.T.: 0.006 min
Response: 5587736
Conc: 3.81 ug/ml

Instrument :
ECD_O
ClientSampleId :
SP-25

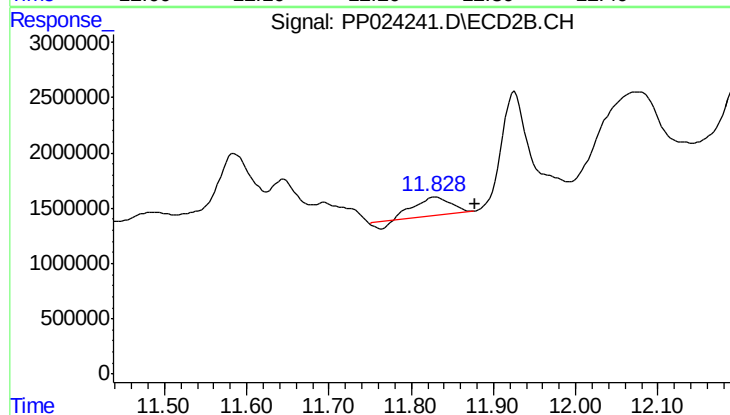


#6 MCPP

R.T.: 11.830 min
Delta R.T.: -0.048 min
Response: 4637691
Conc: 2.88 ug/ml

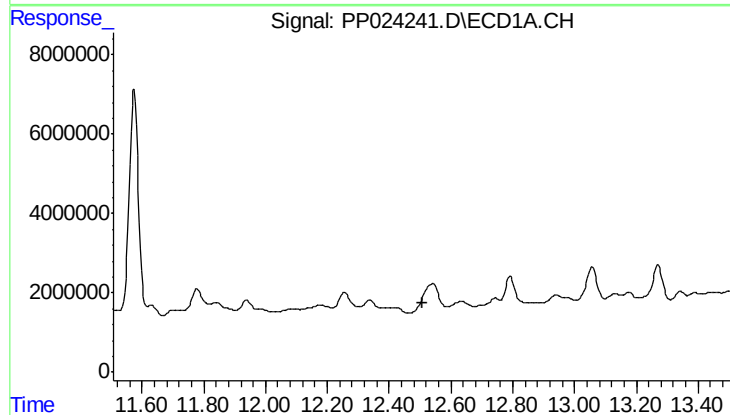


#7 MCPA

R.T.: 12.541 min
Delta R.T.: 0.034 min
Response: -1940899
Conc: N.D.

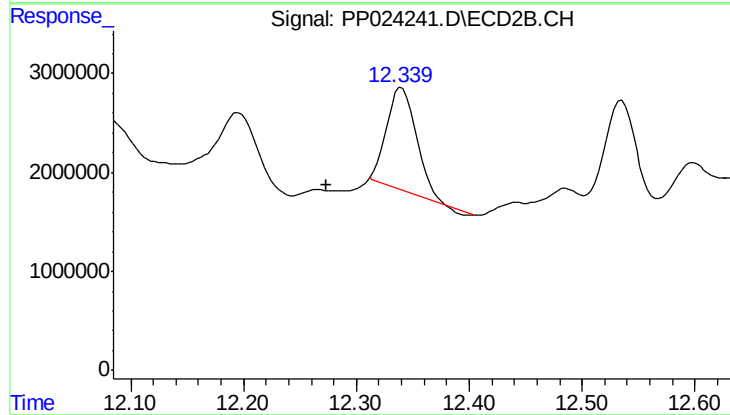

#7 MCPA


R.T.: 12.340 min
Delta R.T.: 0.067 min
Response: 19145269
Conc: 8.22 ug/ml

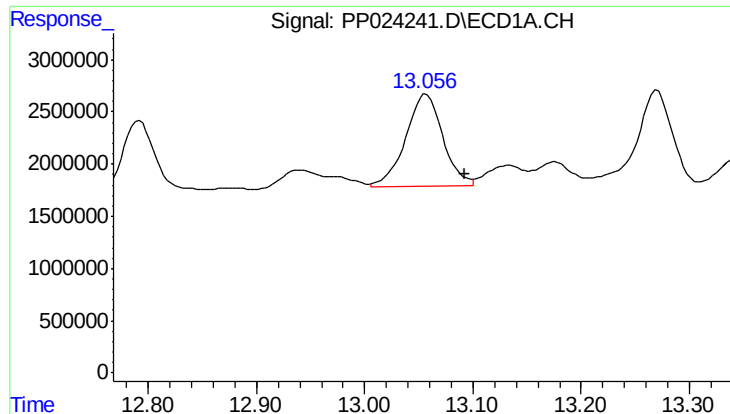

#8 DICHLORPROP


R.T.: 13.057 min
Delta R.T.: -0.036 min
Response: 21007298
Conc: 39.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-25

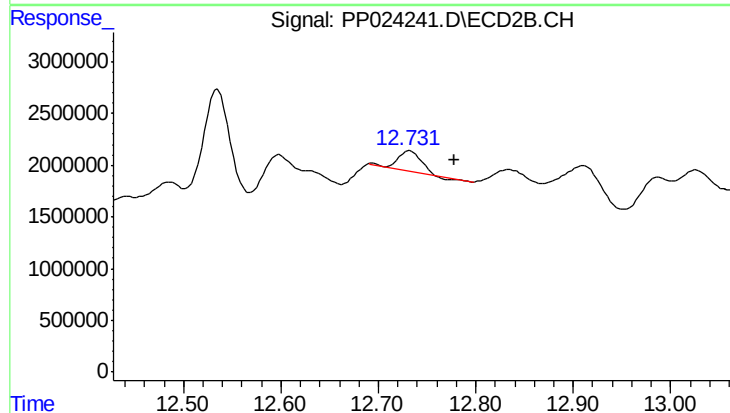


#8 DICHLORPROP

R.T.: 12.733 min
Delta R.T.: -0.045 min
Response: 2897847
Conc: 4.94 ng/ml

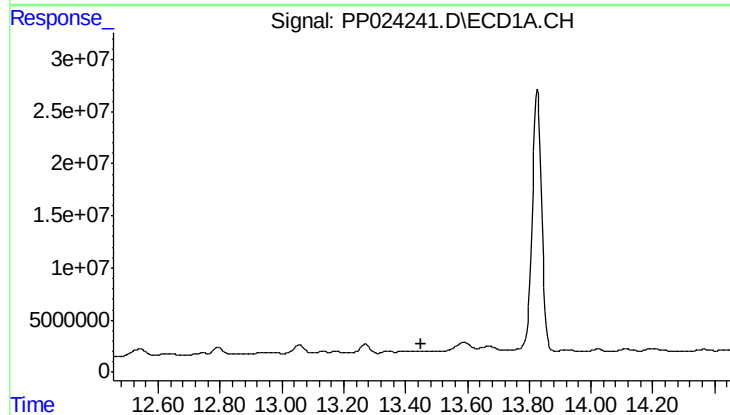


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 13.453 min
Response: 0
Conc: N.D.

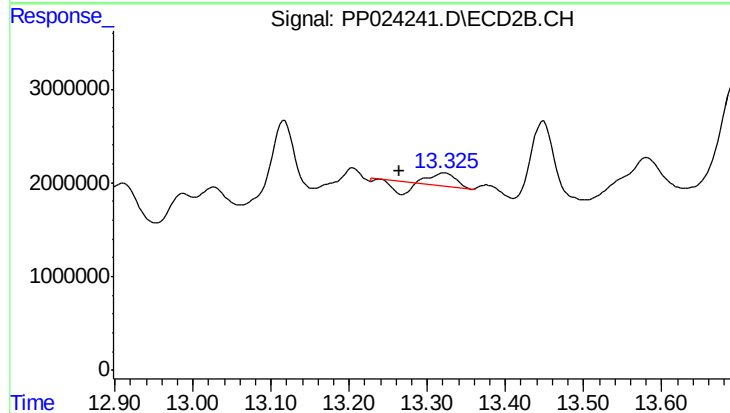

#9 2,4-D


R.T.: 13.324 min
Delta R.T.: 0.059 min
Response: 1101250
Conc: 1.43 ng/ml

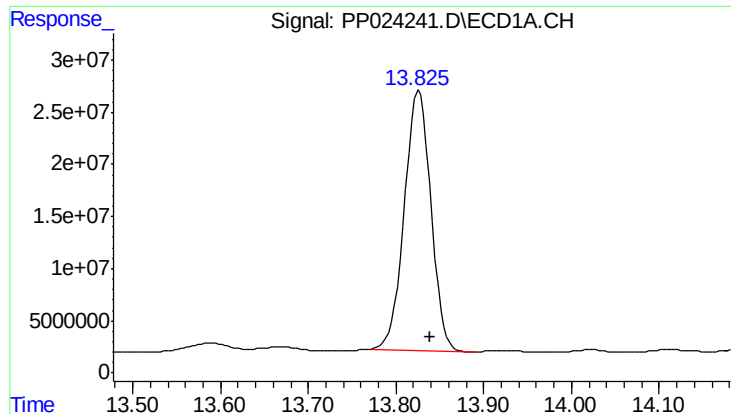

#10 Pentachlorophenol


R.T.: 13.826 min
Delta R.T.: -0.012 min
Response: 524198616
Conc: 64.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-25

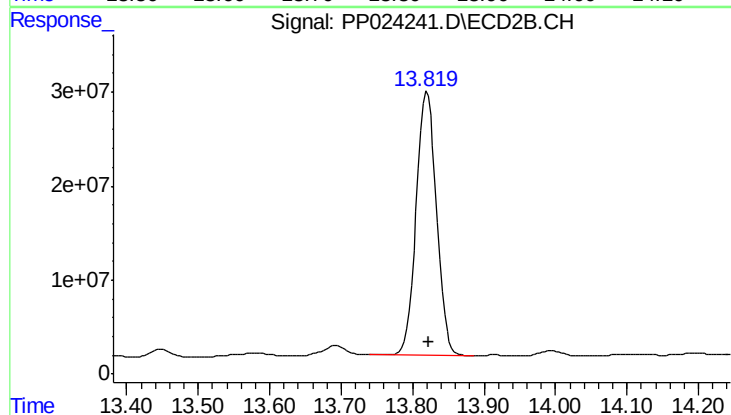


#10 Pentachlorophenol

R.T.: 13.820 min
Delta R.T.: -0.003 min
Response: 553058347
Conc: 64.24 ng/ml

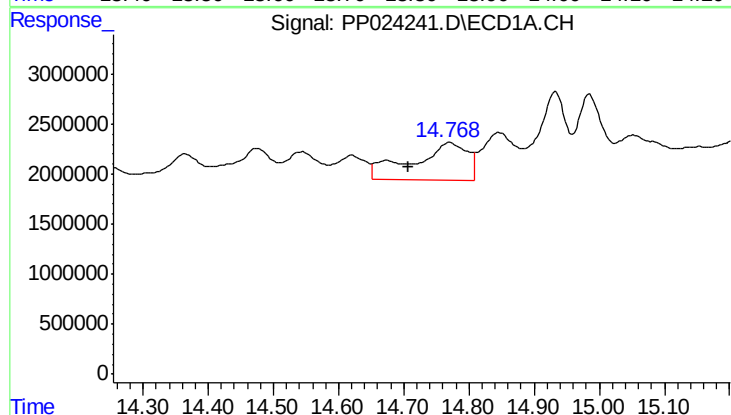


#11 2,4,5-TP (SILVEX)

R.T.: 14.770 min
Delta R.T.: 0.064 min
Response: 22287304
Conc: 6.73 ng/ml

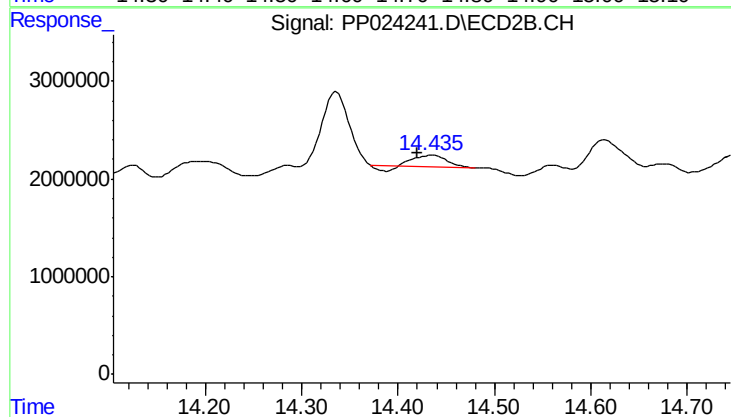

#11 2,4,5-TP (SILVEX)


R.T.: 14.435 min
Delta R.T.: 0.015 min
Response: 2287701
Conc: 0.64 ng/ml

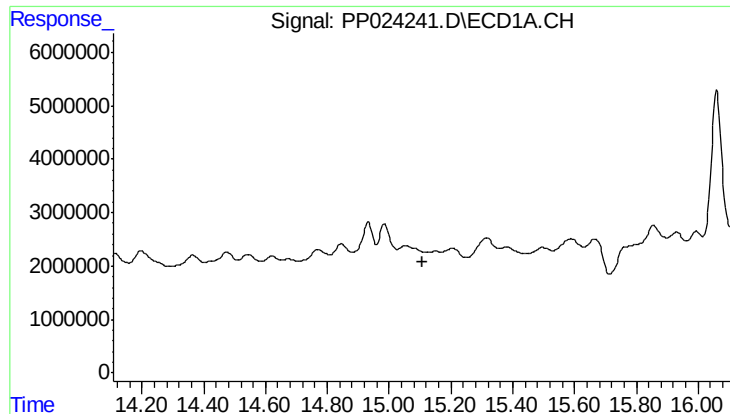

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.106 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SP-25

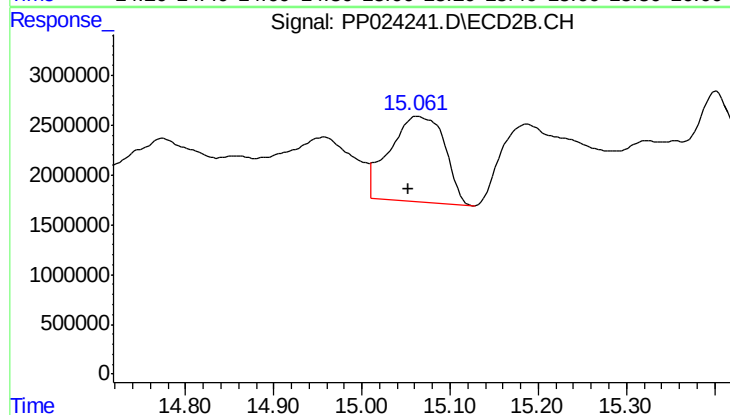


#12 2,4,5-T

R.T.: 15.064 min
Delta R.T.: 0.011 min
Response: 37491558
Conc: 12.17 ng/ml

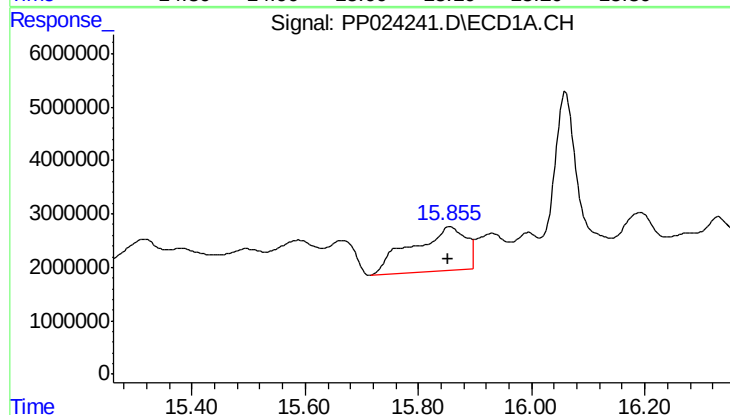


#13 2,4-DB

R.T.: 15.856 min
Delta R.T.: 0.004 min
Response: 54720305
Conc: 139.17 ng/ml

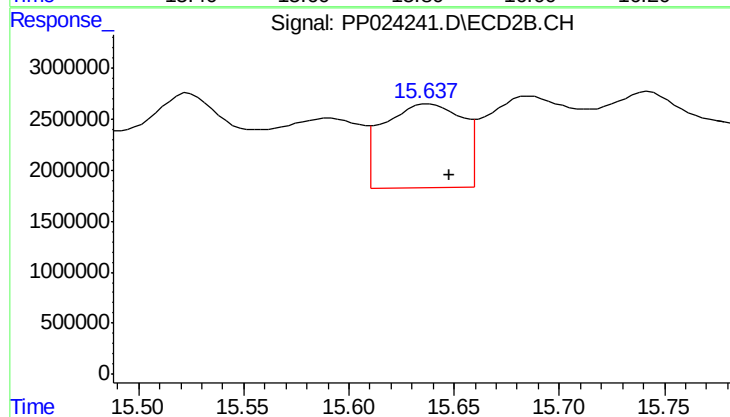

#13 2,4-DB


R.T.: 15.638 min
Delta R.T.: -0.009 min
Response: 21507839
Conc: 49.75 ng/ml

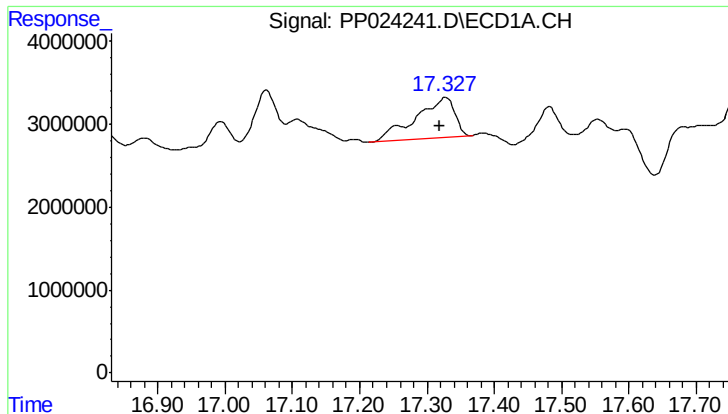

#14 DINOSEB


R.T.: 17.328 min
Delta R.T.: 0.009 min
Response: 19637828
Conc: 8.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-25

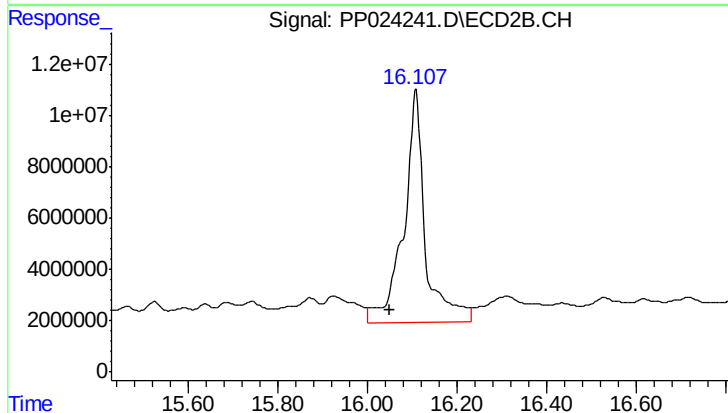


#14 DINOSEB

R.T.: 16.108 min
Delta R.T.: 0.059 min
Response: 301116313
Conc: 122.41 ng/ml

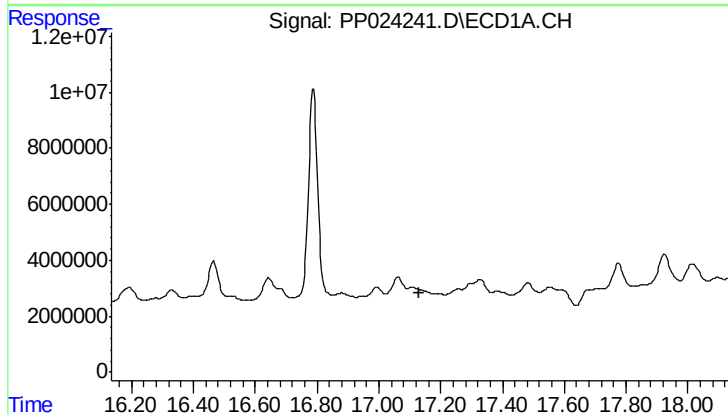


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 17.132 min
Response: 0
Conc: N.D.

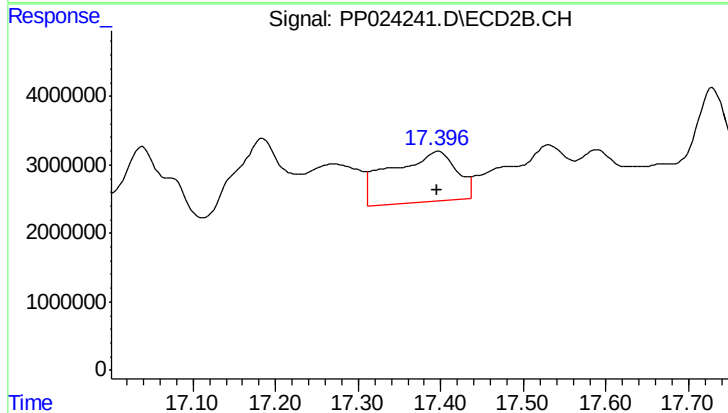

#15 Picloram


R.T.: 17.397 min
Delta R.T.: 0.002 min
Response: 40890337
Conc: 8.21 ng/ml

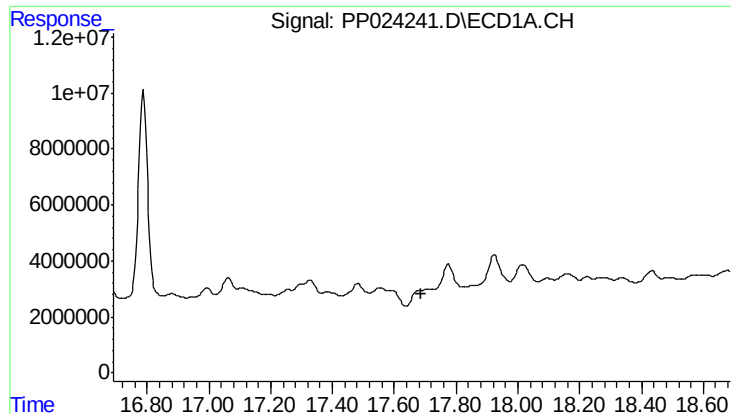

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.689 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SP-25

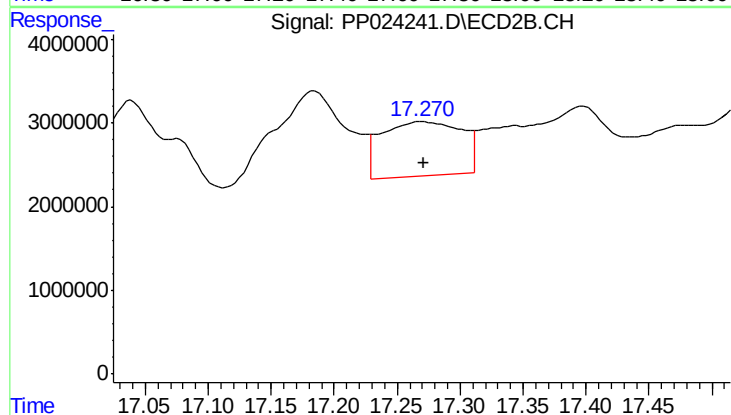

#16 DCPA

R.T.: 17.271 min
Delta R.T.: 0.000 min
Response: 29023503
Conc: 6.67 ng/ml