

Data Path : P:\HPCHEM1\ECD_P\Data\PP030618\
 Data File : PP024249.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Mar 2018 18:39
 Operator : UA/AJ
 Sample : J1783-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SLUDGE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 01:34:31 2018
 Quant Method : P:\HPCHEM1\ECD_P\methods\PP020618.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 06 02:07:55 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.575	11.366	216.8E6	232.8E6	423.004	383.843
Target Compounds							
2) T	3,5-DICHL...	0.000	9.460	0	3218674	N.D.	3.859 #
3) T	4-Nitroph...	11.215	10.525	7420778	5677785	17.259	12.234 #
6) T	MCP	12.256	0.000	28817474	0	19.655	N.D. #
8) T	DICHLORPROP	0.000	12.730	0	36933103	N.D.	62.908 #
10) T	Pentachlo...	13.826	13.820	6357843	8711014	0.782	1.012 #
11) T	2,4,5-TP ...	14.762	0.000	16693672	0	5.040	N.D. #
12) T	2,4,5-T	0.000	15.054	0	19527404	N.D.	6.339 #
14) T	DINOSEB	0.000	16.108	0	93675601	N.D.	38.081 #
15) T	Picloram	17.107	17.389	6430159	16815422	1.321	3.376 #
16) T	DCPA	0.000	17.277	0	15254225	N.D.	3.506 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_P\Data\PP030618\
Data File : PP024249.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Mar 2018 18:39
Operator : UA/AJ
Sample : J1783-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
SLUDGE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 01:34:31 2018
Quant Method : P:\HPCHEM1\ECD_P\methods\PP020618.M
Quant Title : 8080.M
QLast Update : Tue Feb 06 02:07:55 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

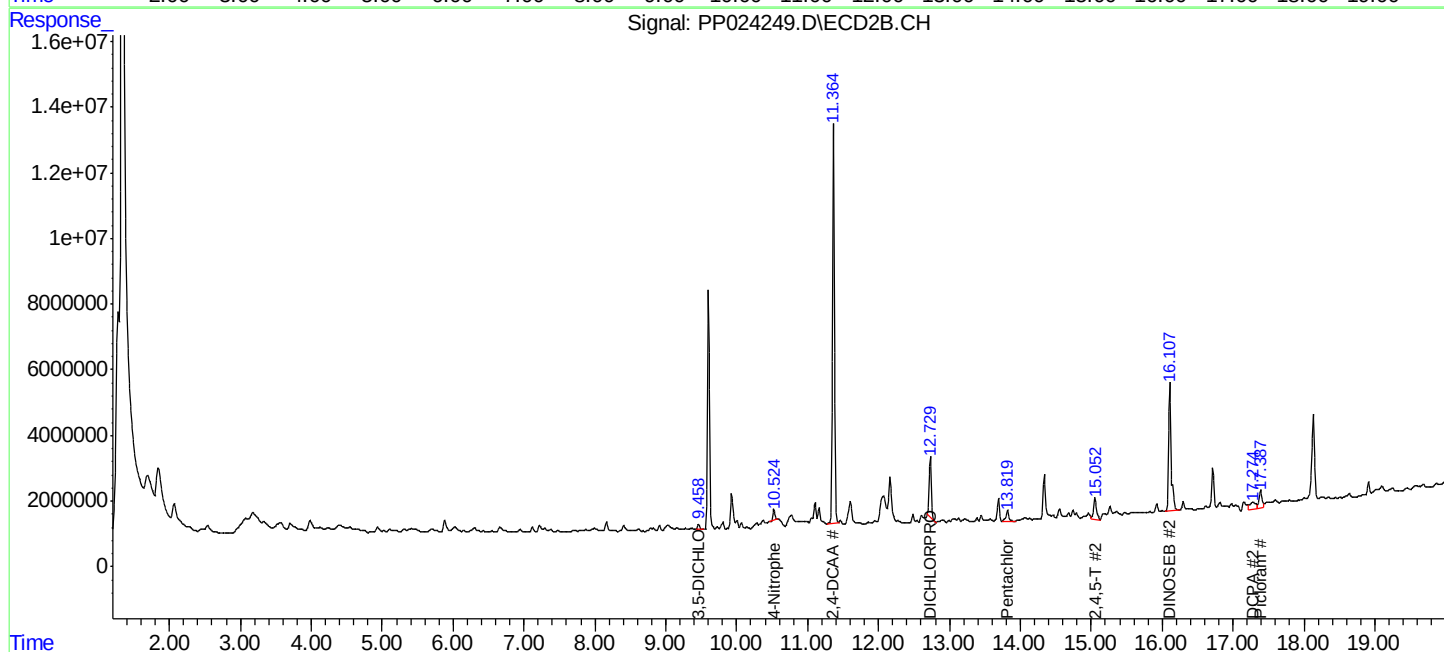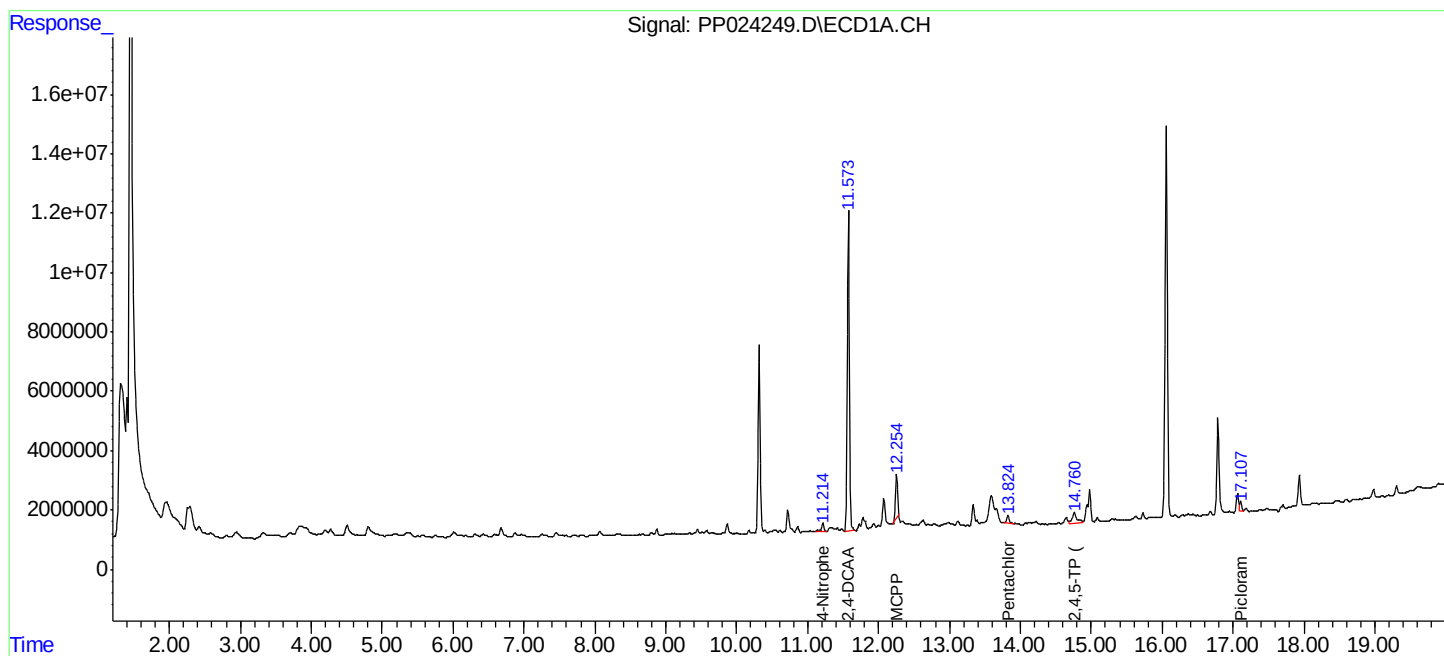


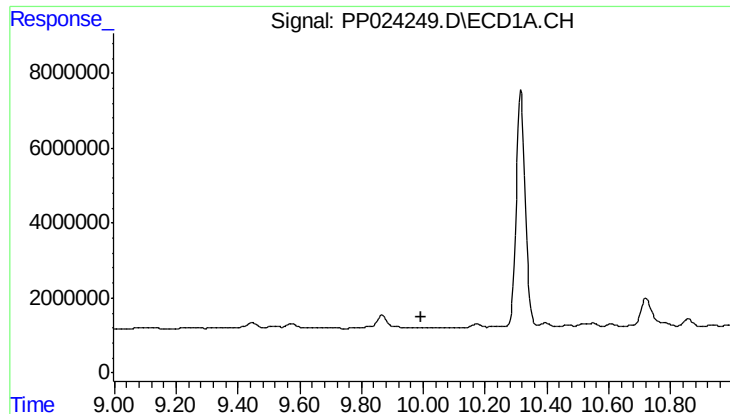

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.994 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SLUDGE

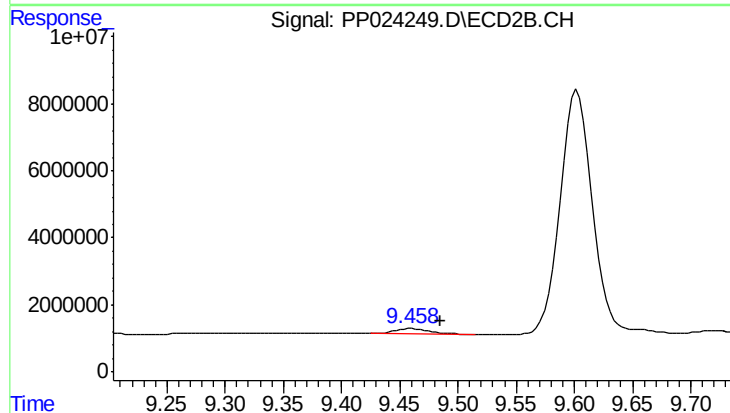


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.460 min
Delta R.T.: -0.025 min
Response: 3218674
Conc: 3.86 ng/ml

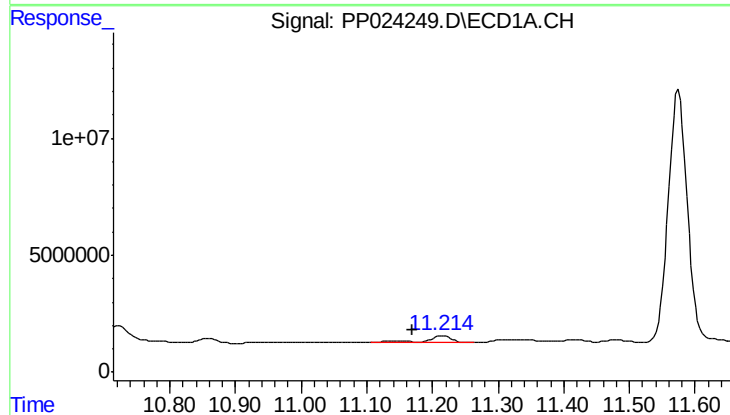


#3 4-Nitrophenol

R.T.: 11.215 min
Delta R.T.: 0.047 min
Response: 7420778
Conc: 17.26 ng/ml

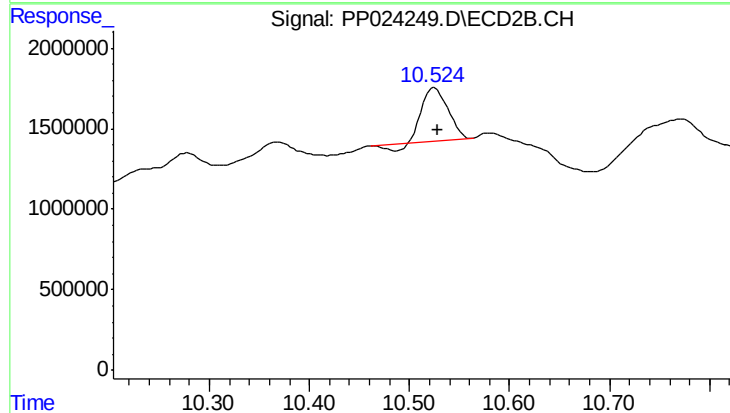

#3 4-Nitrophenol


R.T.: 10.525 min
Delta R.T.: -0.003 min
Response: 5677785
Conc: 12.23 ng/ml

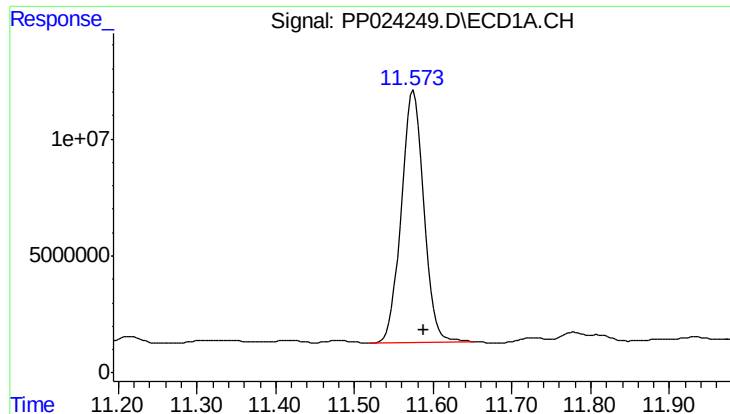

#4 2,4-DCAA


R.T.: 11.575 min
Delta R.T.: -0.014 min
Response: 216777374
Conc: 423.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
SLUDGE

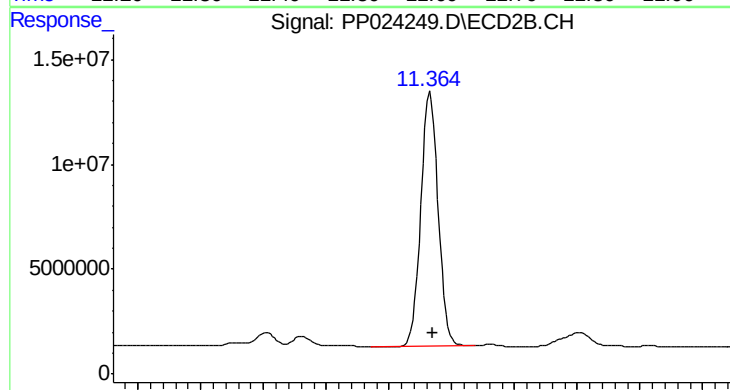


#4 2,4-DCAA

R.T.: 11.366 min
Delta R.T.: -0.003 min
Response: 232769273
Conc: 383.84 ng/ml

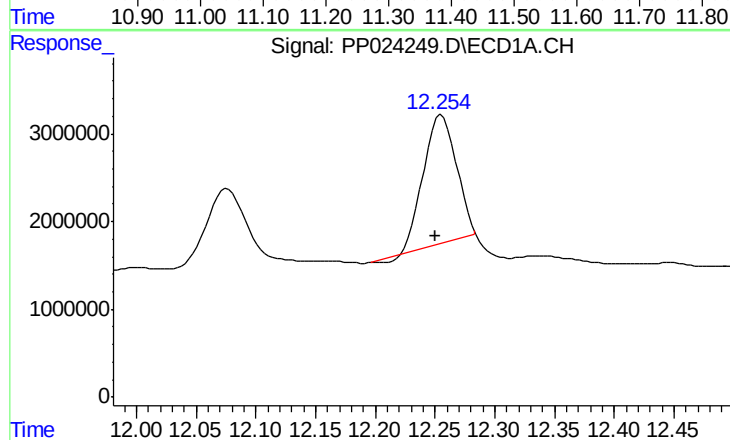


#6 MCP

R.T.: 12.256 min
Delta R.T.: 0.005 min
Response: 28817474
Conc: 19.65 ug/ml

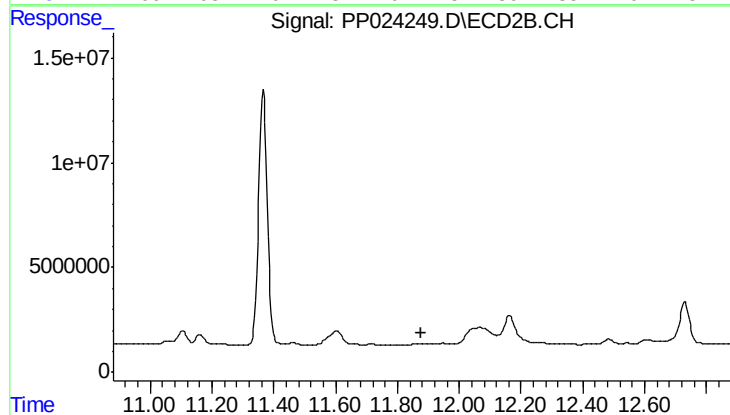

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.878 min
Response: 0
Conc: N.D.

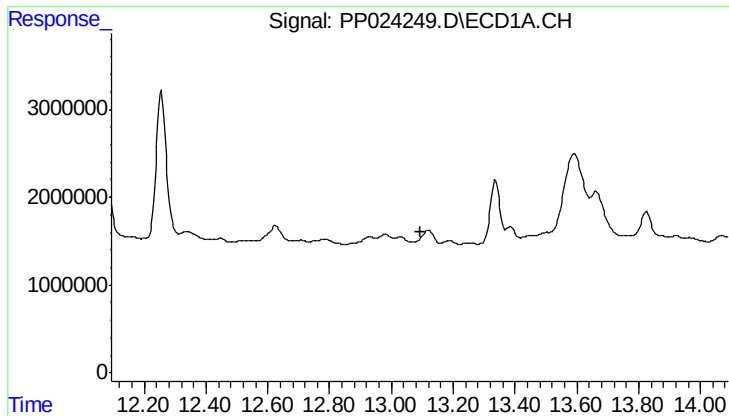

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.092 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SLUDGE

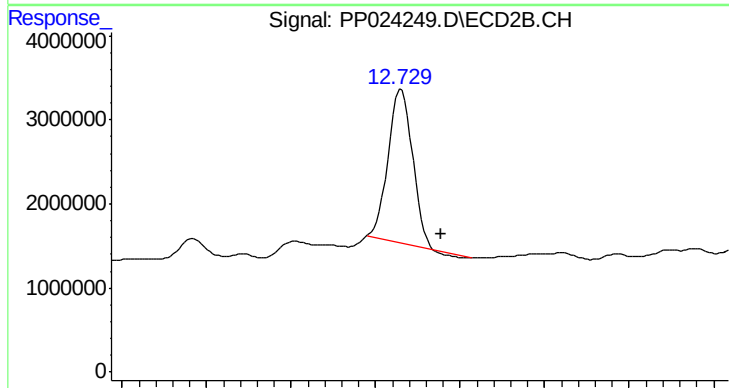


#8 DICHLORPROP

R.T.: 12.730 min
Delta R.T.: -0.047 min
Response: 36933103
Conc: 62.91 ng/ml

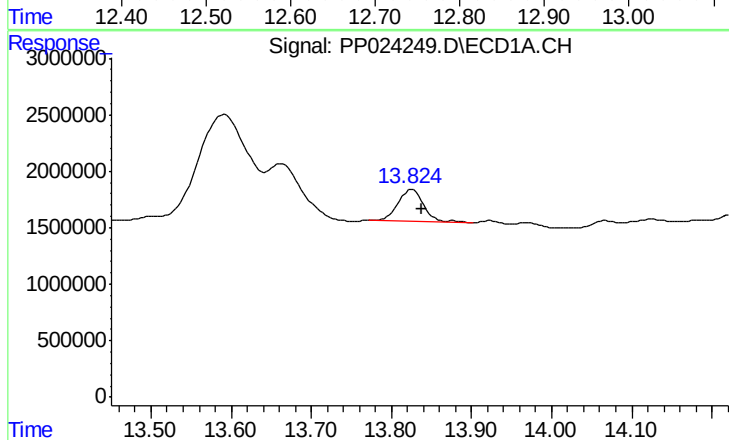


#10 Pentachlorophenol

R.T.: 13.826 min
Delta R.T.: -0.013 min
Response: 6357843
Conc: 0.78 ng/ml

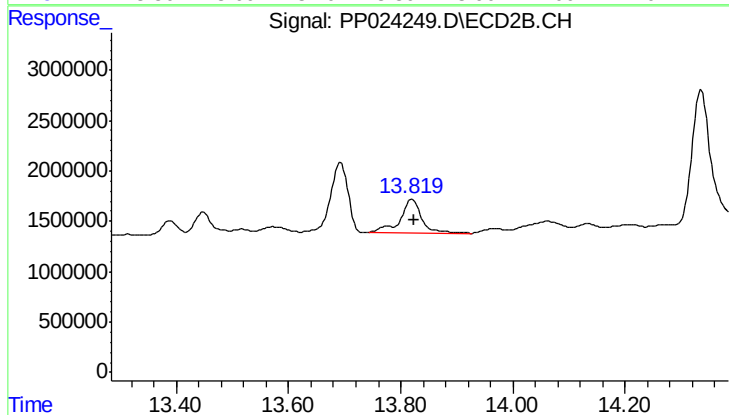

#10 Pentachlorophenol


R.T.: 13.820 min
Delta R.T.: -0.003 min
Response: 8711014
Conc: 1.01 ng/ml

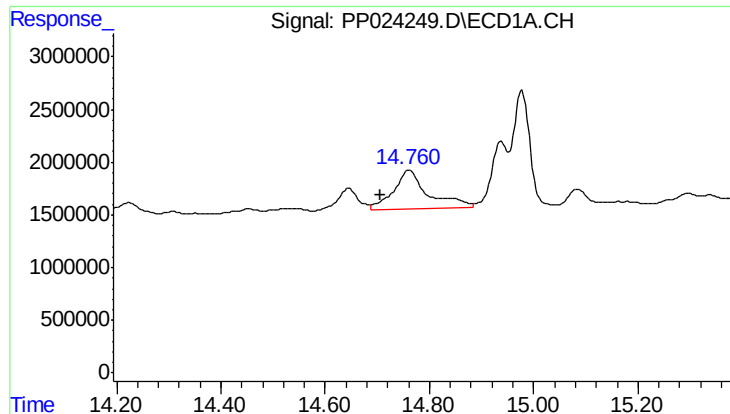

#11 2,4,5-TP (SILVEX)


R.T.: 14.762 min
Delta R.T.: 0.055 min
Response: 16693672
Conc: 5.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
SLUDGE

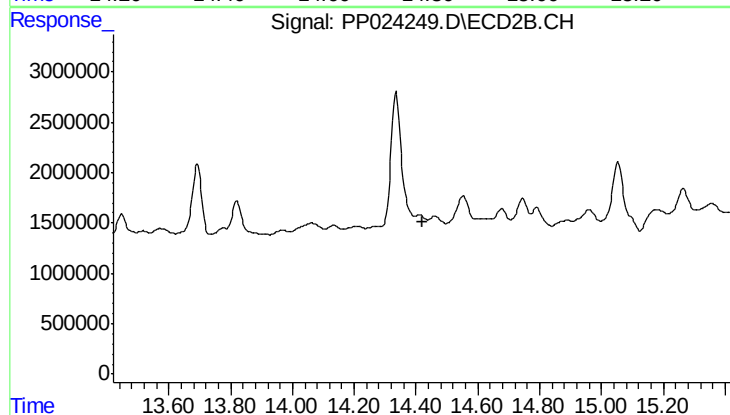


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.421 min
Response: 0
Conc: N.D.

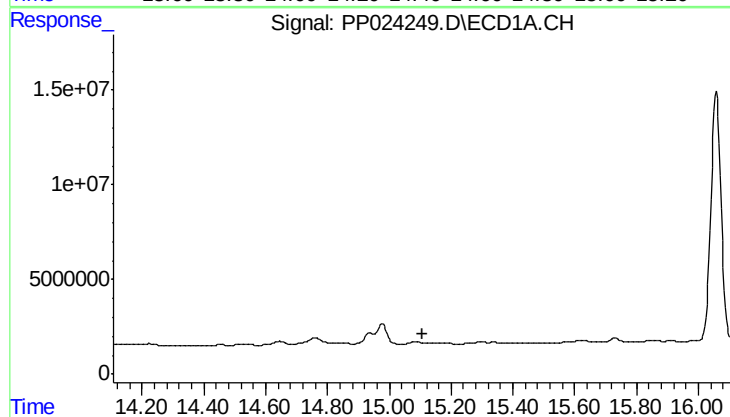


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 15.106 min
Response: 0
Conc: N.D.

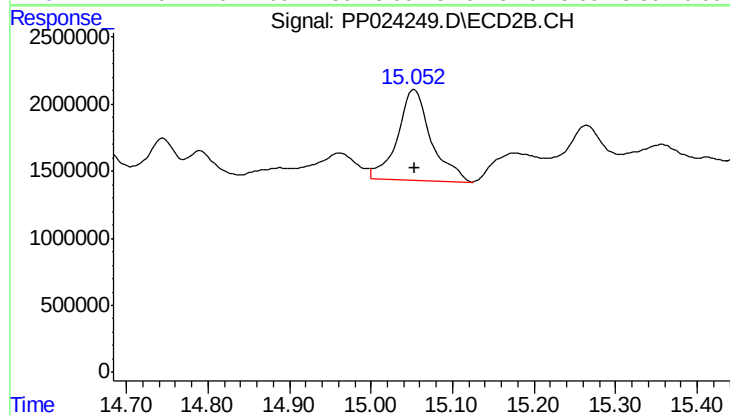

#12 2,4,5-T


R.T.: 15.054 min
Delta R.T.: 0.000 min
Response: 19527404
Conc: 6.34 ng/ml

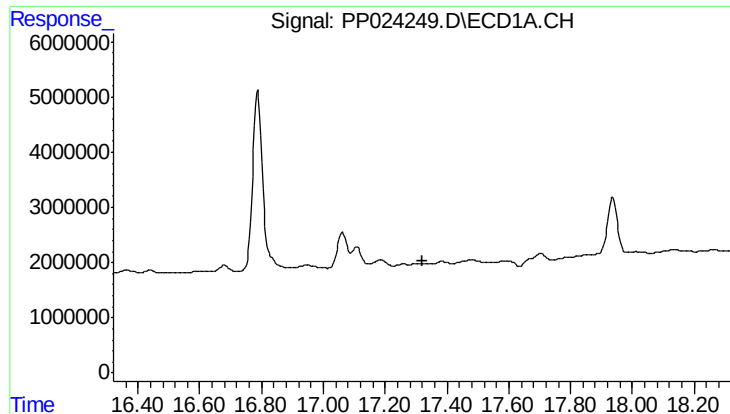

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SLUDGE

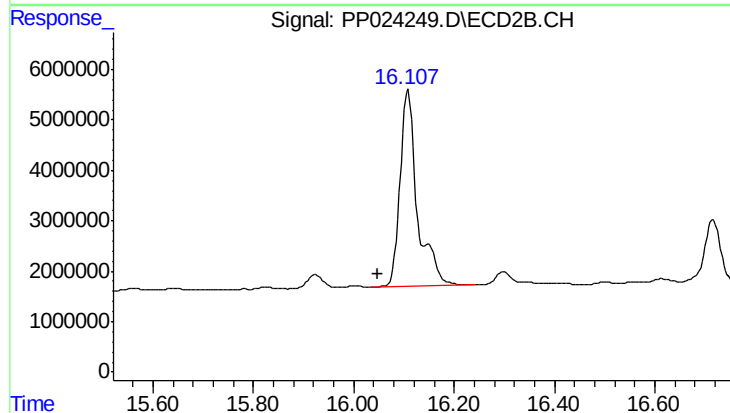


#14 DINOSEB

R.T.: 16.108 min
Delta R.T.: 0.060 min
Response: 93675601
Conc: 38.08 ng/ml

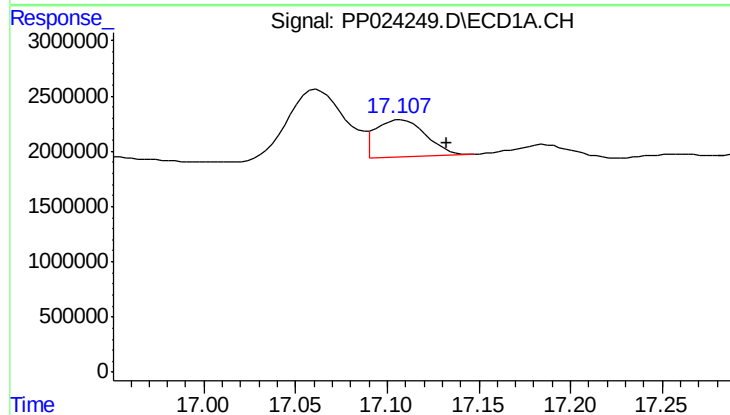


#15 Picloram

R.T.: 17.107 min
Delta R.T.: -0.025 min
Response: 6430159
Conc: 1.32 ng/ml

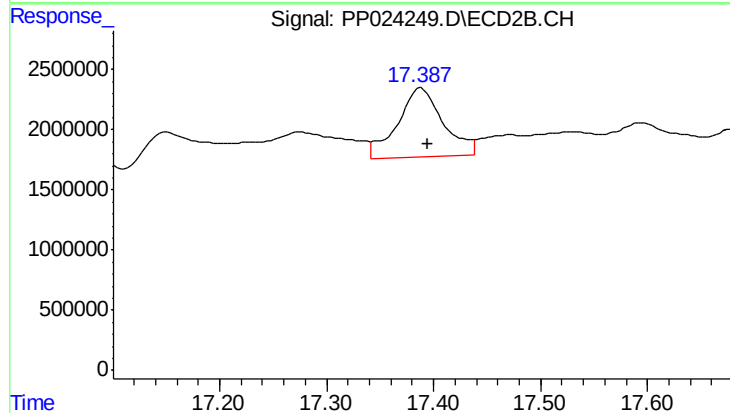

#15 Picloram


R.T.: 17.389 min
Delta R.T.: -0.006 min
Response: 16815422
Conc: 3.38 ng/ml

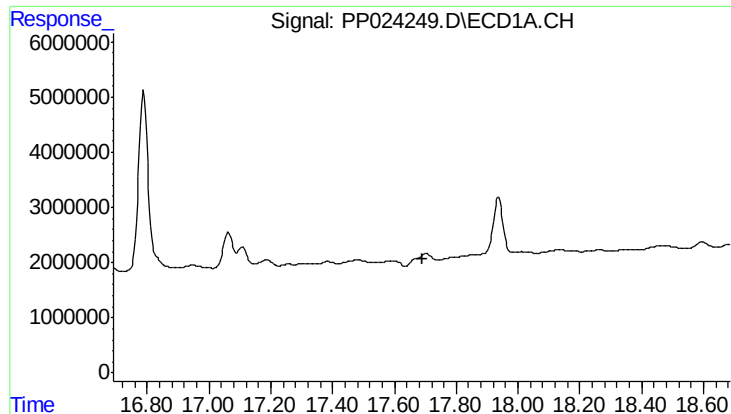

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.689 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SLUDGE

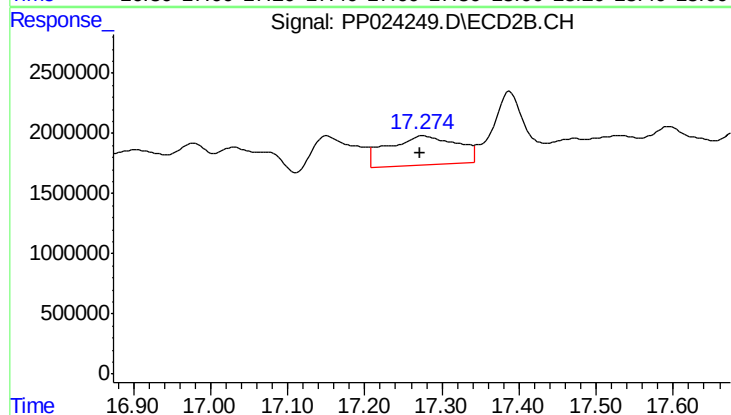

#16 DCPA

R.T.: 17.277 min
Delta R.T.: 0.006 min
Response: 15254225
Conc: 3.51 ng/ml