

Data Path : P:\HPCHEM1\ECD_P\Data\PP030618\
 Data File : PP024250.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Mar 2018 19:03
 Operator : UA/AJ
 Sample : J1792-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 01:34:46 2018
 Quant Method : P:\HPCHEM1\ECD_P\methods\PP020618.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 06 02:07:55 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.574	11.365	214.2E6	229.5E6	417.973	378.402
Target Compounds							
2) T	3,5-DICHL...	0.000	9.460	0	2603540	N.D.	3.121 #
3) T	4-Nitroph...	0.000	10.526	0	10456324	N.D.	22.530 #
6) T	MCP	12.255	0.000	26319098	0	17.951	N.D. #
8) T	DICHLORPROP	0.000	12.730	0	32245395	N.D.	54.923 #
10) T	Pentachlo...	0.000	13.822	0	5851994	N.D.	0.680 #
11) T	2,4,5-TP ...	14.759	0.000	9836794	0	2.970	N.D. #
12) T	2,4,5-T	0.000	15.055	0	16610721	N.D.	5.392 #
14) T	DINOSEB	0.000	16.108	0	90566198	N.D.	36.817 #
15) T	Picloram	0.000	17.389	0	5468159	N.D.	1.098 #
16) T	DCPA	17.705	17.322	1606975	899098	0.410	0.207 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_P\Data\PP030618\
Data File : PP024250.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Mar 2018 19:03
Operator : UA/AJ
Sample : J1792-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
TP-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 01:34:46 2018
Quant Method : P:\HPCHEM1\ECD_P\methods\PP020618.M
Quant Title : 8080.M
QLast Update : Tue Feb 06 02:07:55 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

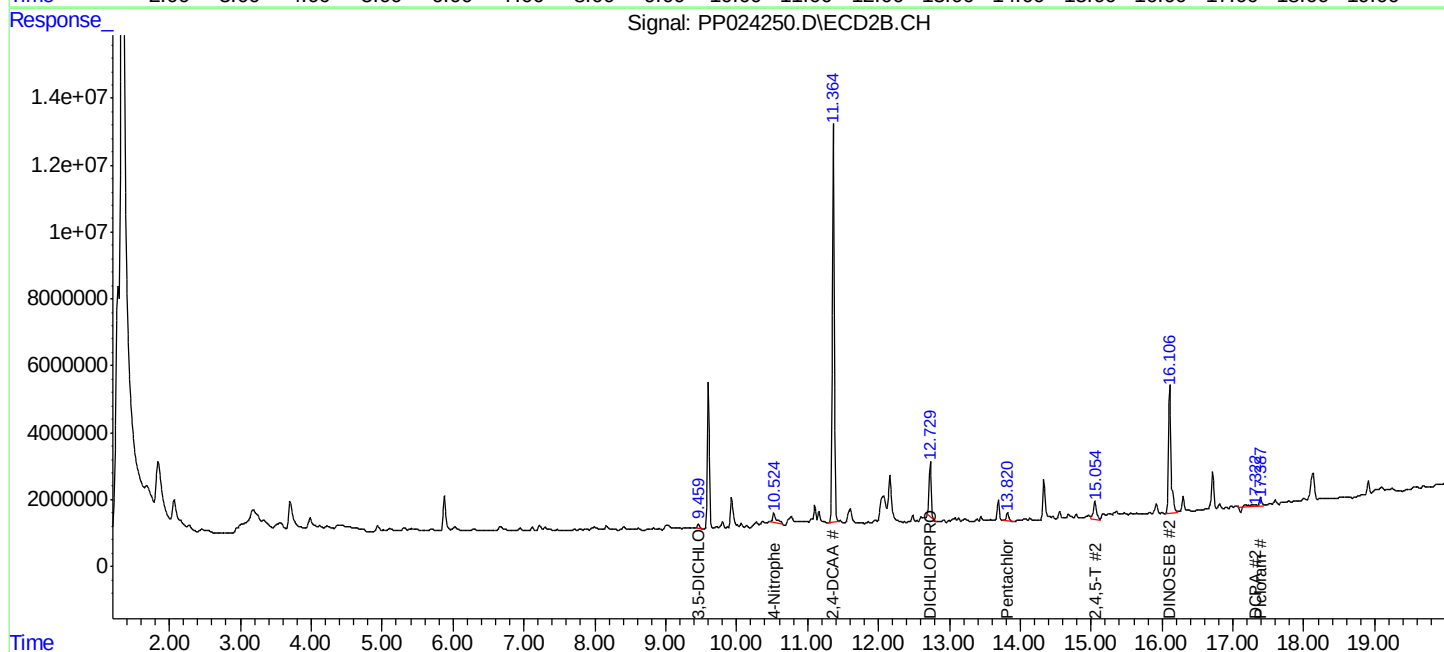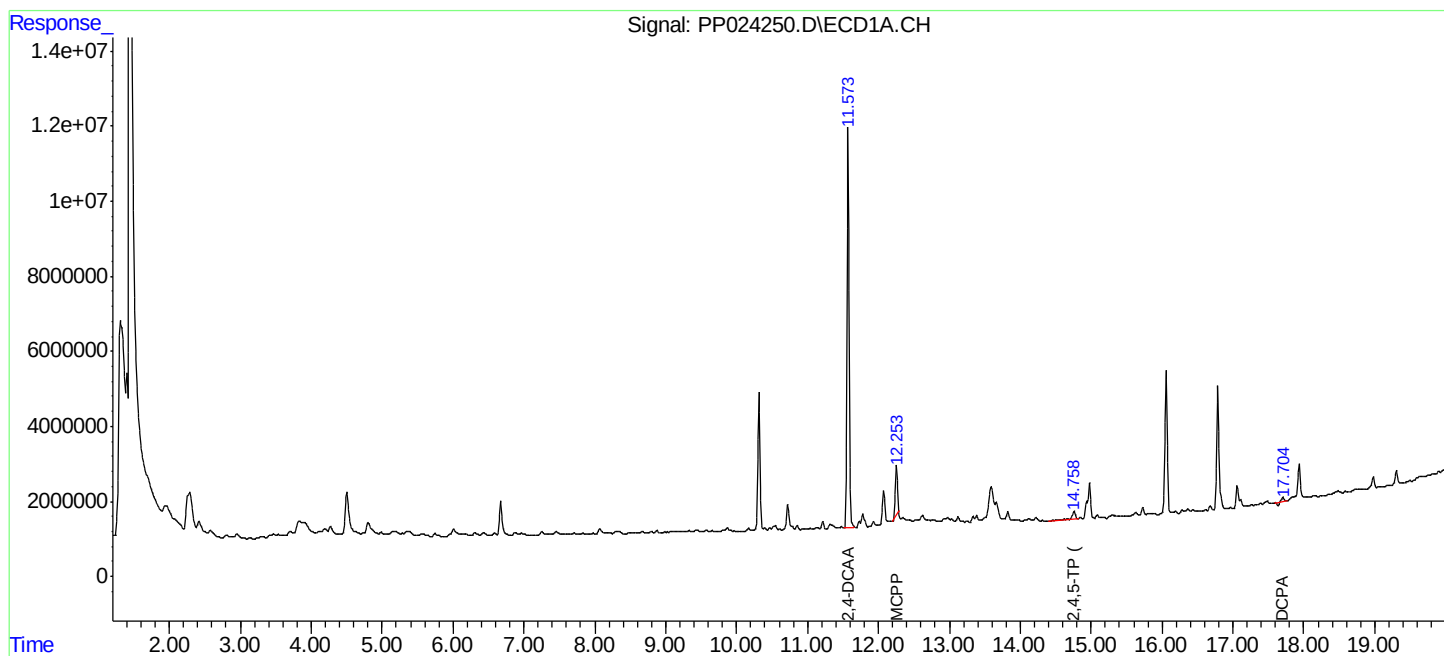


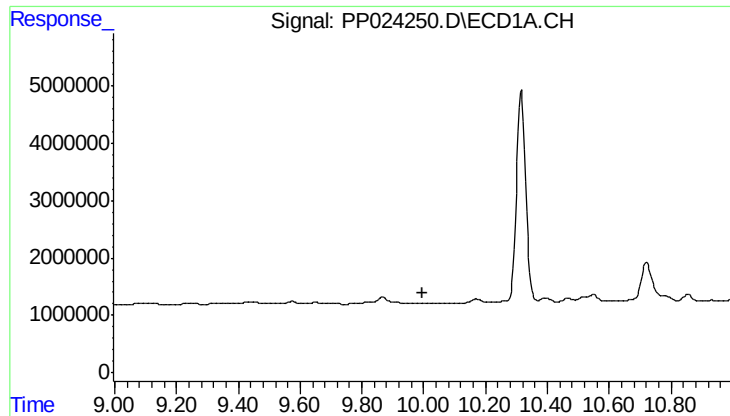

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.994 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-6

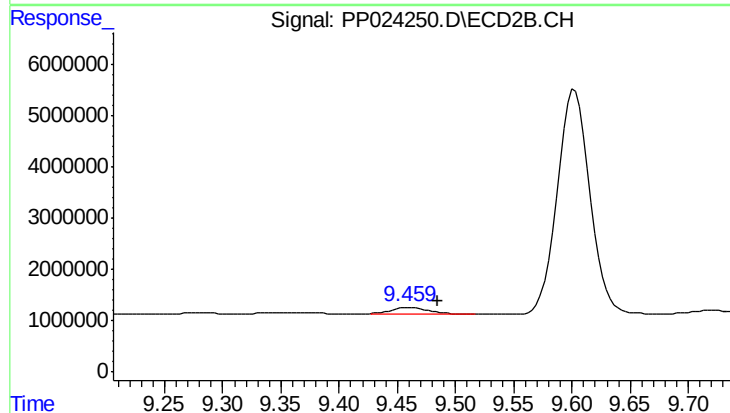


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.460 min
Delta R.T.: -0.024 min
Response: 2603540
Conc: 3.12 ng/ml

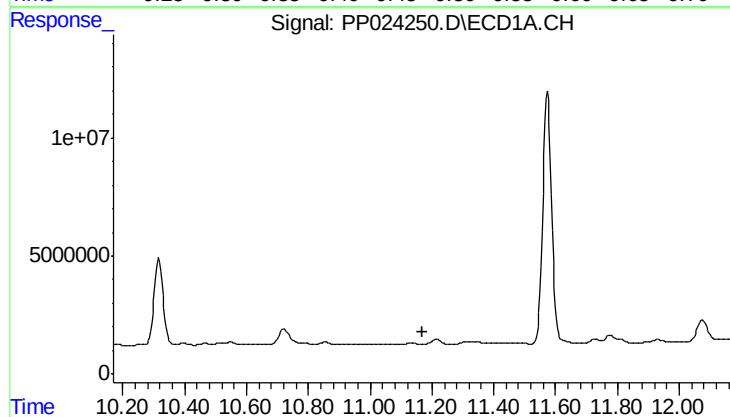


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 11.169 min
Response: 0
Conc: N.D.

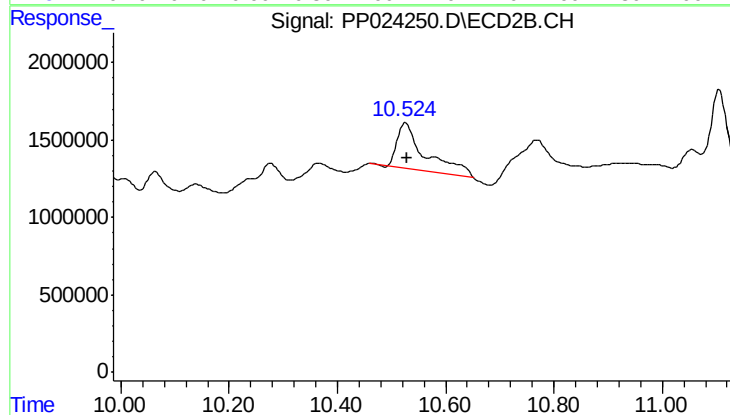

#3 4-Nitrophenol


R.T.: 10.526 min
Delta R.T.: -0.002 min
Response: 10456324
Conc: 22.53 ng/ml

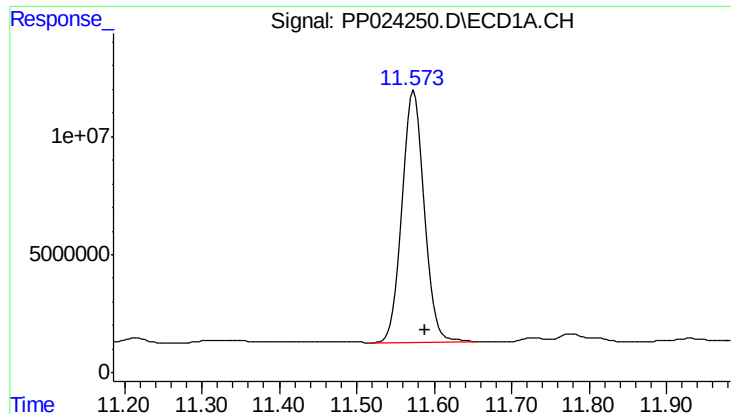

#4 2,4-DCAA


R.T.: 11.574 min
Delta R.T.: -0.015 min
Response: 214198967
Conc: 417.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-6

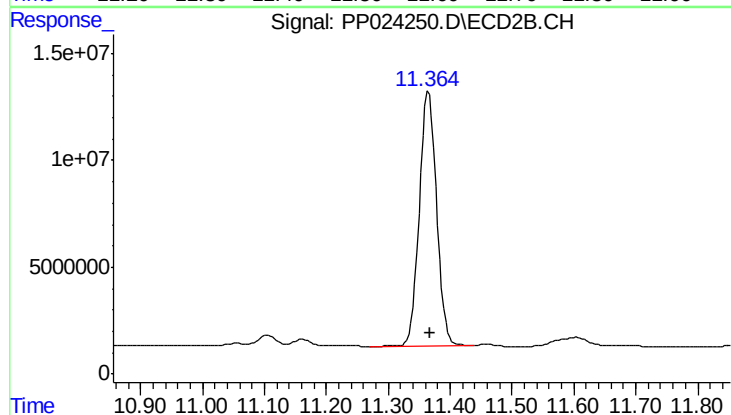


#4 2,4-DCAA

R.T.: 11.365 min
Delta R.T.: -0.004 min
Response: 229469541
Conc: 378.40 ng/ml

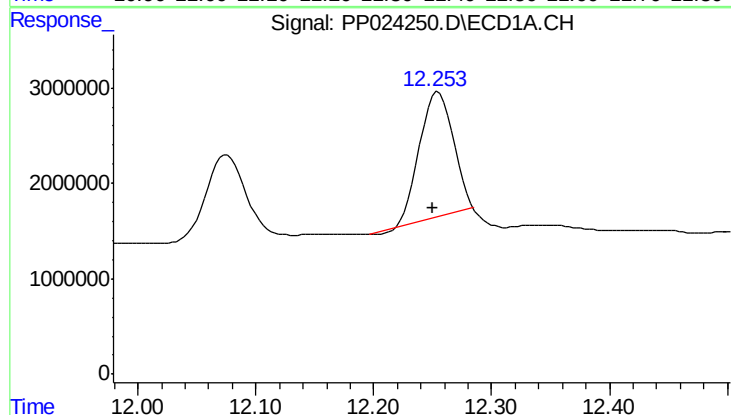


#6 MCP

R.T.: 12.255 min
Delta R.T.: 0.004 min
Response: 26319098
Conc: 17.95 ug/ml

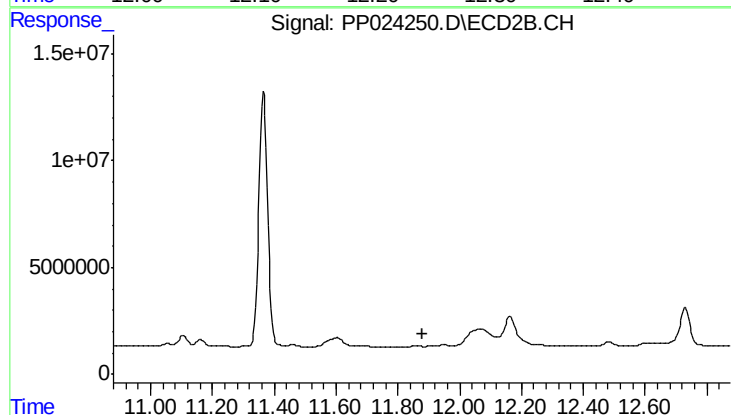

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.878 min
Response: 0
Conc: N.D.

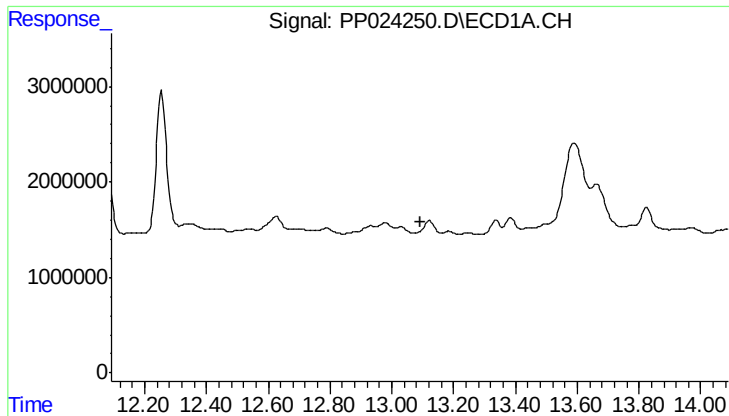

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.092 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-6

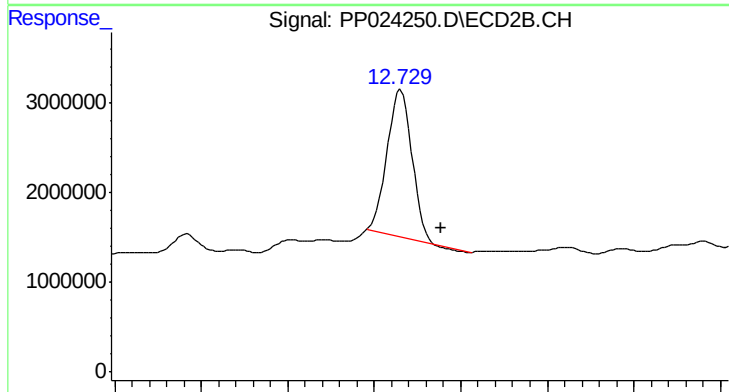


#8 DICHLORPROP

R.T.: 12.730 min
Delta R.T.: -0.047 min
Response: 32245395
Conc: 54.92 ng/ml

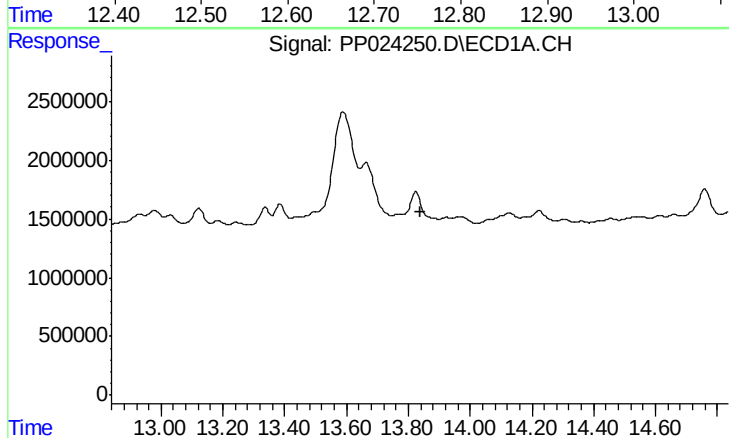


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 13.838 min
Response: 0
Conc: N.D.

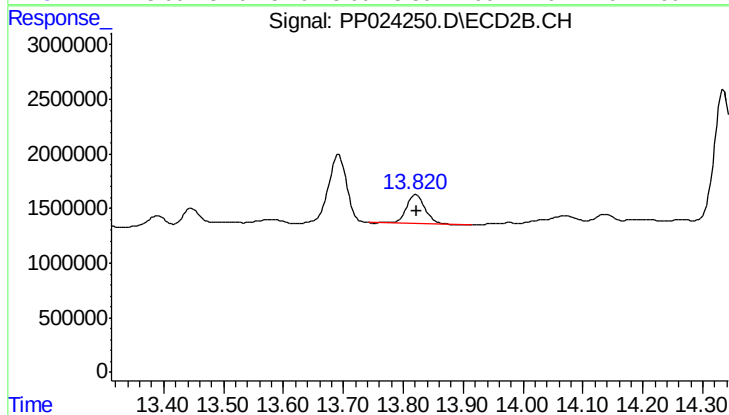

#10 Pentachlorophenol


R.T.: 13.822 min
Delta R.T.: -0.001 min
Response: 5851994
Conc: 0.68 ng/ml

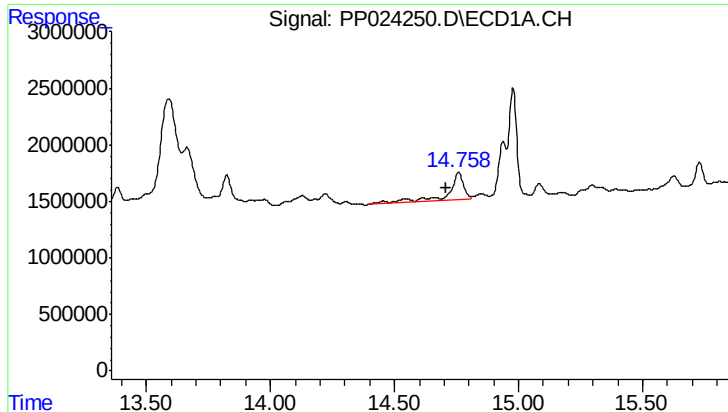

#11 2,4,5-TP (SILVEX)


R.T.: 14.759 min
Delta R.T.: 0.053 min
Response: 9836794
Conc: 2.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-6

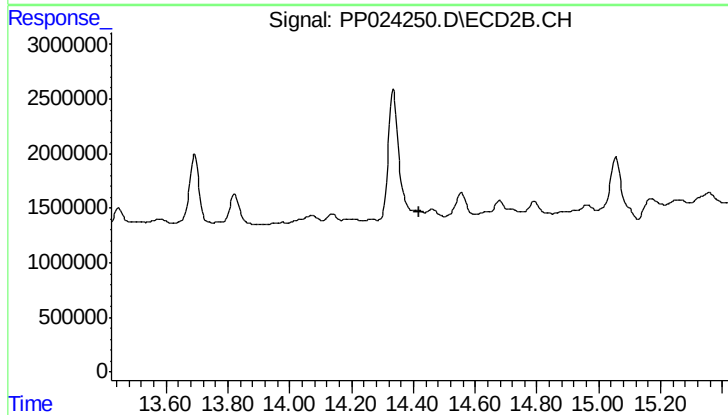


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.421 min
Response: 0
Conc: N.D.

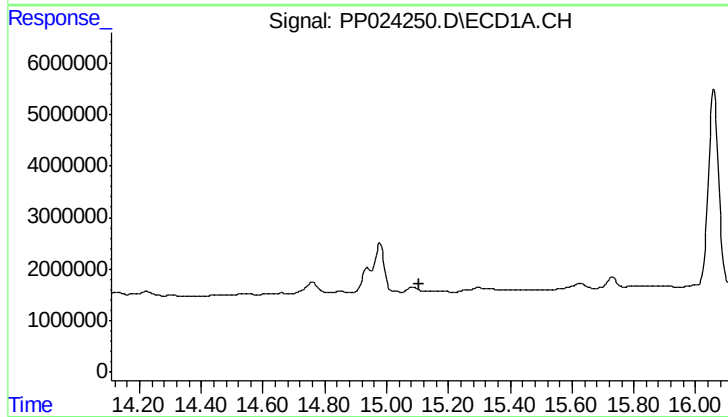


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 15.106 min
Response: 0
Conc: N.D.

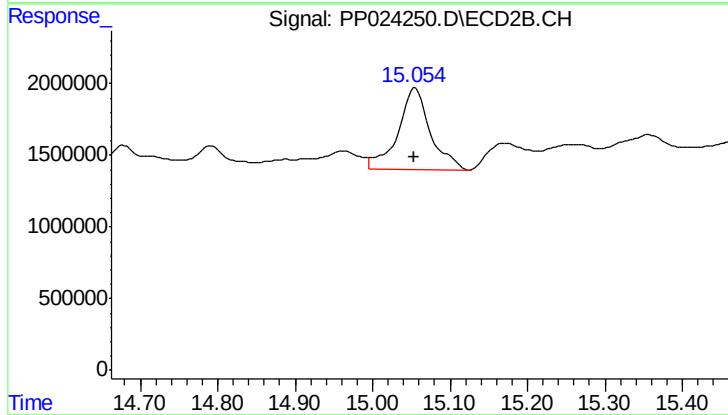

#12 2,4,5-T


R.T.: 15.055 min
Delta R.T.: 0.002 min
Response: 16610721
Conc: 5.39 ng/ml

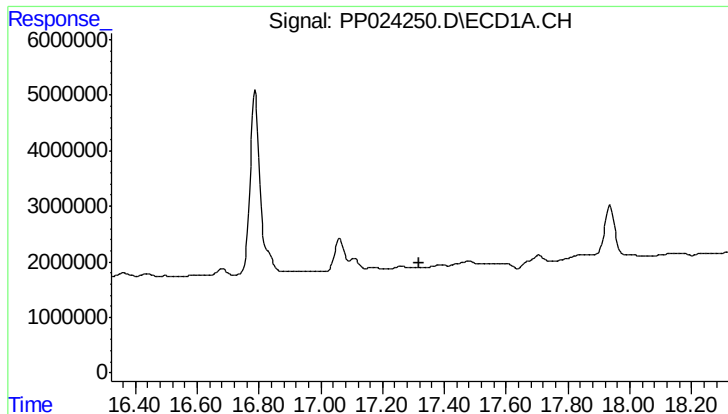

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-6

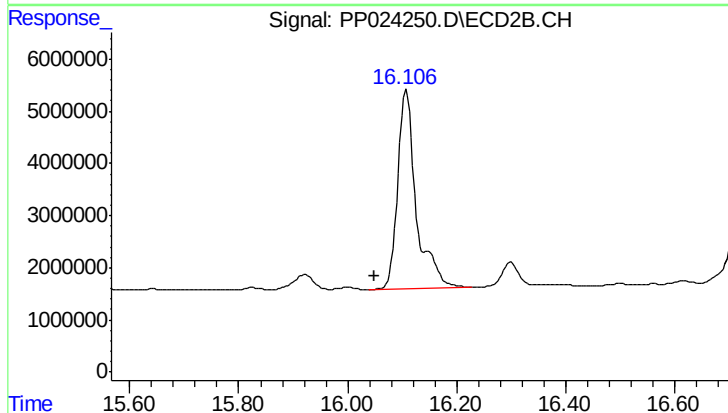


#14 DINOSEB

R.T.: 16.108 min
Delta R.T.: 0.059 min
Response: 90566198
Conc: 36.82 ng/ml

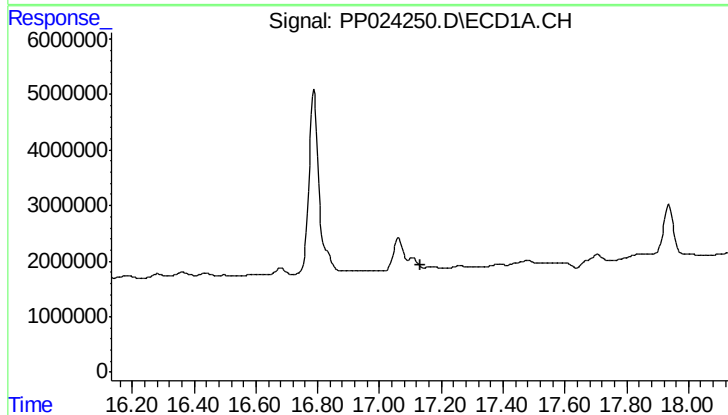


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 17.132 min
Response: 0
Conc: N.D.

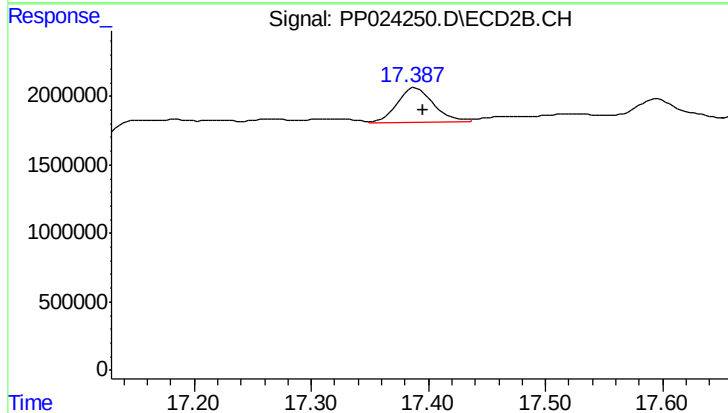

#15 Picloram


R.T.: 17.389 min
Delta R.T.: -0.006 min
Response: 5468159
Conc: 1.10 ng/ml

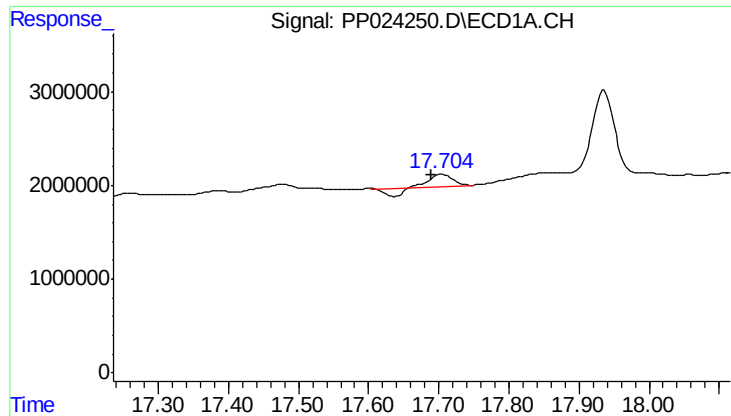

#16 DCPA

R.T.: 17.705 min
Delta R.T.: 0.016 min
Response: 1606975
Conc: 0.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-6

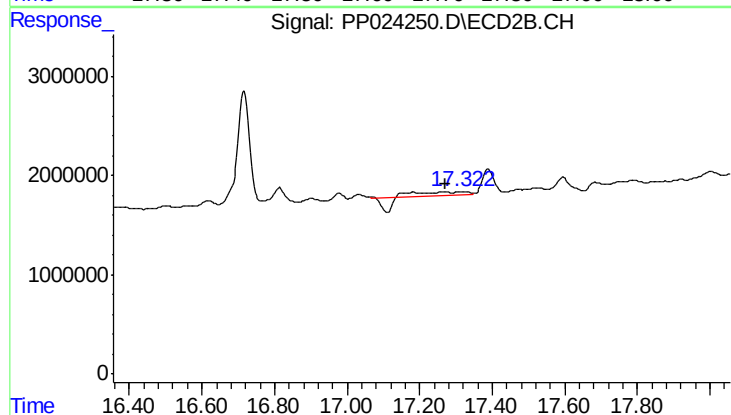

#16 DCPA

R.T.: 17.322 min
Delta R.T.: 0.051 min
Response: 899098
Conc: 0.21 ng/ml