

Data Path : P:\HPCHEM1\ECD_P\Data\PP030618\
 Data File : PP024254.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Mar 2018 20:41
 Operator : UA/AJ
 Sample : J1792-10
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-13

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 01:35:57 2018
 Quant Method : P:\HPCHEM1\ECD_P\methods\PP020618.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 06 02:07:55 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.574	11.365	222.2E6	237.9E6	433.510	392.349
Target Compounds							
2) T	3,5-DICHL...	0.000	9.460	0	2266067	N.D.	2.717 #
3) T	4-Nitroph...	0.000	10.525	0	10721333	N.D.	23.101 #
6) T	MCP	12.255	0.000	24129892	0	16.458	N.D. #
8) T	DICHLORPROP	0.000	12.730	0	29899663	N.D.	50.928 #
10) T	Pentachlo...	13.825	13.821	5149006	6869853	0.633	0.798 #
12) T	2,4,5-T	0.000	15.056	0	20576321	N.D.	6.679 #
14) T	DINOSEB	0.000	16.108	0	83358604	N.D.	33.887 #
15) T	Picloram	0.000	17.391	0	3923758	N.D.	0.788 #
16) T	DCPA	17.706	0.000	1144266	0	0.292	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_P\Data\PP030618\
Data File : PP024254.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Mar 2018 20:41
Operator : UA/AJ
Sample : J1792-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
TP-13

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 01:35:57 2018
Quant Method : P:\HPCHEM1\ECD_P\methods\PP020618.M
Quant Title : 8080.M
QLast Update : Tue Feb 06 02:07:55 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

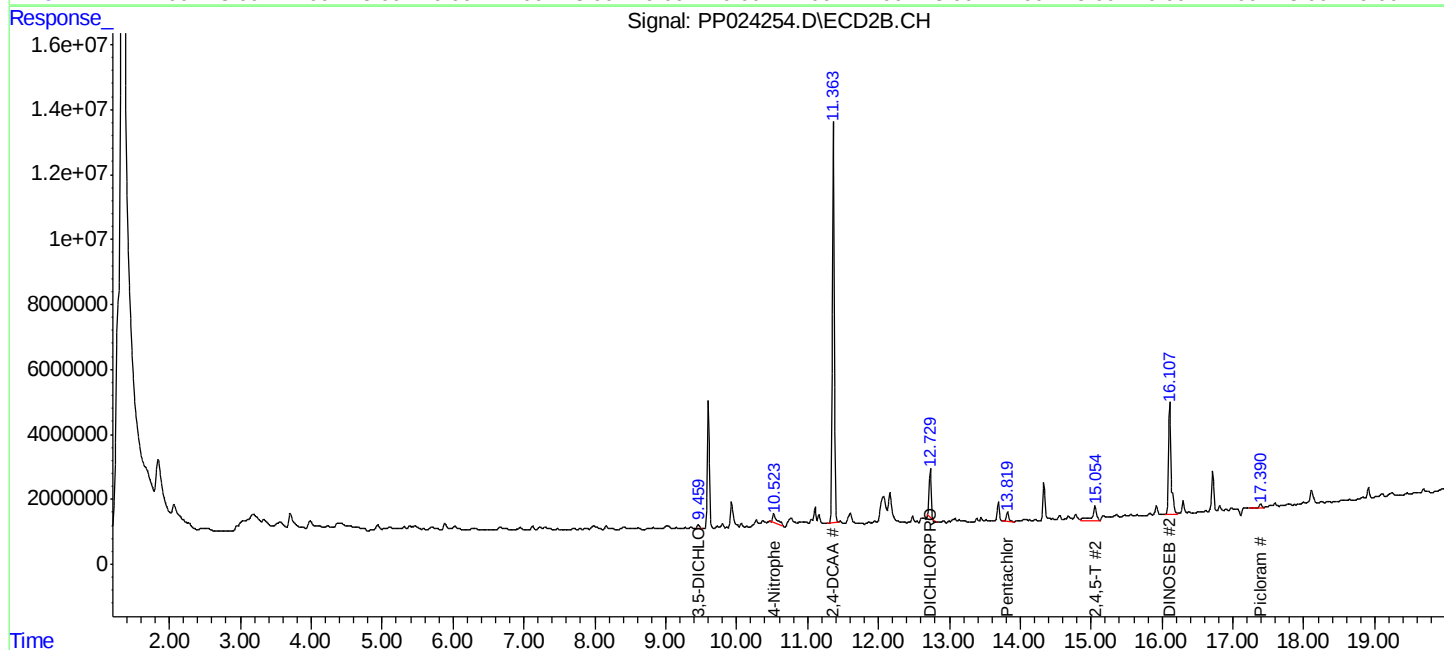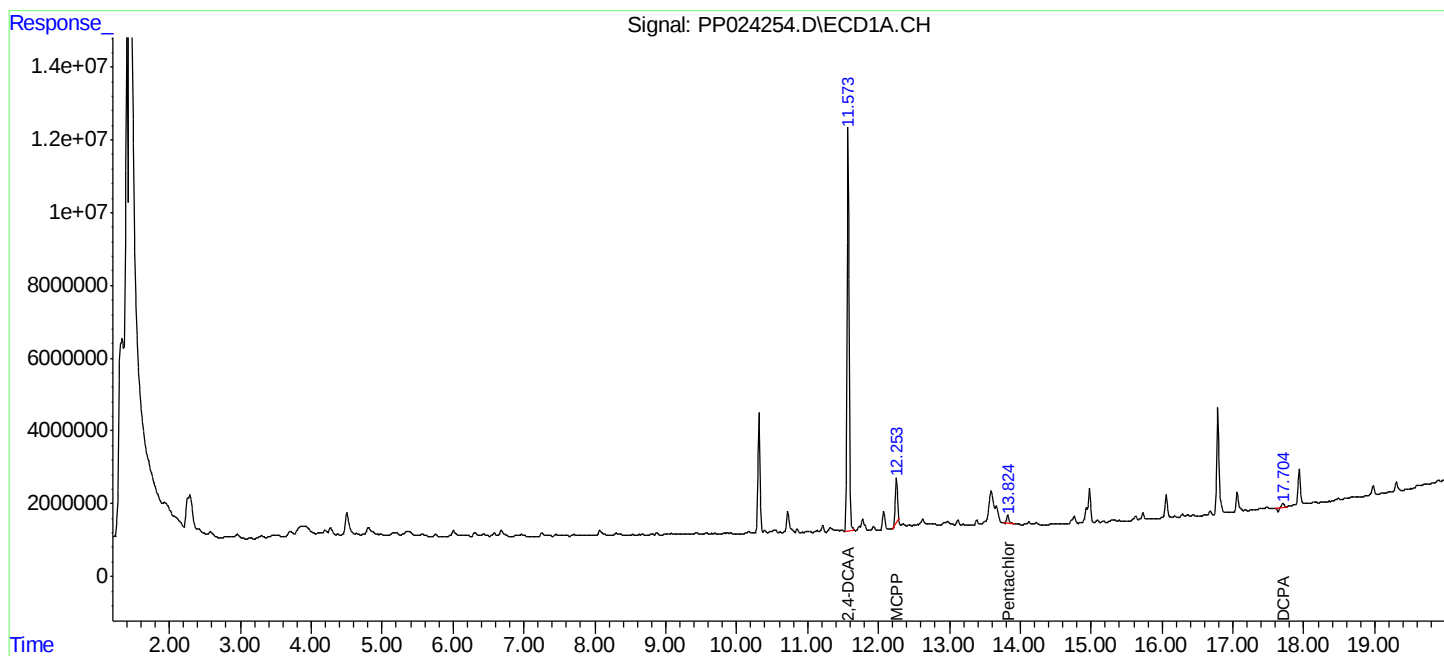


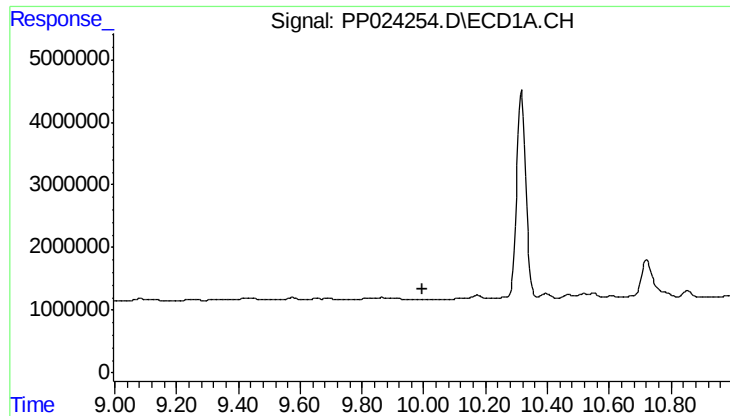

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.994 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-13

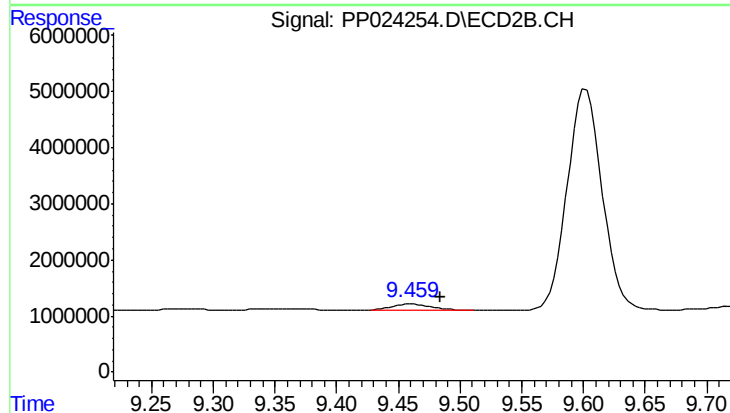


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.460 min
Delta R.T.: -0.024 min
Response: 2266067
Conc: 2.72 ng/ml

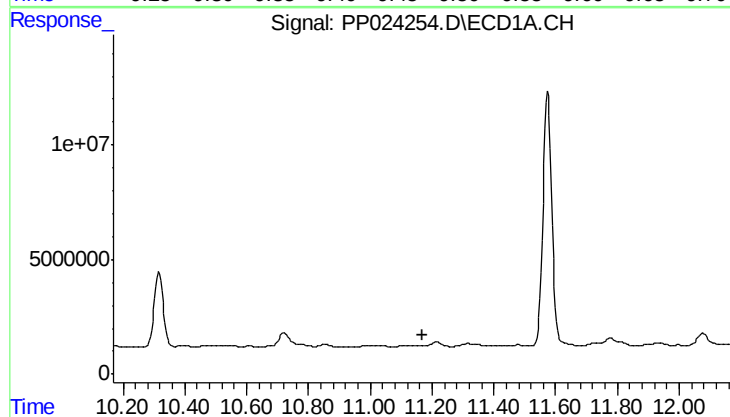


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 11.169 min
Response: 0
Conc: N.D.

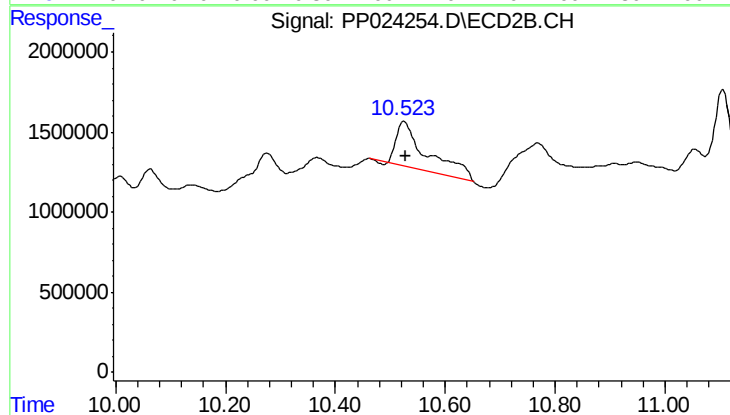

#3 4-Nitrophenol


R.T.: 10.525 min
Delta R.T.: -0.003 min
Response: 10721333
Conc: 23.10 ng/ml

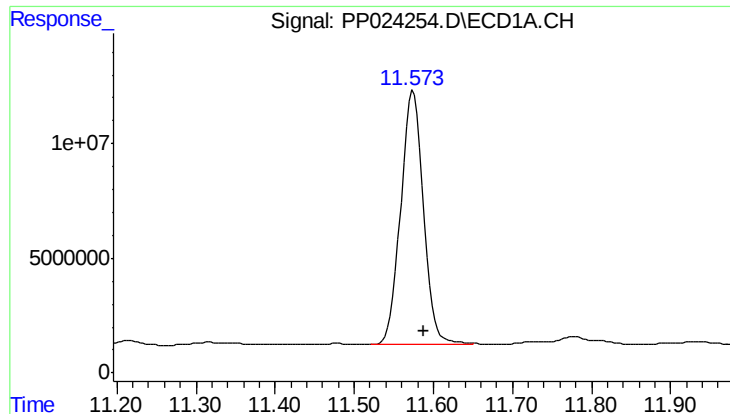

#4 2,4-DCAA


R.T.: 11.574 min
Delta R.T.: -0.014 min
Response: 222161185
Conc: 433.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-13

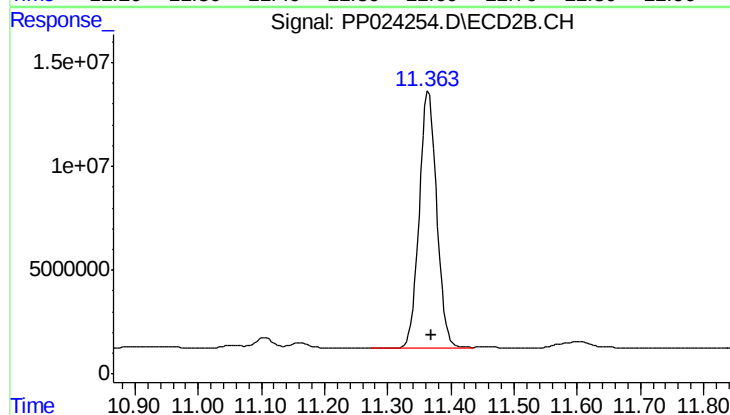


#4 2,4-DCAA

R.T.: 11.365 min
Delta R.T.: -0.004 min
Response: 237927304
Conc: 392.35 ng/ml

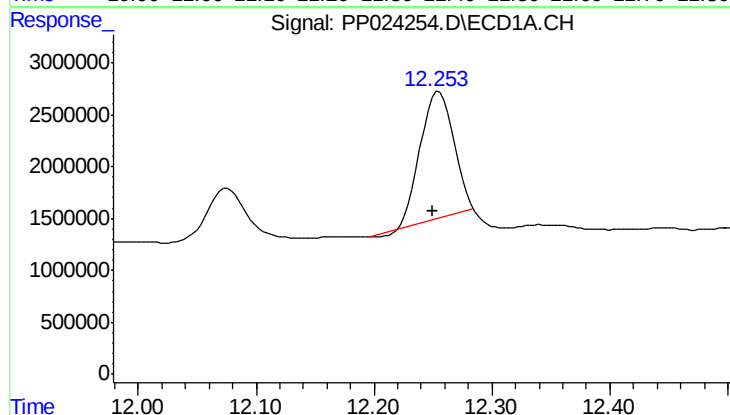


#6 MCP

R.T.: 12.255 min
Delta R.T.: 0.005 min
Response: 24129892
Conc: 16.46 ug/ml

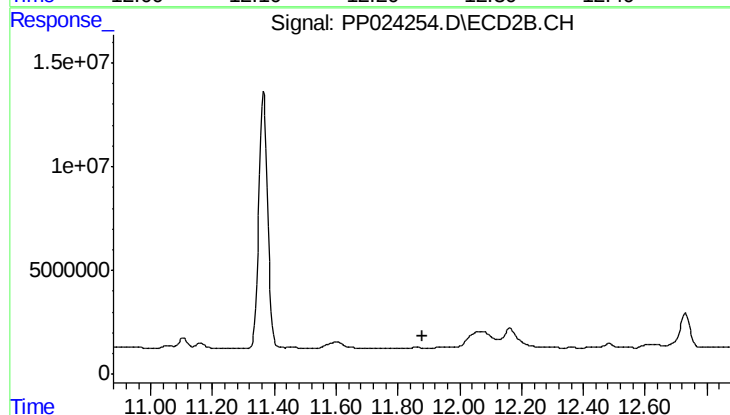

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.878 min
Response: 0
Conc: N.D.

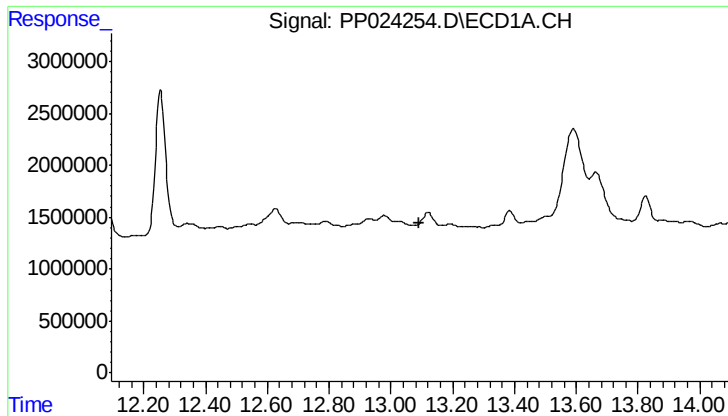

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.092 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-13

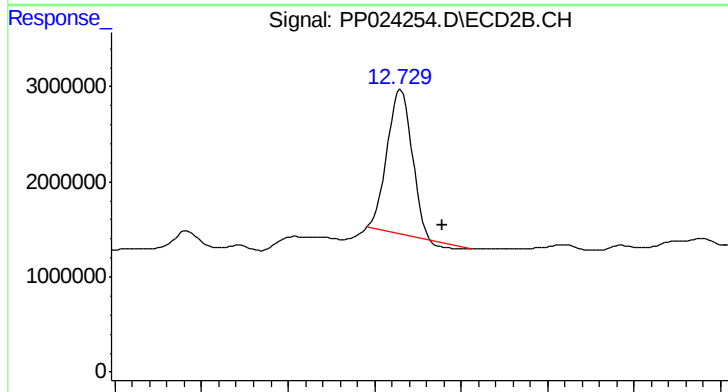


#8 DICHLORPROP

R.T.: 12.730 min
Delta R.T.: -0.048 min
Response: 29899663
Conc: 50.93 ng/ml

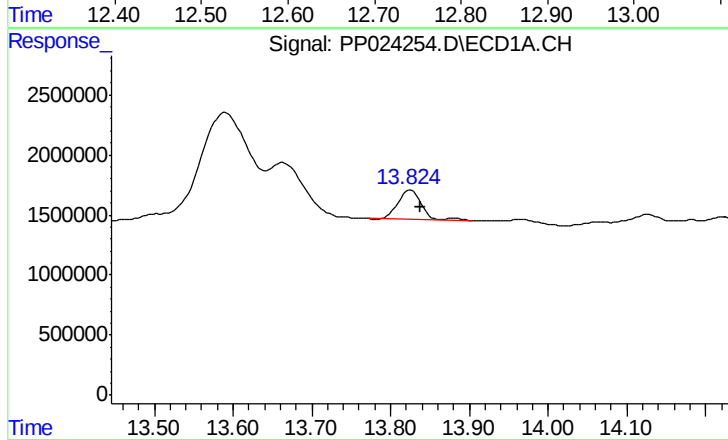


#10 Pentachlorophenol

R.T.: 13.825 min
Delta R.T.: -0.013 min
Response: 5149006
Conc: 0.63 ng/ml

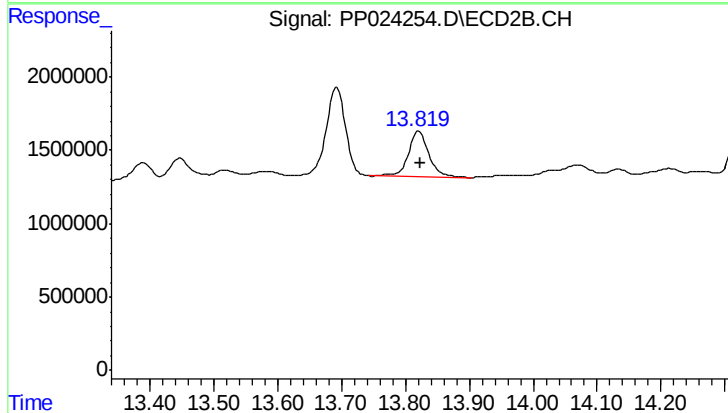

#10 Pentachlorophenol


R.T.: 13.821 min
Delta R.T.: -0.002 min
Response: 6869853
Conc: 0.80 ng/ml

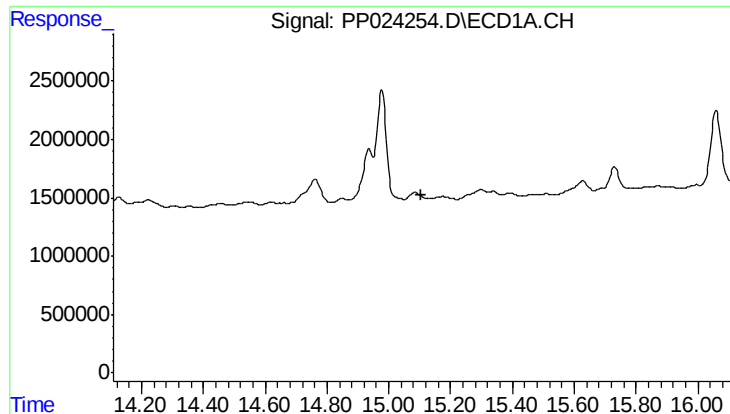

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.106 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-13

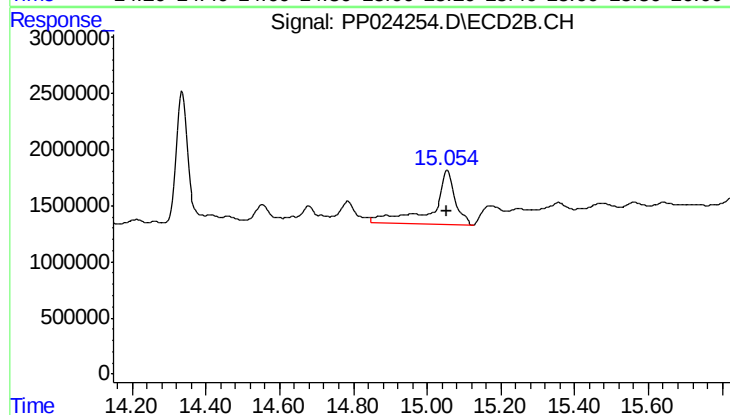


#12 2,4,5-T

R.T.: 15.056 min
Delta R.T.: 0.002 min
Response: 20576321
Conc: 6.68 ng/ml

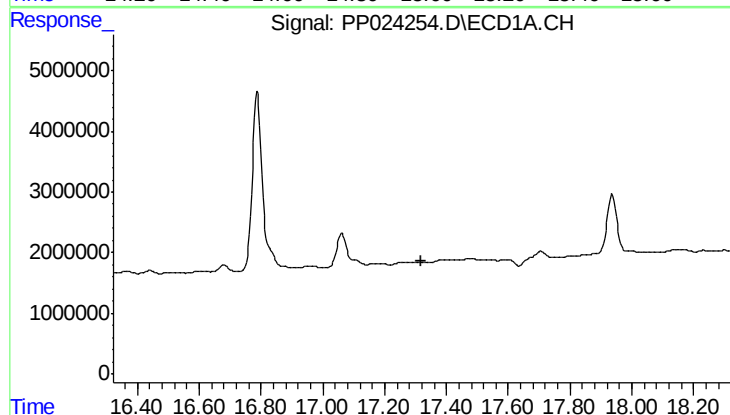


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 17.319 min
Response: 0
Conc: N.D.

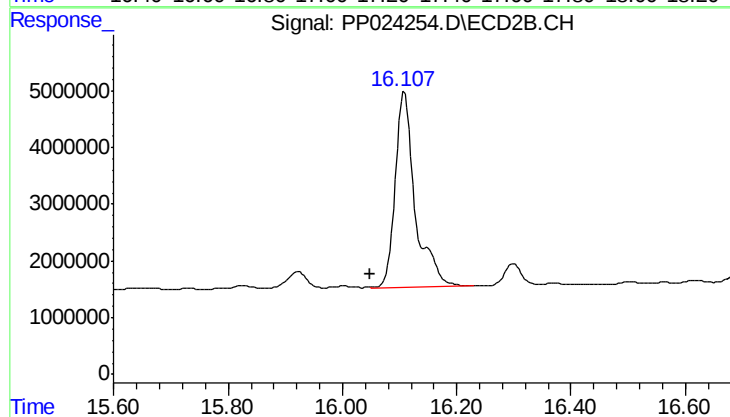

#14 DINOSEB


R.T.: 16.108 min
Delta R.T.: 0.060 min
Response: 83358604
Conc: 33.89 ng/ml

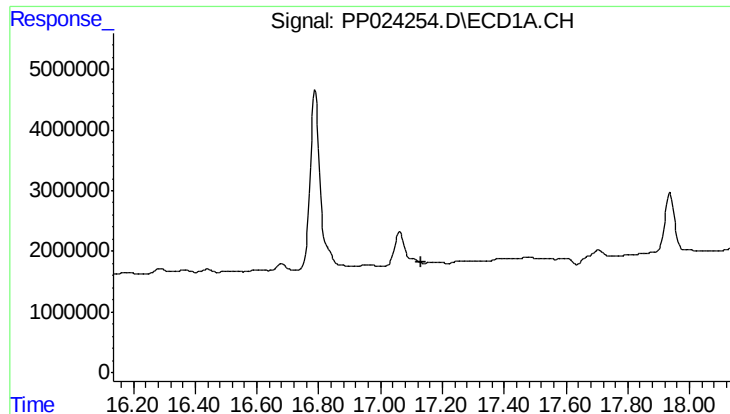

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 17.132 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-13

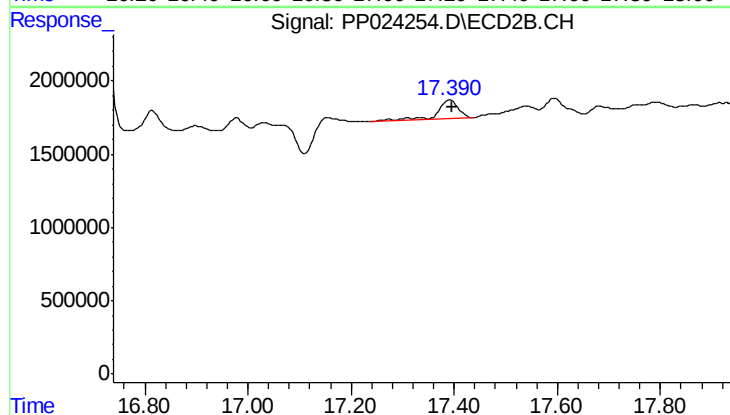


#15 Picloram

R.T.: 17.391 min
Delta R.T.: -0.004 min
Response: 3923758
Conc: 0.79 ng/ml

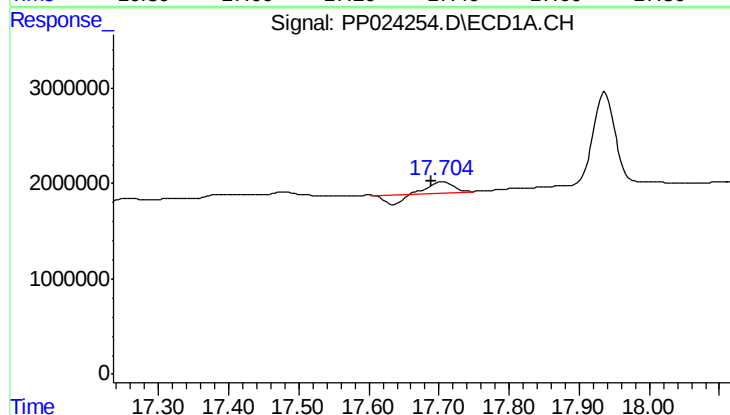

#16 DCPA

R.T.: 17.706 min
Delta R.T.: 0.017 min
Response: 1144266
Conc: 0.29 ng/ml

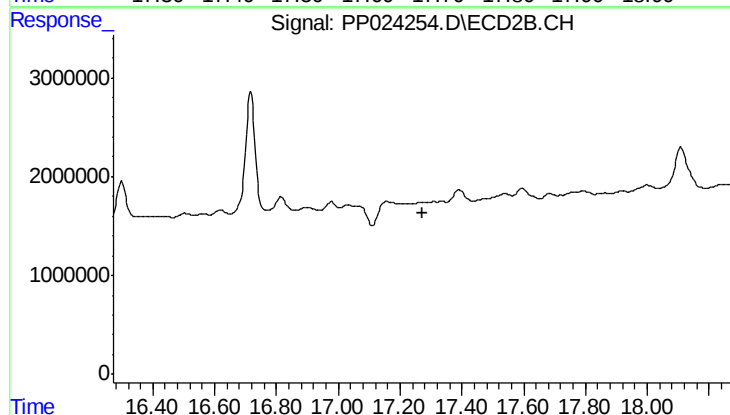

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.271 min
Response: 0
Conc: N.D.