

Data Path : P:\HPCHEM1\ECD_P\Data\PP030618\
 Data File : PP024255.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Mar 2018 21:05
 Operator : UA/AJ
 Sample : J1699-64
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 B21

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 01:36:13 2018
 Quant Method : P:\HPCHEM1\ECD_P\methods\PP020618.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 06 02:07:55 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.575	11.366	191.0E6	205.0E6	372.798	338.076
Target Compounds							
2) T	3,5-DICHL...	0.000	9.464	0	3601986	N.D.	4.319 #
3) T	4-Nitroph...	0.000	10.527	0	9473002	N.D.	20.412 #
6) T	MCP	12.256	0.000	25739358	0	17.555	N.D. #
8) T	DICHLORPROP	0.000	12.731	0	32310763	N.D.	55.035 #
10) T	Pentachlo...	13.826	13.821	6228637	8809689	0.766	1.023 #
11) T	2,4,5-TP ...	14.764	0.000	8315470	0	2.510	N.D. #
12) T	2,4,5-T	0.000	15.056	0	14350719	N.D.	4.658 #
14) T	DINOSEB	0.000	16.109	0	79327060	N.D.	32.248 #
15) T	Picloram	17.063	17.390	14364573	5905399	2.950	1.186 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_P\Data\PP030618\
Data File : PP024255.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Mar 2018 21:05
Operator : UA/AJ
Sample : J1699-64
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
B21

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 01:36:13 2018
Quant Method : P:\HPCHEM1\ECD_P\methods\PP020618.M
Quant Title : 8080.M
QLast Update : Tue Feb 06 02:07:55 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

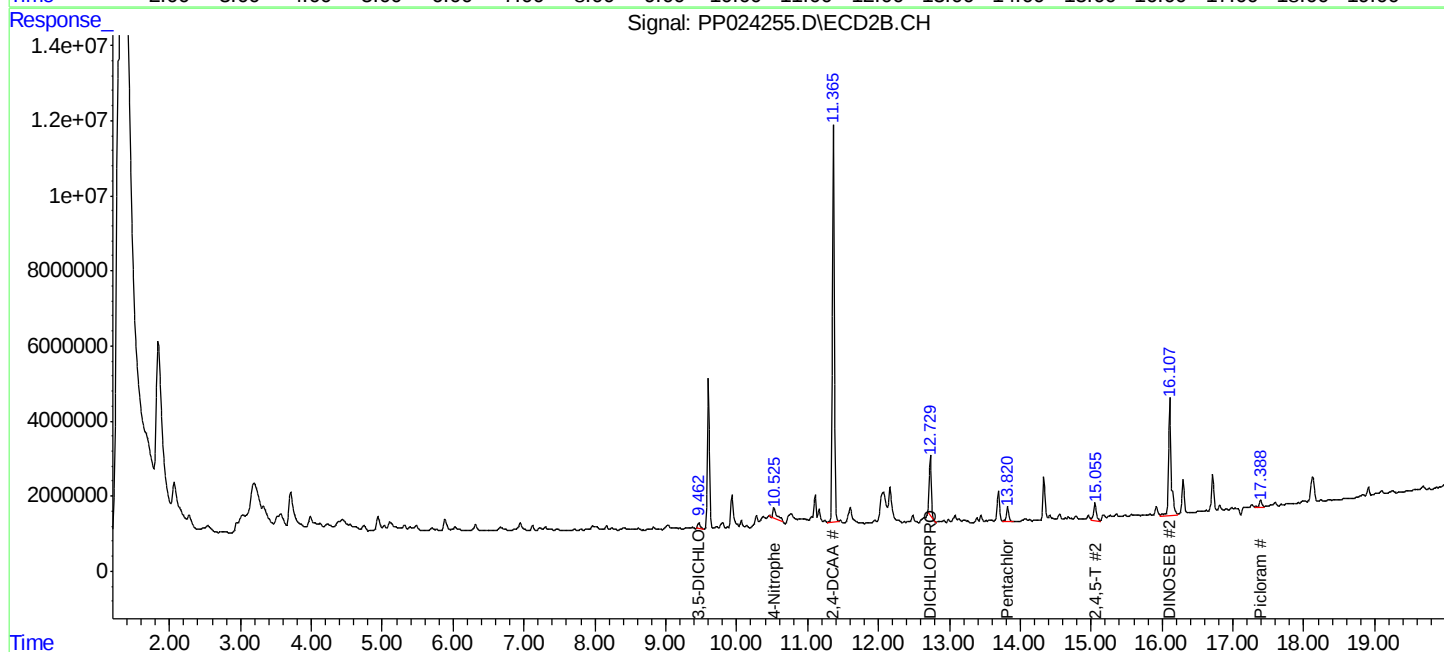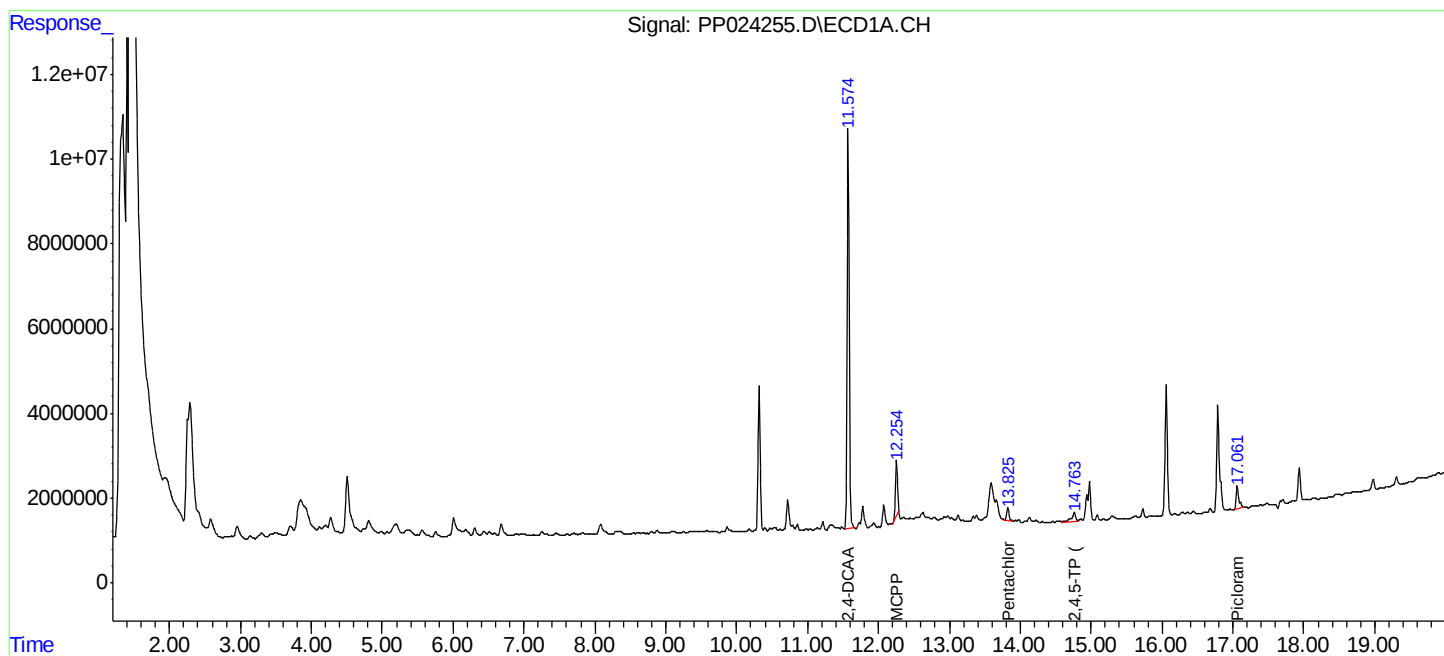


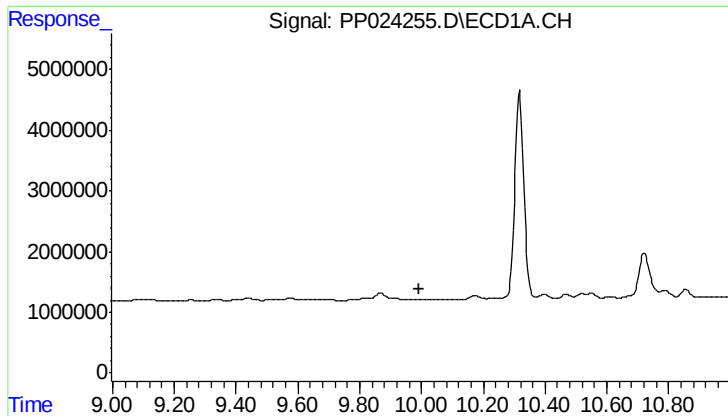

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.994 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
B21

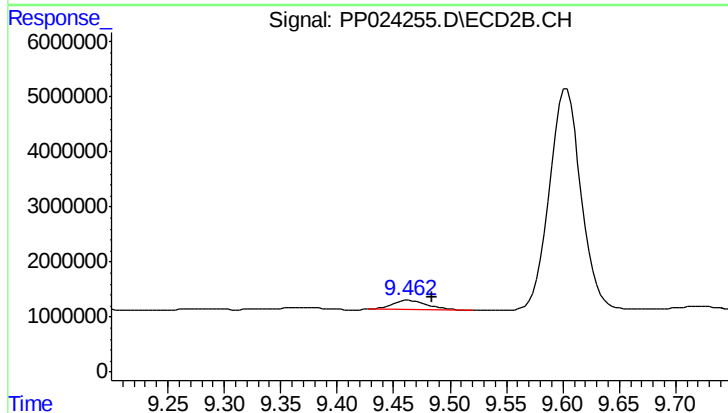


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.464 min
Delta R.T.: -0.020 min
Response: 3601986
Conc: 4.32 ng/ml

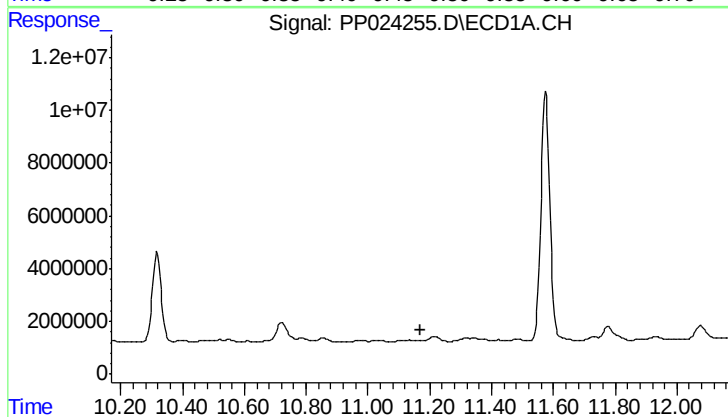


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 11.169 min
Response: 0
Conc: N.D.

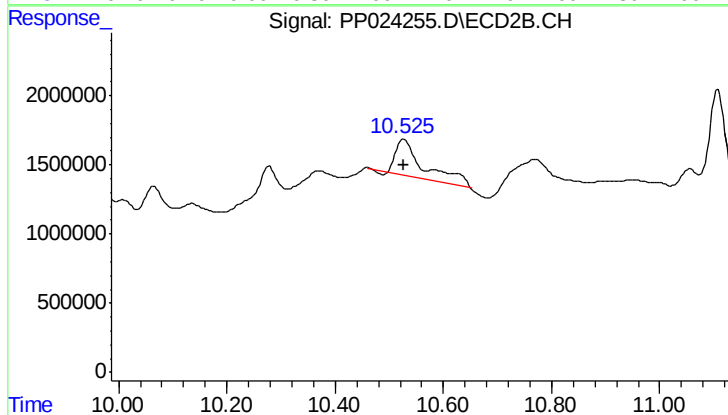

#3 4-Nitrophenol


R.T.: 10.527 min
Delta R.T.: -0.001 min
Response: 9473002
Conc: 20.41 ng/ml

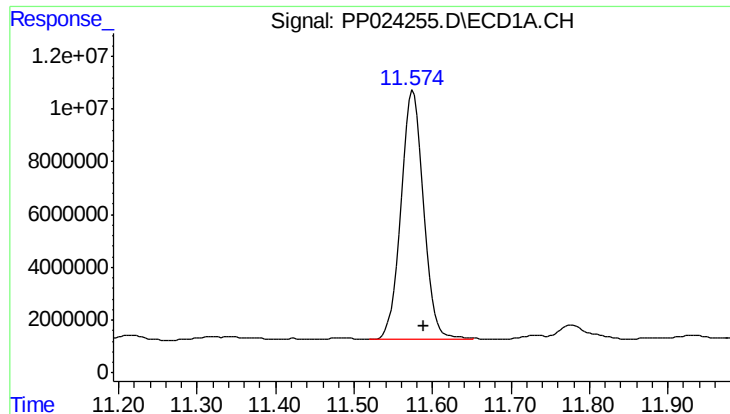

#4 2,4-DCAA


R.T.: 11.575 min
Delta R.T.: -0.014 min
Response: 191048103
Conc: 372.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
B21

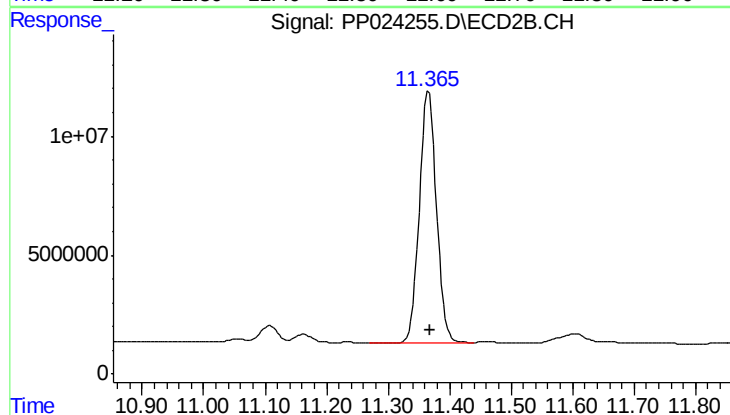


#4 2,4-DCAA

R.T.: 11.366 min
Delta R.T.: -0.003 min
Response: 205015473
Conc: 338.08 ng/ml

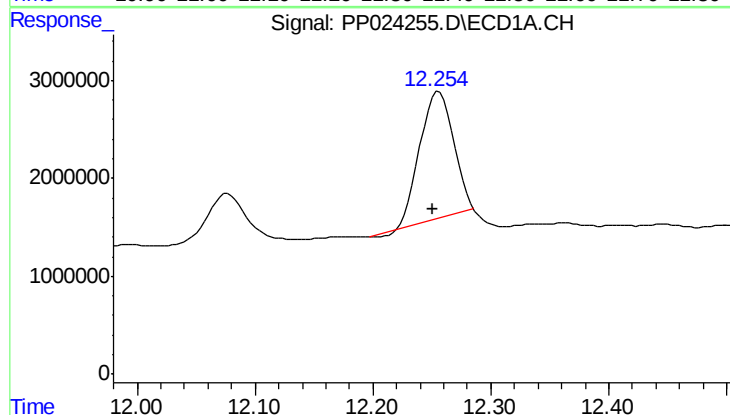


#6 MCP

R.T.: 12.256 min
Delta R.T.: 0.006 min
Response: 25739358
Conc: 17.56 ug/ml

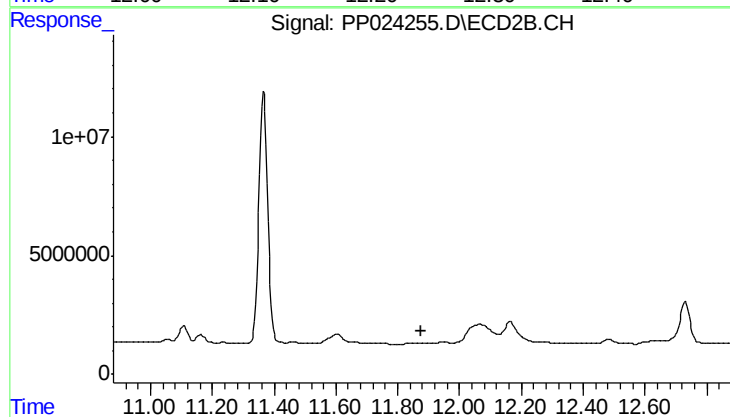

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.878 min
Response: 0
Conc: N.D.

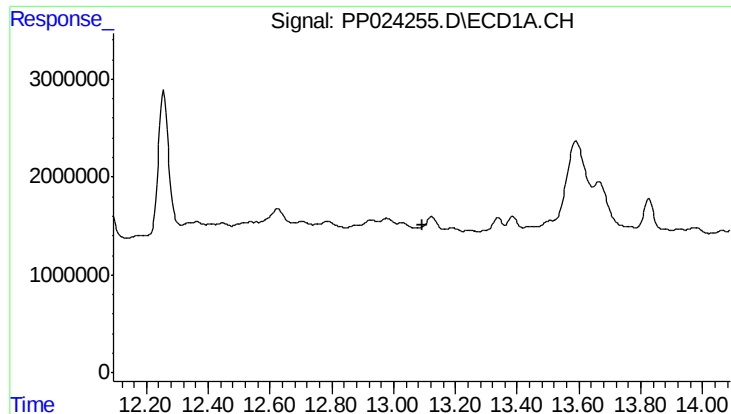

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.092 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
B21

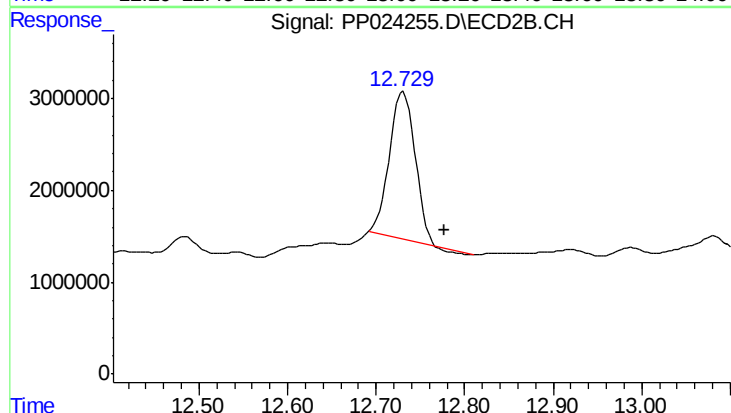


#8 DICHLORPROP

R.T.: 12.731 min
Delta R.T.: -0.047 min
Response: 32310763
Conc: 55.03 ng/ml

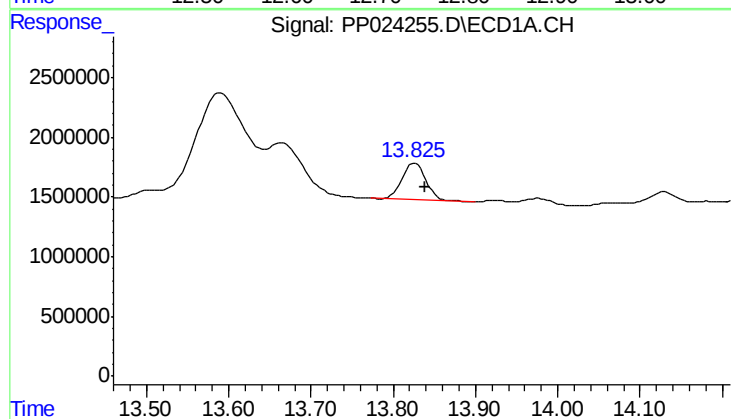


#10 Pentachlorophenol

R.T.: 13.826 min
Delta R.T.: -0.012 min
Response: 6228637
Conc: 0.77 ng/ml

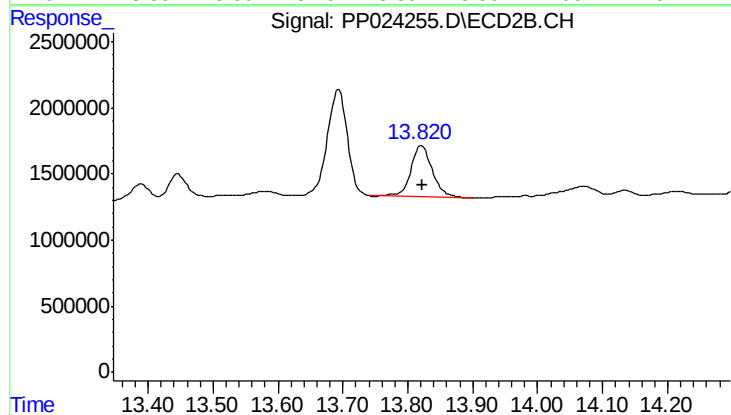

#10 Pentachlorophenol


R.T.: 13.821 min
Delta R.T.: -0.002 min
Response: 8809689
Conc: 1.02 ng/ml

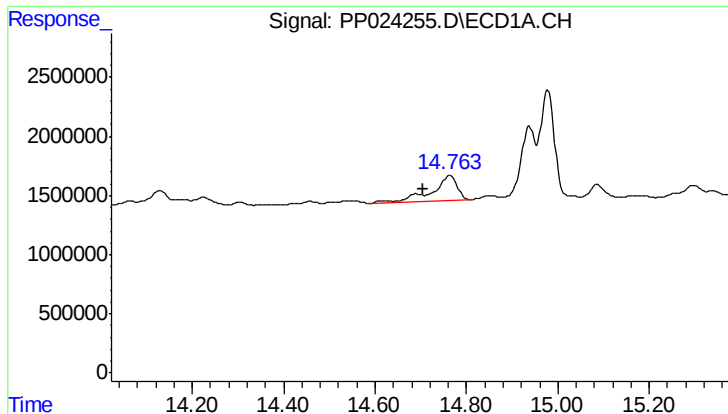

#11 2,4,5-TP (SILVEX)


R.T.: 14.764 min
Delta R.T.: 0.057 min
Response: 8315470
Conc: 2.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
B21

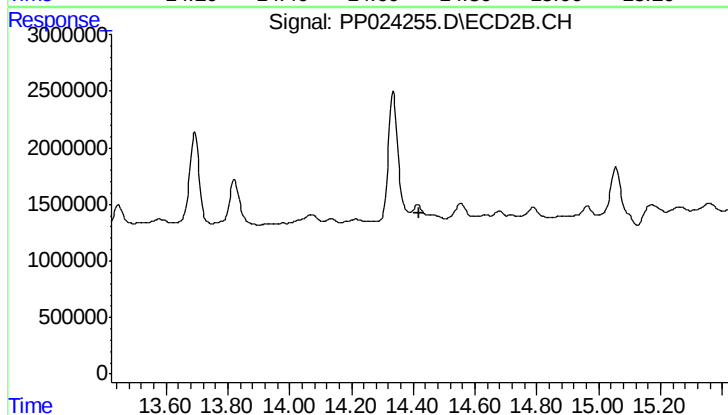


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.421 min
Response: 0
Conc: N.D.

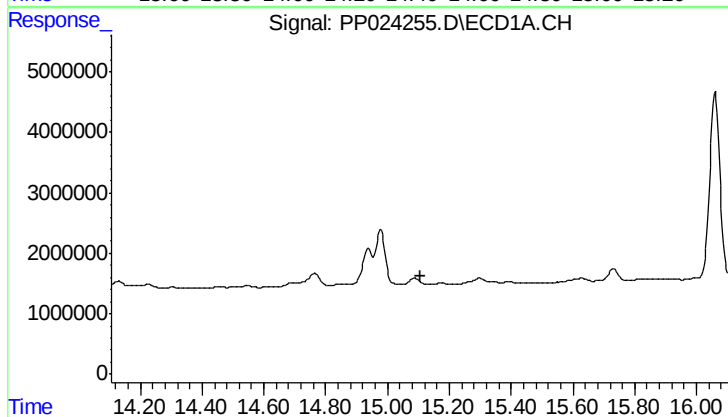


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 15.106 min
Response: 0
Conc: N.D.

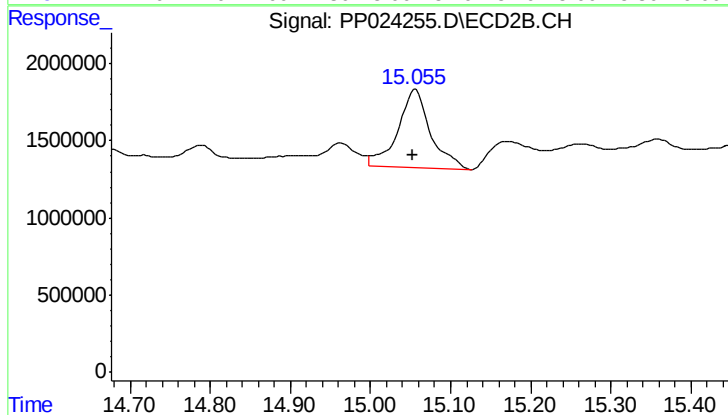

#12 2,4,5-T


R.T.: 15.056 min
Delta R.T.: 0.003 min
Response: 14350719
Conc: 4.66 ng/ml

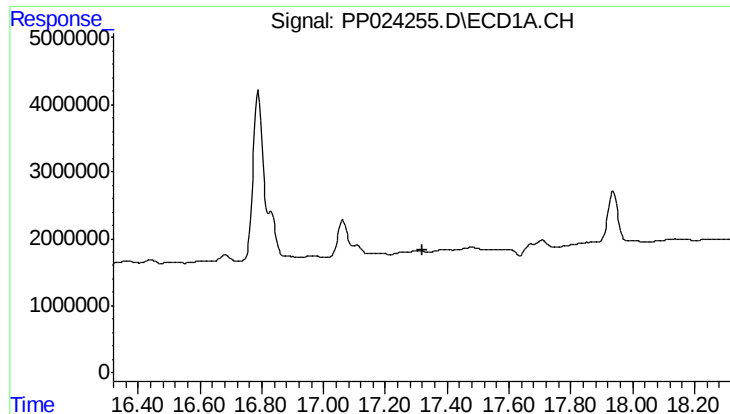

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
B21

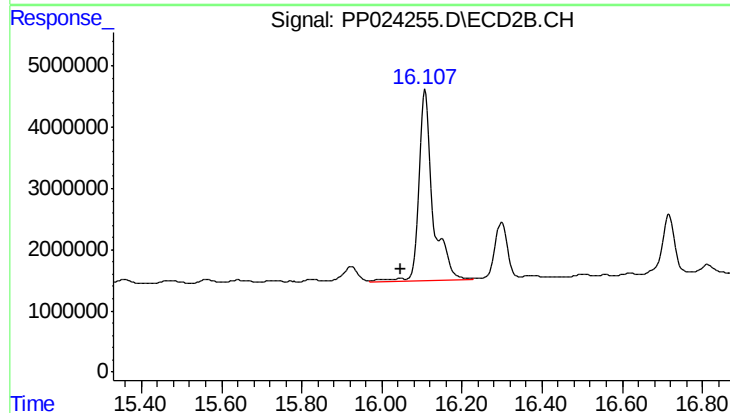


#14 DINOSEB

R.T.: 16.109 min
Delta R.T.: 0.060 min
Response: 79327060
Conc: 32.25 ng/ml

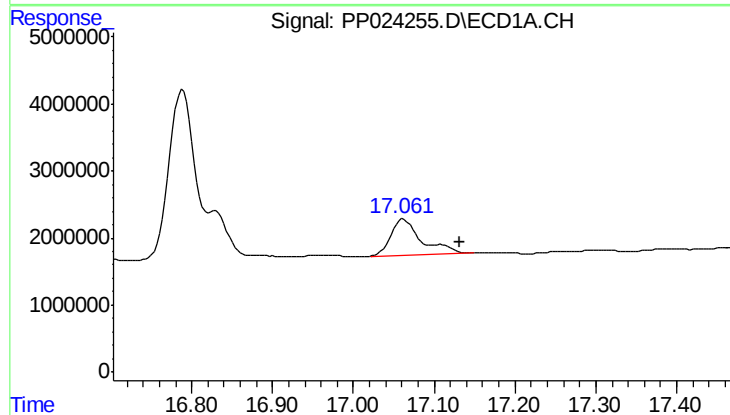

#15 Picloram

R.T.: 17.063 min
Delta R.T.: -0.070 min
Response: 14364573
Conc: 2.95 ng/ml

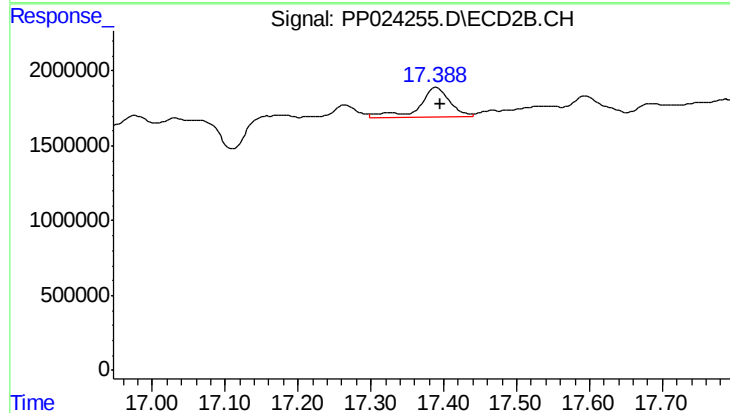

#15 Picloram

R.T.: 17.390 min
Delta R.T.: -0.005 min
Response: 5905399
Conc: 1.19 ng/ml