

Data Path : P:\HPCHEM1\ECD_P\Data\PP030618\
 Data File : PP024275.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Mar 2018 5:14
 Operator : UA/AJ
 Sample : J1809-08
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 RO-5-7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 06:01:22 2018
 Quant Method : P:\HPCHEM1\ECD_P\methods\PP020618.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 06 02:07:55 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.575	11.366	205.5E6	219.8E6	401.066	362.379
Target Compounds							
1) T	Dalapon	2.950	0.000	3488421	0	4.371	N.D. #
2) T	3,5-DICHL...	0.000	9.460	0	9685910	N.D.	11.613 #
3) T	4-Nitroph...	11.216	10.524	11840445	14707660	27.538	31.691
6) T	MCP	12.255	0.000	34481908	0	23.518	N.D. #
8) T	DICHLORPROP	0.000	12.731	0	40836828	N.D.	69.557 #
10) T	Pentachlo...	0.000	13.823	0	5854645	N.D.	0.680 #
11) T	2,4,5-TP ...	14.771	0.000	7937081	0	2.396	N.D. #
12) T	2,4,5-T	0.000	15.052	0	9176937	N.D.	2.979 #
15) T	Picloram	0.000	17.389	0	3868676	N.D.	0.777 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_P\Data\PP030618\
Data File : PP024275.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Mar 2018 5:14
Operator : UA/AJ
Sample : J1809-08
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
RO-5-7

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 06:01:22 2018
Quant Method : P:\HPCHEM1\ECD_P\methods\PP020618.M
Quant Title : 8080.M
QLast Update : Tue Feb 06 02:07:55 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

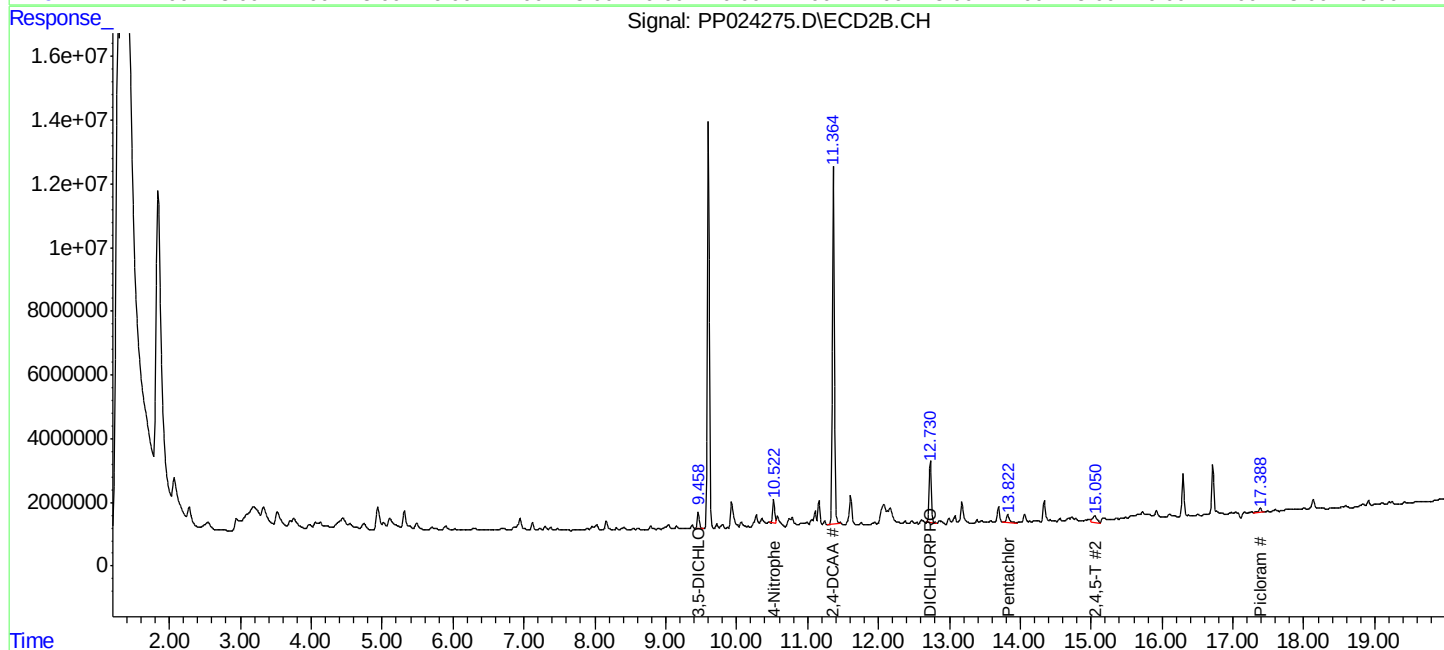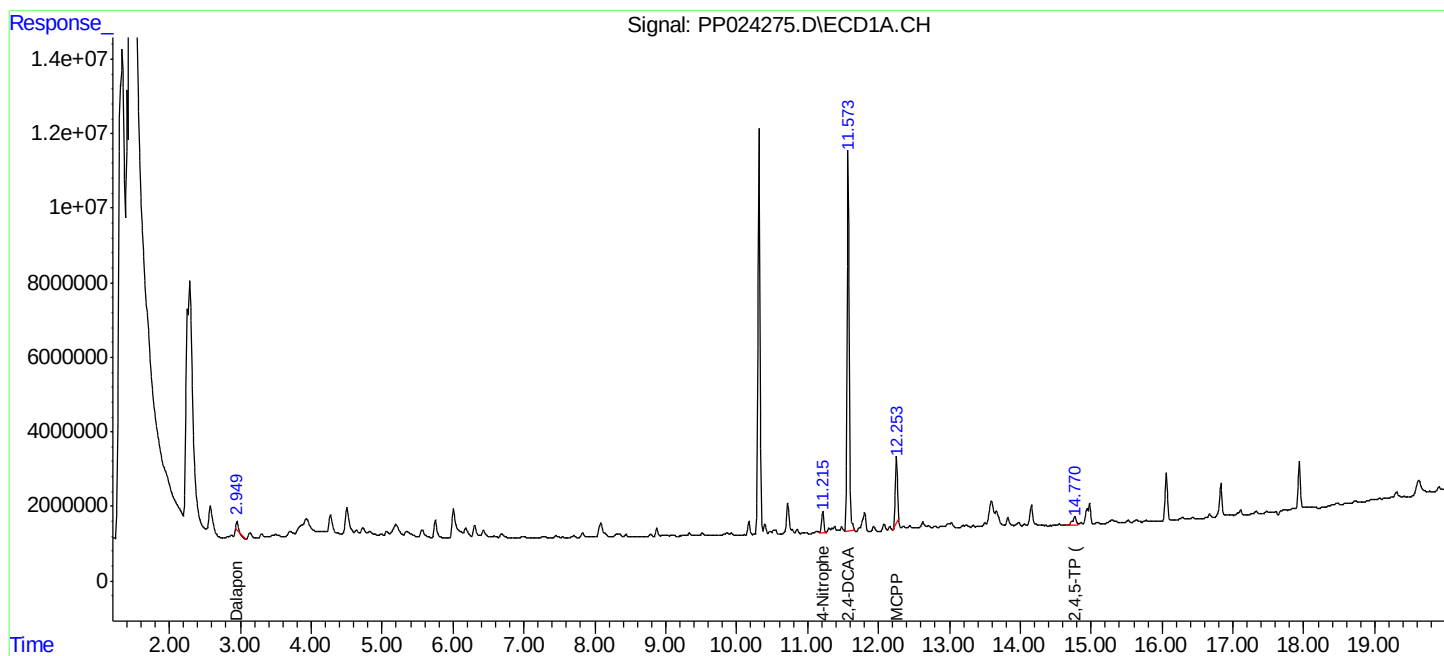


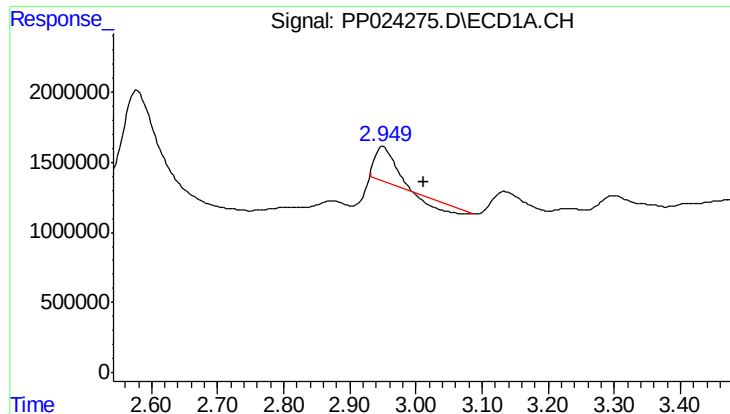

#1 Dalapon


R.T.: 2.950 min
Delta R.T.: -0.062 min
Response: 3488421
Conc: 4.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
RO-5-7

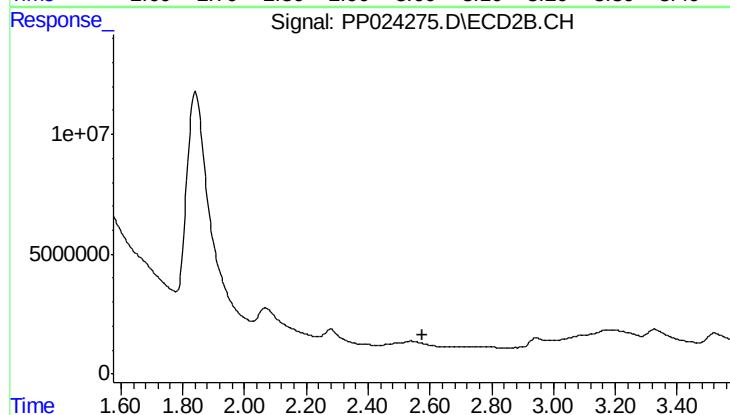


#1 Dalapon

R.T.: 0.000 min
Exp R.T.: 2.575 min
Response: 0
Conc: N.D.

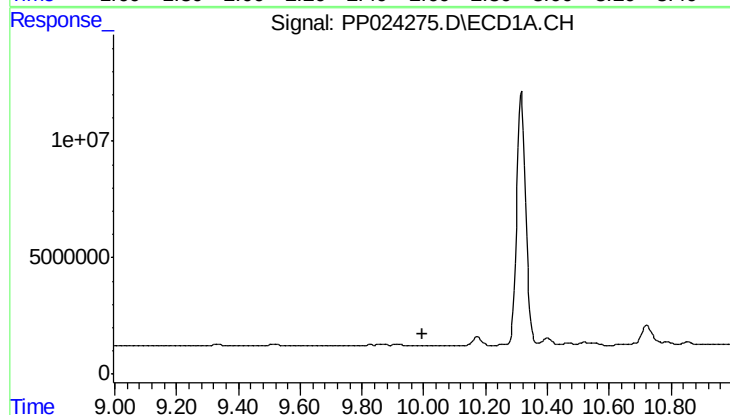


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 9.994 min
Response: 0
Conc: N.D.

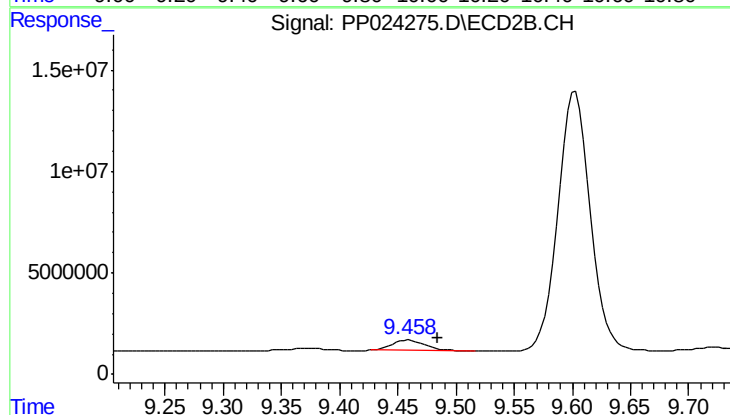

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.460 min
Delta R.T.: -0.025 min
Response: 9685910
Conc: 11.61 ng/ml

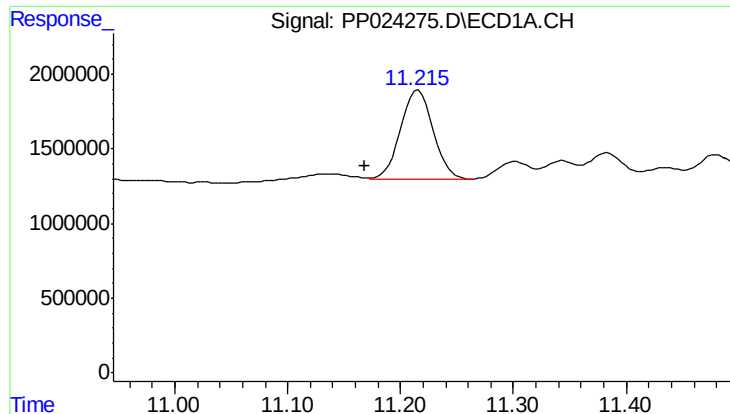

#3 4-Nitrophenol


R.T.: 11.216 min
Delta R.T.: 0.047 min
Response: 11840445
Conc: 27.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
RO-5-7

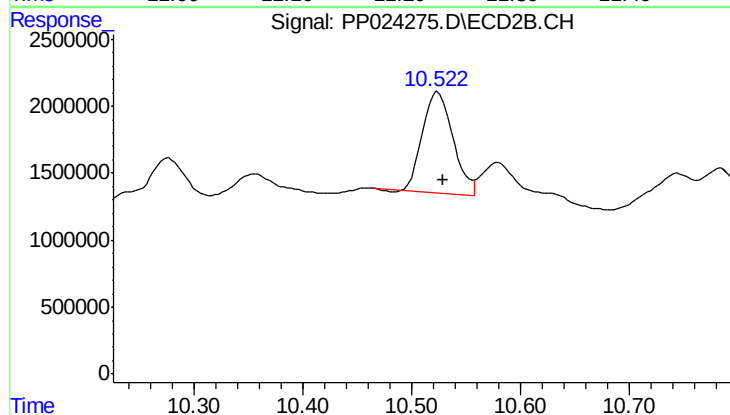


#3 4-Nitrophenol

R.T.: 10.524 min
Delta R.T.: -0.004 min
Response: 14707660
Conc: 31.69 ng/ml

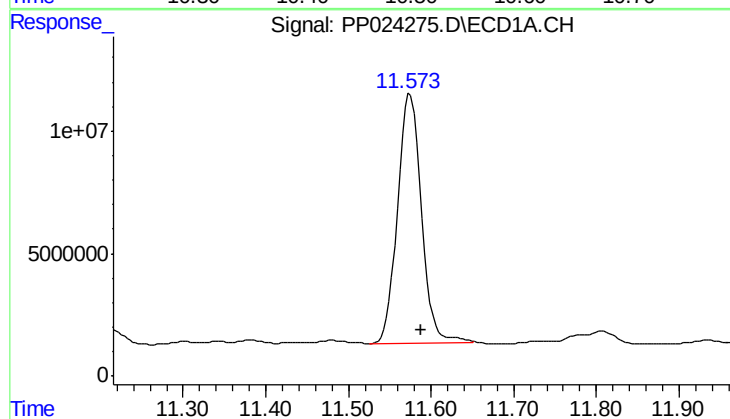


#4 2,4-DCAA

R.T.: 11.575 min
Delta R.T.: -0.014 min
Response: 205534702
Conc: 401.07 ng/ml

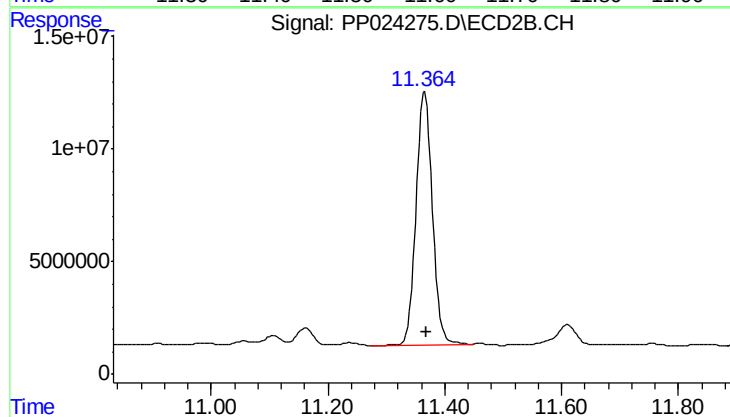

#4 2,4-DCAA


R.T.: 11.366 min
Delta R.T.: -0.003 min
Response: 219753164
Conc: 362.38 ng/ml

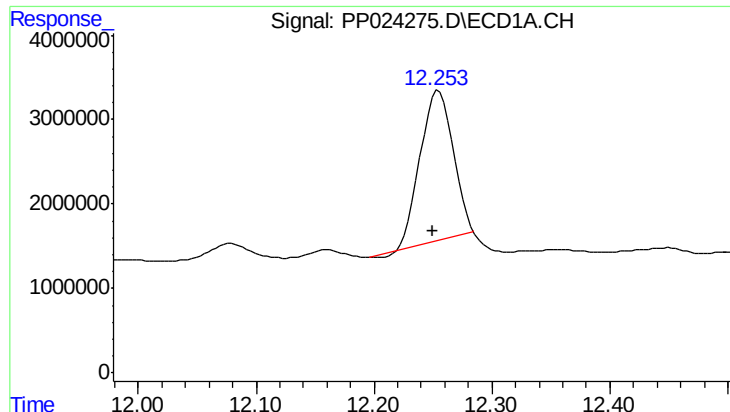

#6 MCPP


R.T.: 12.255 min
Delta R.T.: 0.005 min
Response: 34481908
Conc: 23.52 ug/ml

Instrument :
ECD_O
ClientSampleId :
RO-5-7

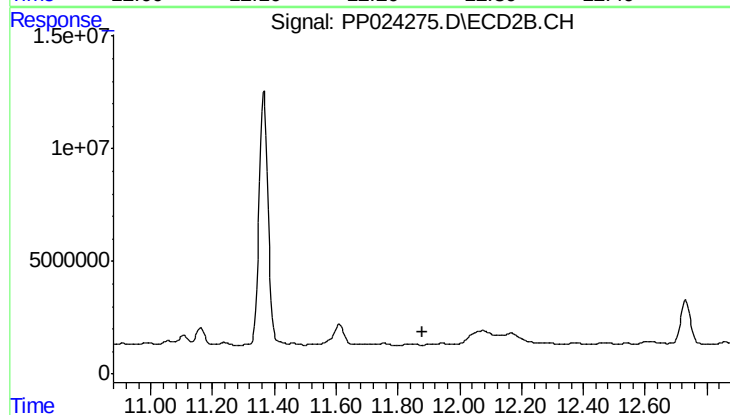


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 11.878 min
Response: 0
Conc: N.D.

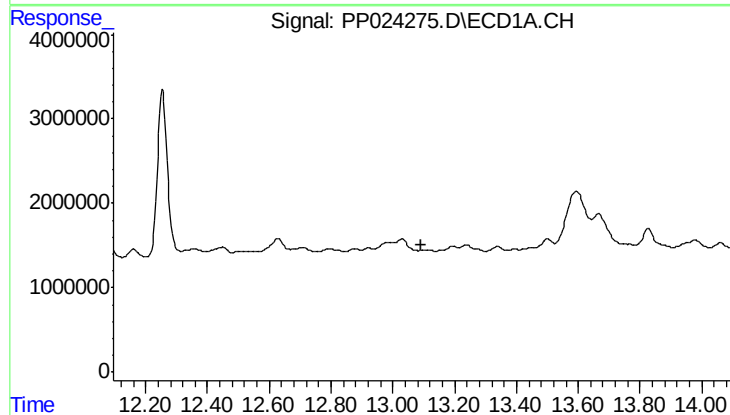


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 13.092 min
Response: 0
Conc: N.D.

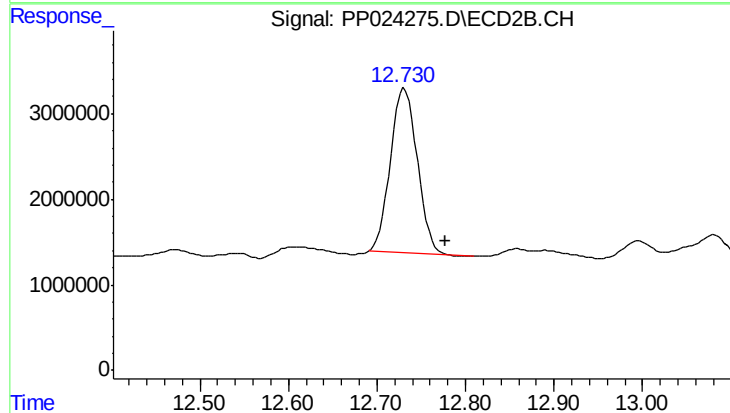

#8 DICHLORPROP


R.T.: 12.731 min
Delta R.T.: -0.046 min
Response: 40836828
Conc: 69.56 ng/ml

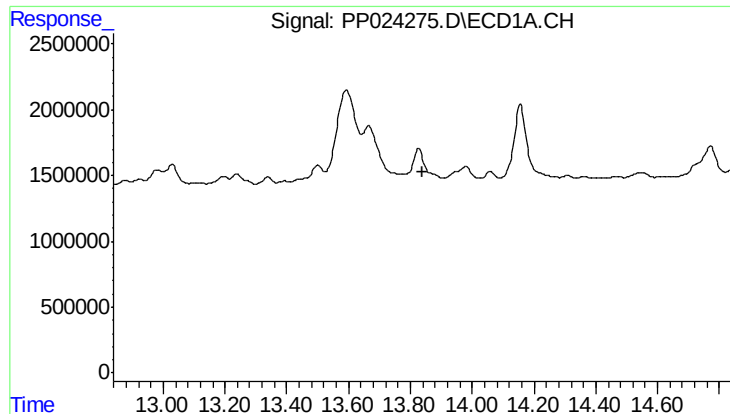

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.838 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
RO-5-7

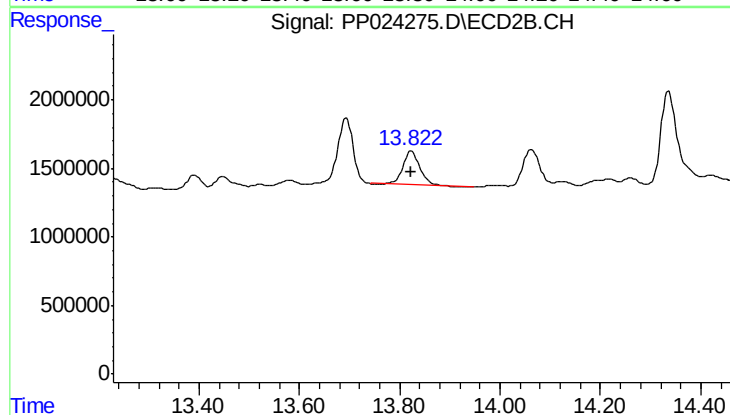


#10 Pentachlorophenol

R.T.: 13.823 min
Delta R.T.: 0.000 min
Response: 5854645
Conc: 0.68 ng/ml

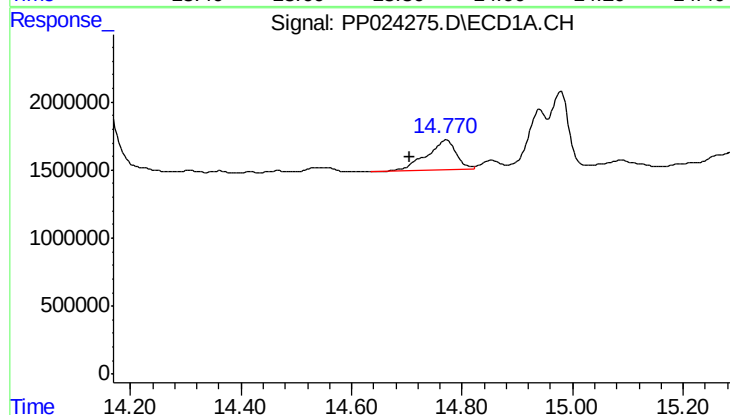


#11 2,4,5-TP (SILVEX)

R.T.: 14.771 min
Delta R.T.: 0.065 min
Response: 7937081
Conc: 2.40 ng/ml

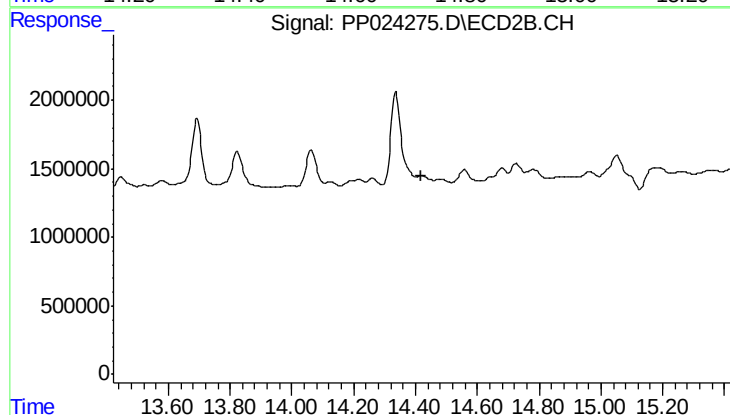

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.421 min
Response: 0
Conc: N.D.

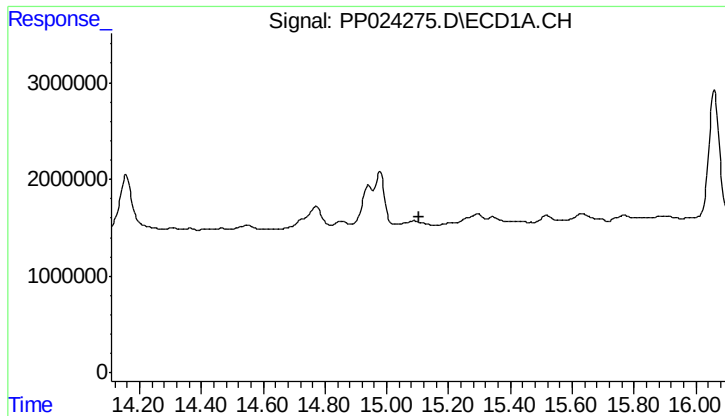

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.106 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
RO-5-7

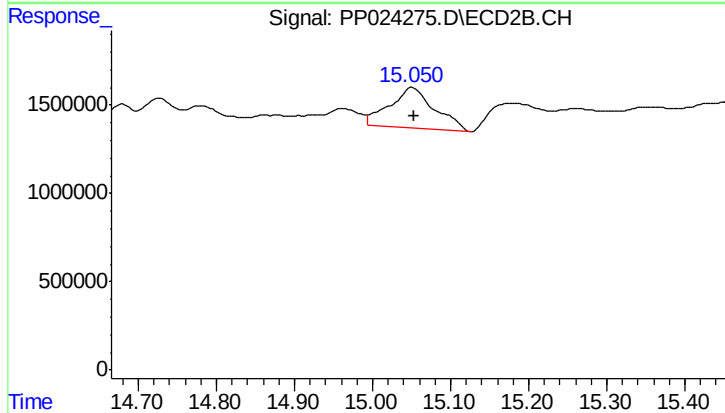


#12 2,4,5-T

R.T.: 15.052 min
Delta R.T.: -0.002 min
Response: 9176937
Conc: 2.98 ng/ml

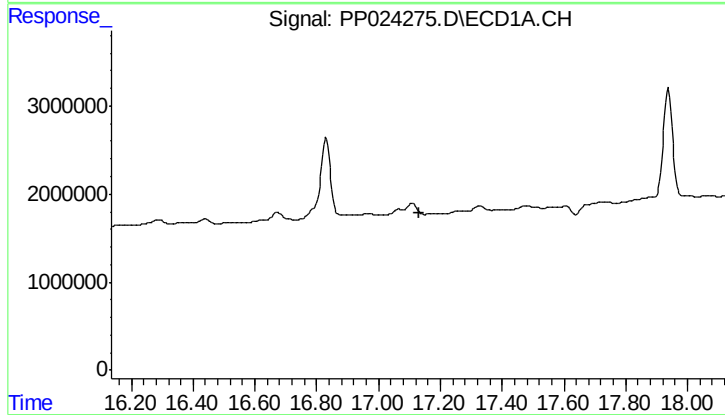

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 17.132 min
Response: 0
Conc: N.D.

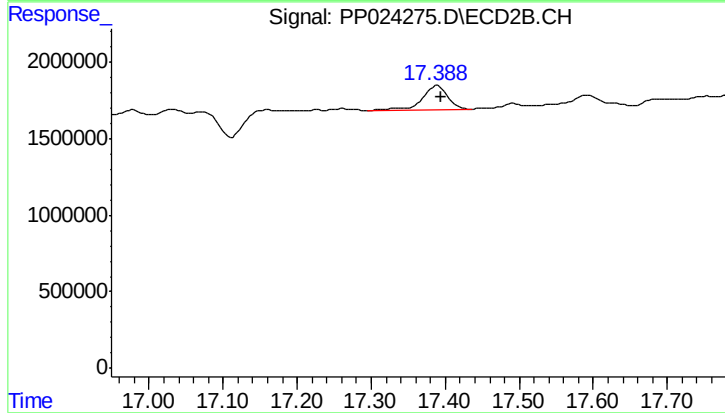

#15 Picloram

R.T.: 17.389 min
Delta R.T.: -0.006 min
Response: 3868676
Conc: 0.78 ng/ml