

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030620\
 Data File : P0066987.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Mar 2020 15:18
 Operator : DD\AJ
 Sample : L1366-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 03-05-C

Manual Integrations
 APPROVED

Sohil
 3/11/2020 10:55:14 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 16:11:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 04 13:48:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.118	3.402	1252229	1056696	23.490m	22.792
2) SA Decachlor...	9.587	8.282	1135273	1153716	20.620	22.315m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030620\
Data File : P0066987.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Mar 2020 15:18
Operator : DD\AJ
Sample : L1366-03
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
03-05-C


Manual Integrations
APPROVED

Sohil
3/11/2020 10:55:14 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 16:11:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 04 13:48:03 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

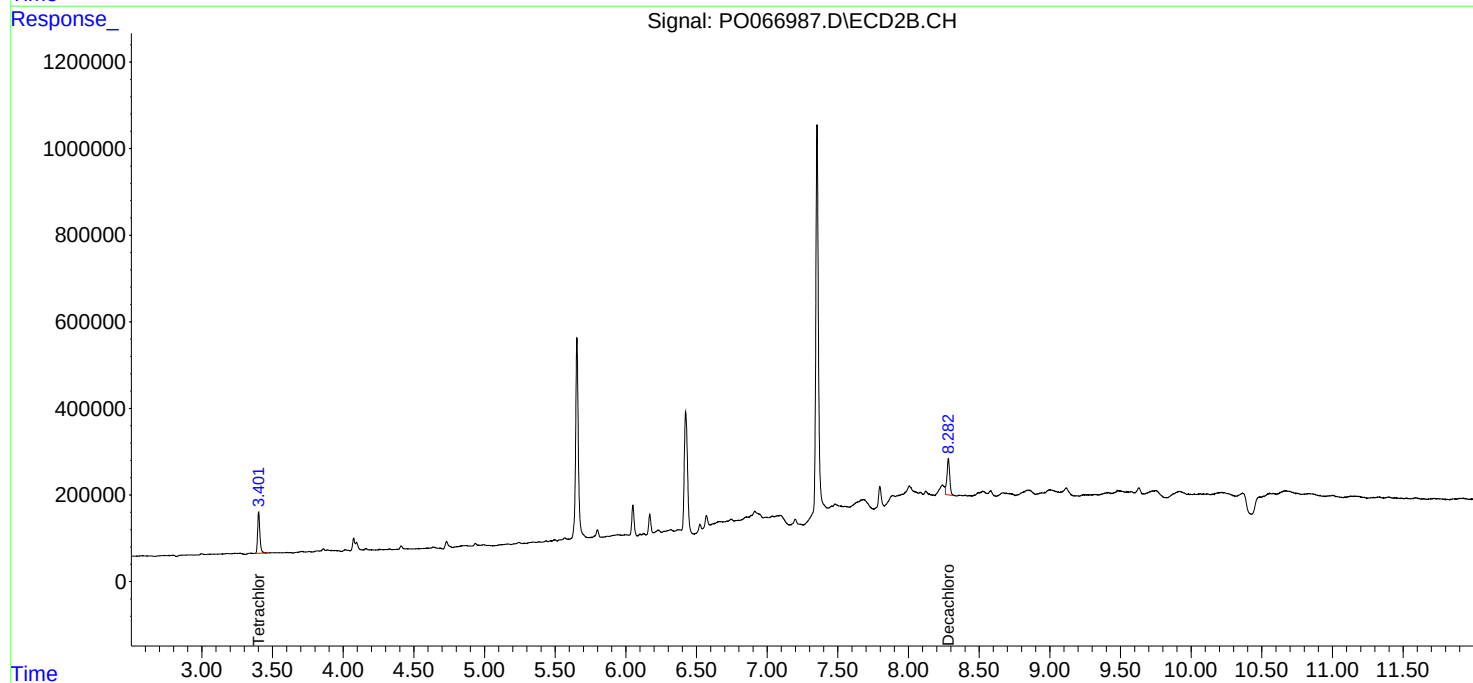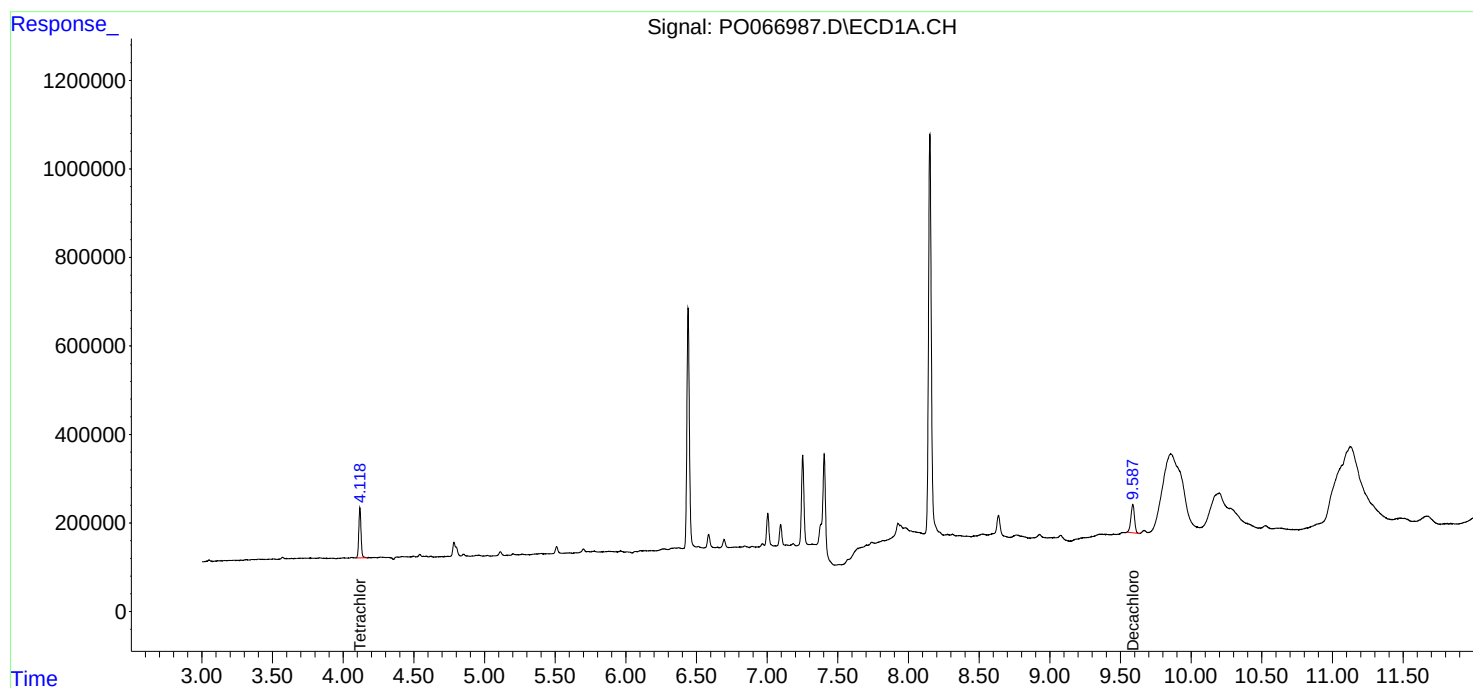

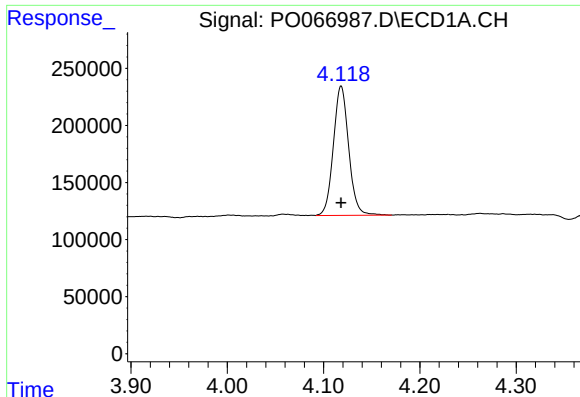


#1 Tetrachloro-m-xylene

R.T.: 4.118 min
Delta R.T.: 0.000 min
Response: 1252229
Conc: 23.49 ng/ml m

Instrument :
ECD_O
ClientSampleId :
03-05-C


Manual Integrations
APPROVED

Sohil
3/11/2020 10:55:14 AM

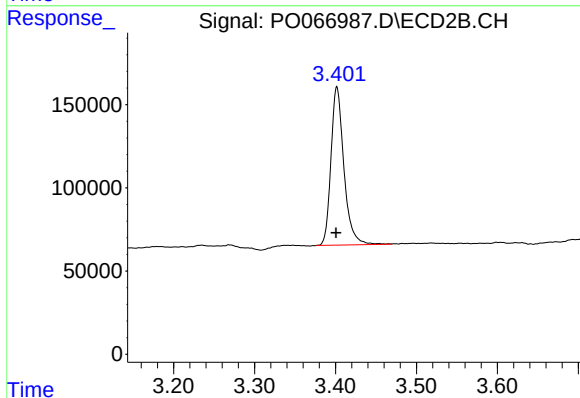


#1 Tetrachloro-m-xylene

R.T.: 3.402 min
Delta R.T.: 0.001 min
Response: 1056696
Conc: 22.79 ng/ml

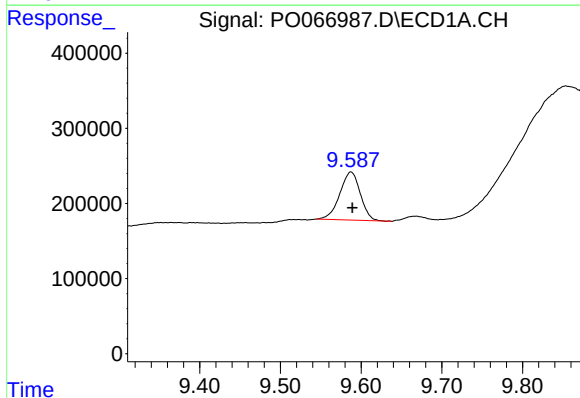

#2 Decachlorobiphenyl

R.T.: 9.587 min
Delta R.T.: -0.002 min
Response: 1135273
Conc: 20.62 ng/ml

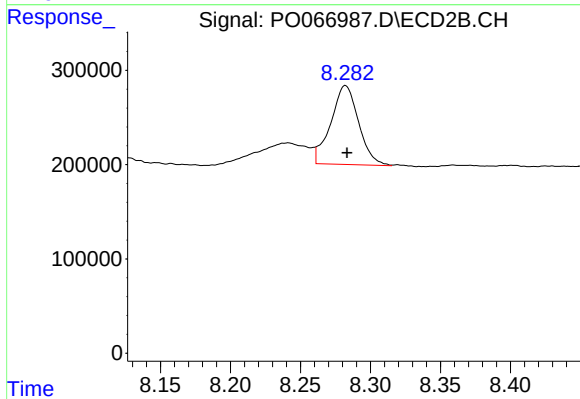

#2 Decachlorobiphenyl

R.T.: 8.282 min
Delta R.T.: -0.002 min
Response: 1153716
Conc: 22.32 ng/ml m