

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030620\
 Data File : P0066998.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Mar 2020 19:43
 Operator : DD\AJ
 Sample : L1753-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CL-01-030520

Manual Integrations
 APPROVED

Sohil
 3/11/2020 10:55:22 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 03:15:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 04 13:48:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.118	3.402	886691	838659	16.633m	18.089
2) SA Decachlor...	9.585	8.282	915948	883566	16.636	17.090

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030620\
Data File : P0066998.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Mar 2020 19:43
Operator : DD\AJ
Sample : L1753-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CL-01-030520


Manual Integrations
APPROVED

Sohil
3/11/2020 10:55:22 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 03:15:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 04 13:48:03 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

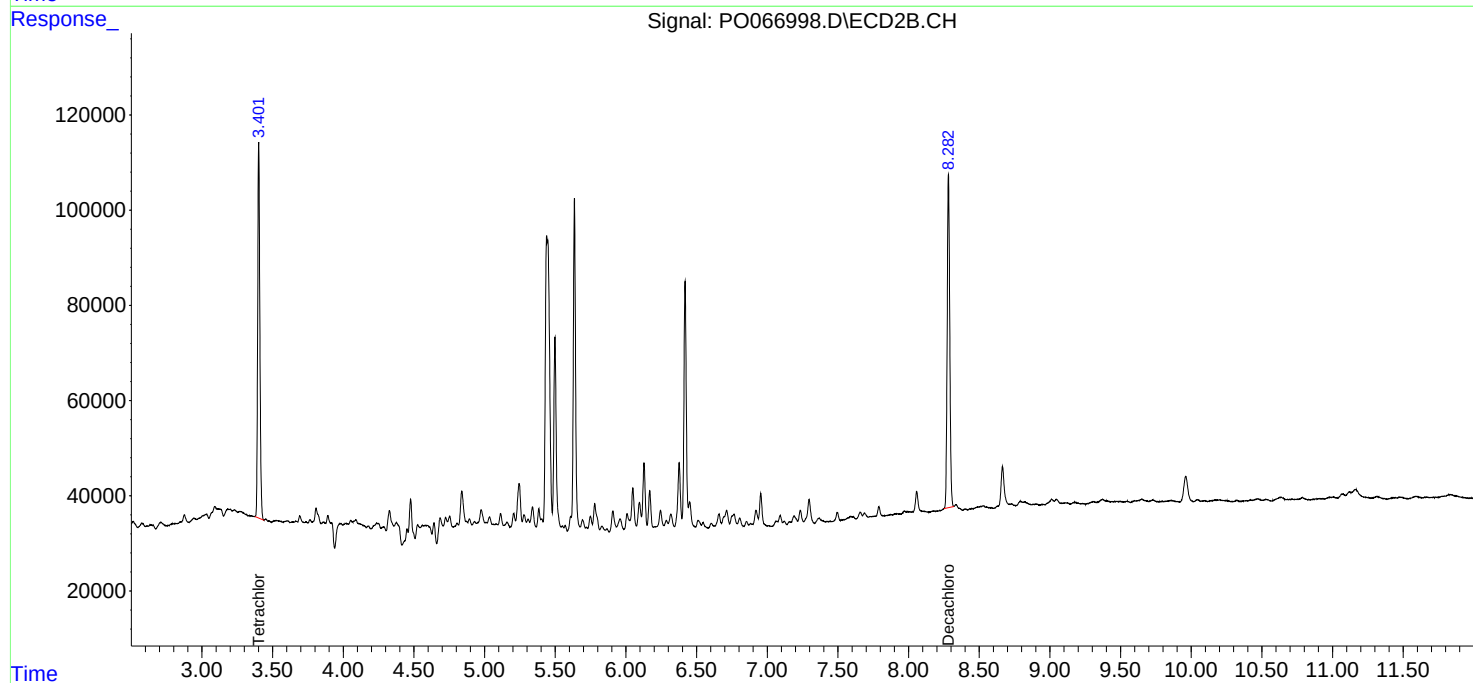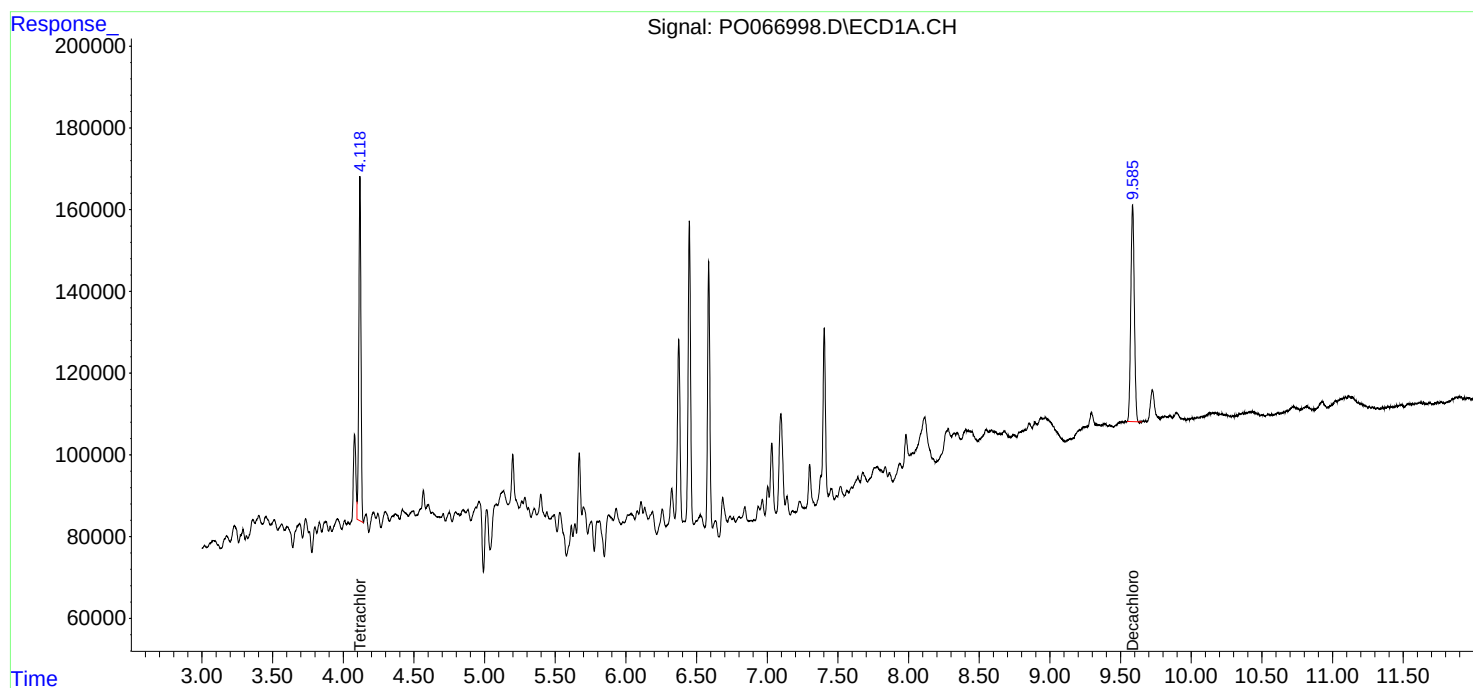

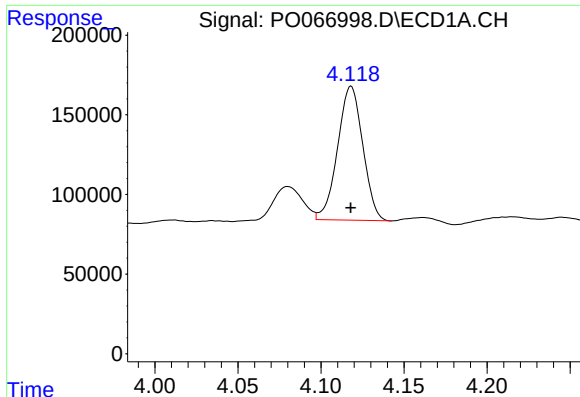


#1 Tetrachloro-m-xylene

R.T.: 4.118 min
Delta R.T.: 0.000 min
Response: 886691
Conc: 16.63 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CL-01-030520


Manual Integrations
APPROVED

Sohil
3/11/2020 10:55:22 AM

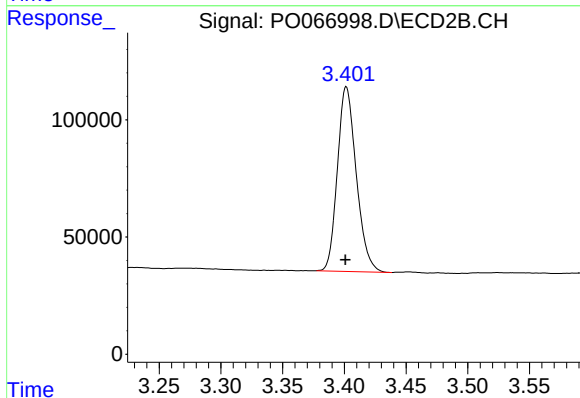


#1 Tetrachloro-m-xylene

R.T.: 3.402 min
Delta R.T.: 0.000 min
Response: 838659
Conc: 18.09 ng/ml

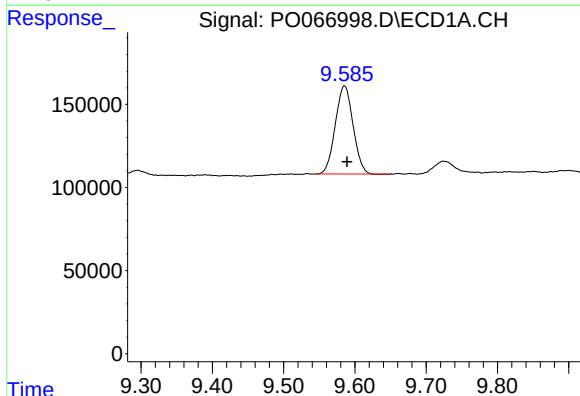

#2 Decachlorobiphenyl

R.T.: 9.585 min
Delta R.T.: -0.004 min
Response: 915948
Conc: 16.64 ng/ml

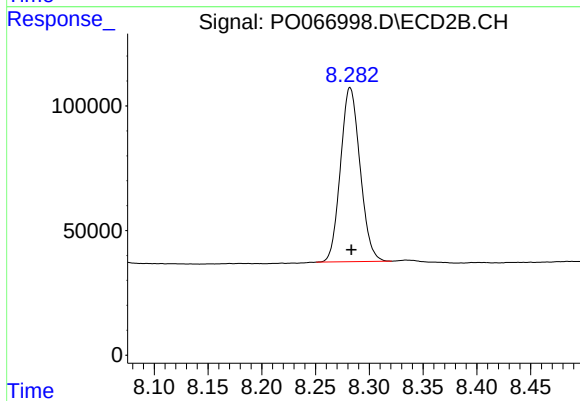

#2 Decachlorobiphenyl

R.T.: 8.282 min
Delta R.T.: -0.001 min
Response: 883566
Conc: 17.09 ng/ml