

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030725\
 Data File : P0109734.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2025 20:54
 Operator : YP/AJ
 Sample : Q1516-03
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 GAS-AUD-25-0026

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 00:07:09 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:40:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.696	3.694	230.5E6	129.1E6	24.351	24.670
2) SA Decachlor...	8.752	8.704	170.6E6	68446583	19.834	21.495

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030725\
Data File : PO109734.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2025 20:54
Operator : YP/AJ
Sample : Q1516-03
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
GAS-AUD-25-0026

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 00:07:09 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:40:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

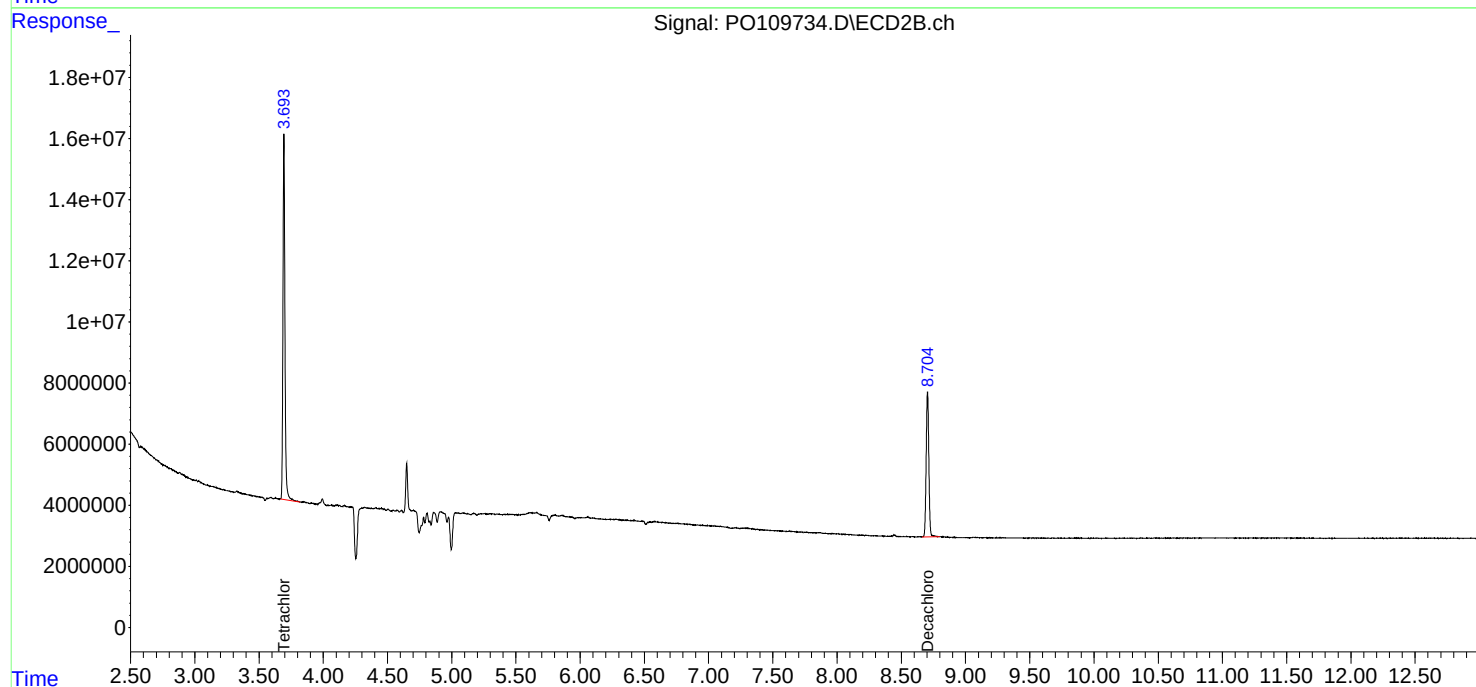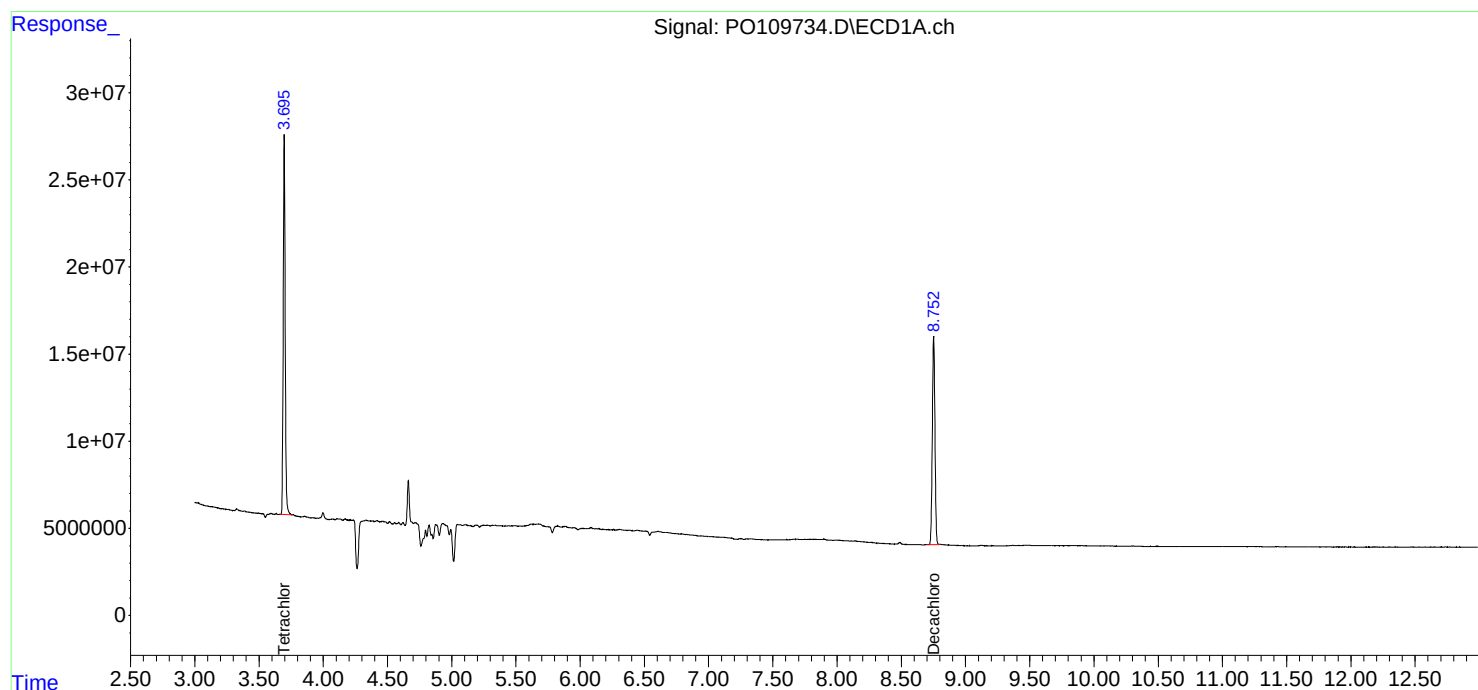


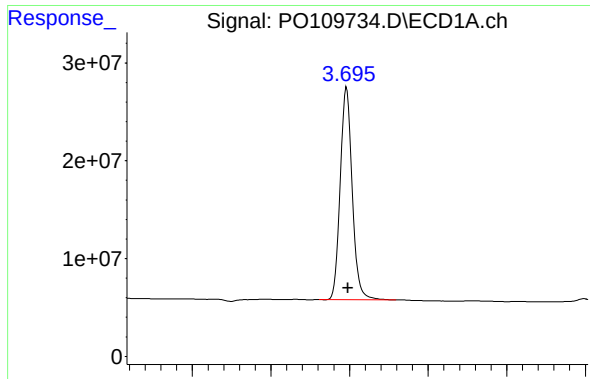

#1 Tetrachloro-m-xylene


R.T.: 3.696 min
Delta R.T.: -0.002 min
Response: 230488769
Conc: 24.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
GAS-AUD-25-0026

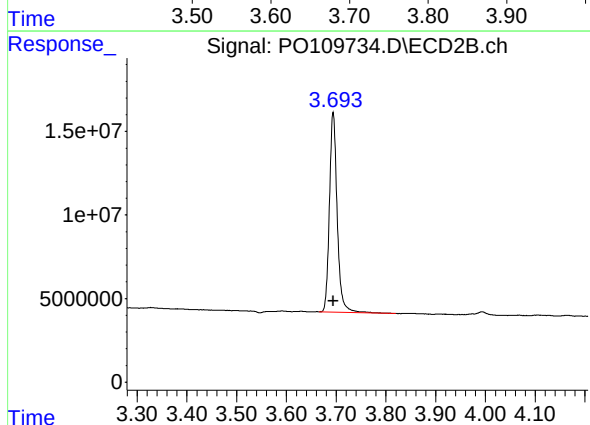


#1 Tetrachloro-m-xylene

R.T.: 3.694 min
Delta R.T.: 0.000 min
Response: 129128644
Conc: 24.67 ng/ml

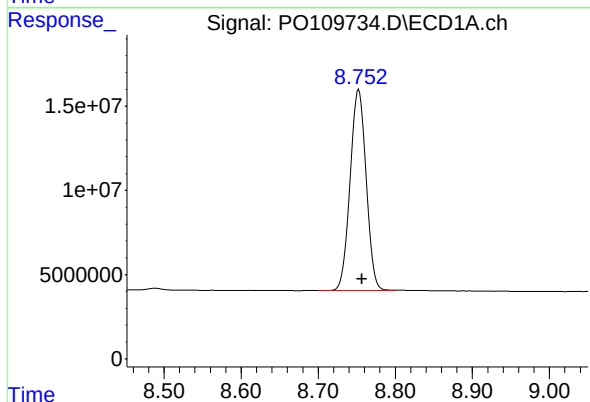

#2 Decachlorobiphenyl

R.T.: 8.752 min
Delta R.T.: -0.004 min
Response: 170606472
Conc: 19.83 ng/ml

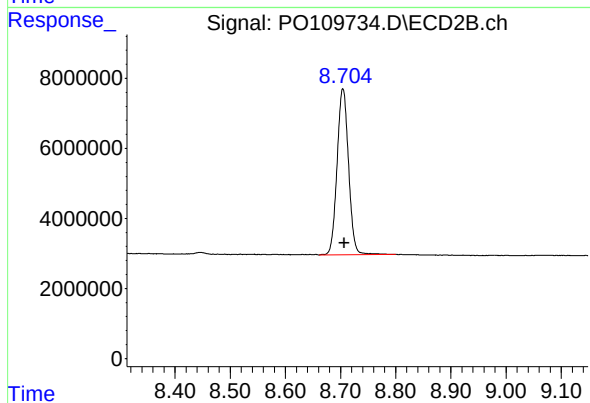

#2 Decachlorobiphenyl

R.T.: 8.704 min
Delta R.T.: -0.003 min
Response: 68446583
Conc: 21.50 ng/ml