

Data Path : P:\HPCHEM1\ECD_0\Data\P0030918\
Data File : P0042858.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Mar 2018 10:29
Operator : SM/UA
Sample : J1814-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DREDGE-DECANT-WATER

Manual Integrations
APPROVED

ugo
3/9/2018 9:41:33 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 11:56:10 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0022118.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 26 14:24:10 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.093	3.340	5888448	4193186	23.771m	11.347m#
2)	SA Decachlor...	9.461	8.117	2182982	2469312	8.638	6.403 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\P0030918\
Data File : P0042858.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Mar 2018 10:29
Operator : SM/UA
Sample : J1814-01
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
DREDGE-DECANT-WATER


Manual Integrations
APPROVED

ugo
3/9/2018 9:41:33 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 11:56:10 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0022118.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 26 14:24:10 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

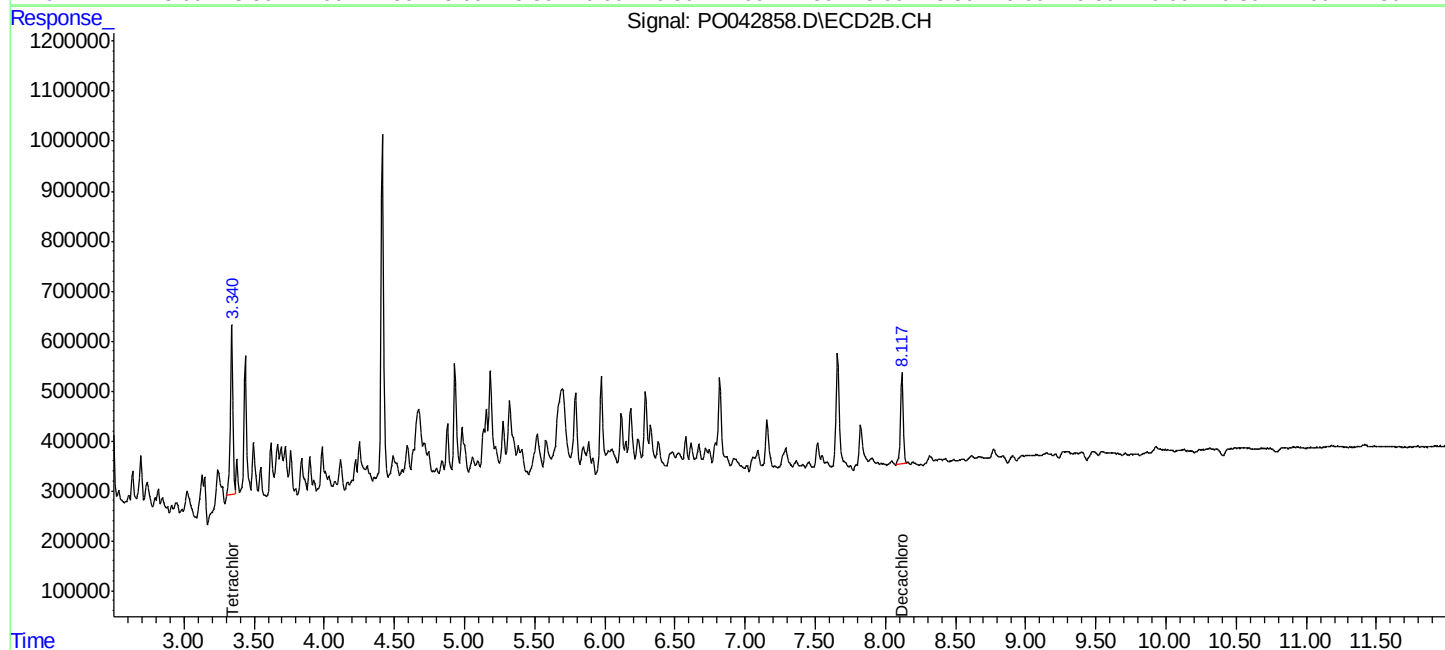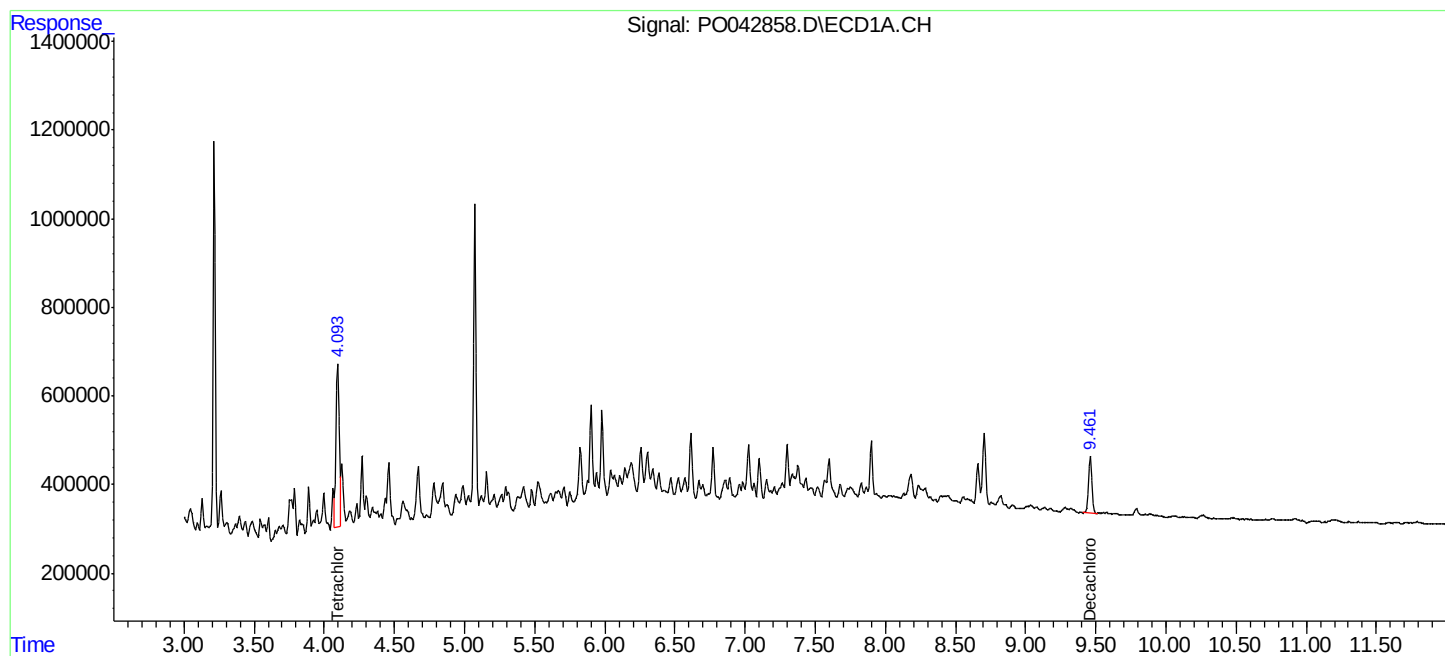

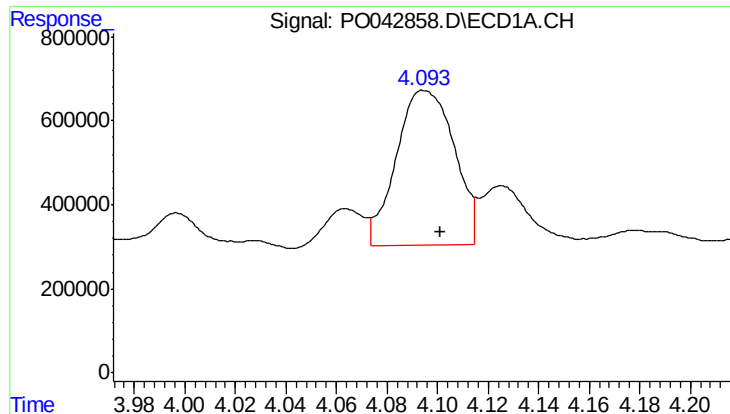


#1 Tetrachloro-m-xylene

R.T.: 4.093 min
Delta R.T.: -0.008 min
Response: 5888448
Conc: 23.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
DREDGE-DECANT-WATER


Manual Integrations
APPROVED

ugo
3/9/2018 9:41:33 PM

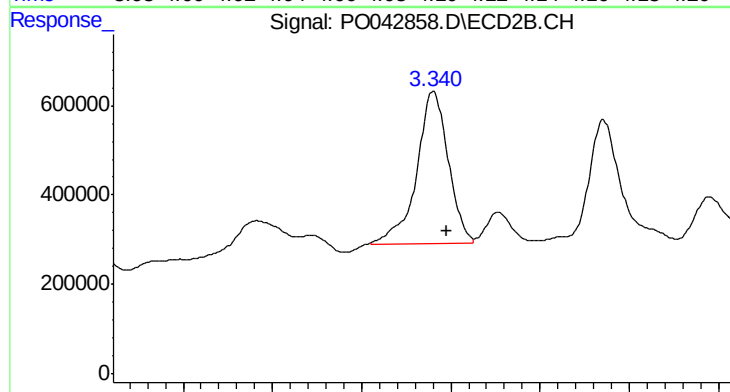


#1 Tetrachloro-m-xylene

R.T.: 3.340 min
Delta R.T.: -0.008 min
Response: 4193186
Conc: 11.35 ng/ml m

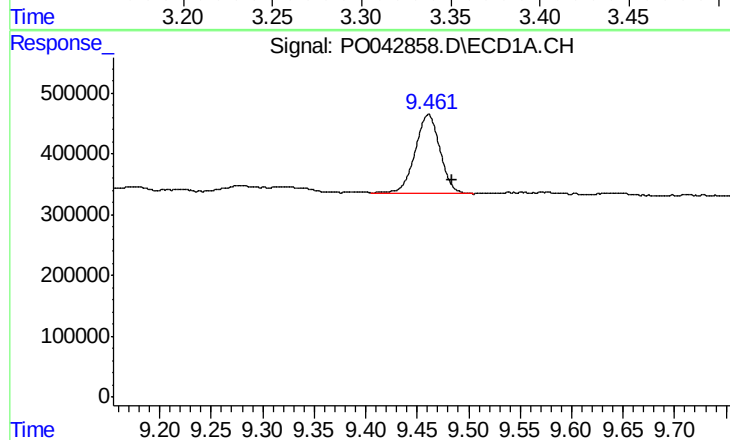

#2 Decachlorobiphenyl

R.T.: 9.461 min
Delta R.T.: -0.023 min
Response: 2182982
Conc: 8.64 ng/ml

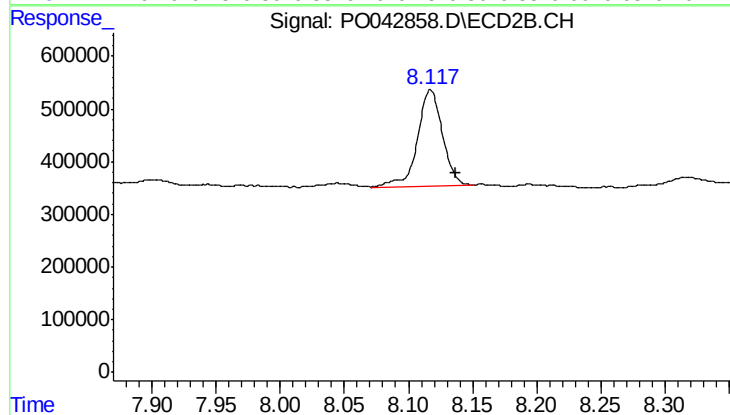

#2 Decachlorobiphenyl

R.T.: 8.117 min
Delta R.T.: -0.019 min
Response: 2469312
Conc: 6.40 ng/ml