

Data Path : P:\HPCHEM1\ECD_0\Data\P0030918\
Data File : P0042859.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Mar 2018 10:44
Operator : SM/UA
Sample : J1794-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
030118-SIDI-F-D-M

Manual Integrations
APPROVED

ugo
3/9/2018 9:41:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 11:57:47 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0022118.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 26 14:24:10 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.089	3.339	3356327	4606808	13.549m	12.467m
2) SA Decachlor...	9.459	8.115	2550930	3230178	10.093m	8.377

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\P0030918\
Data File : P0042859.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Mar 2018 10:44
Operator : SM/UA
Sample : J1794-01
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
030118-SIDI-F-D-M


Manual Integrations
APPROVED

ugo
3/9/2018 9:41:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 11:57:47 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0022118.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 26 14:24:10 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

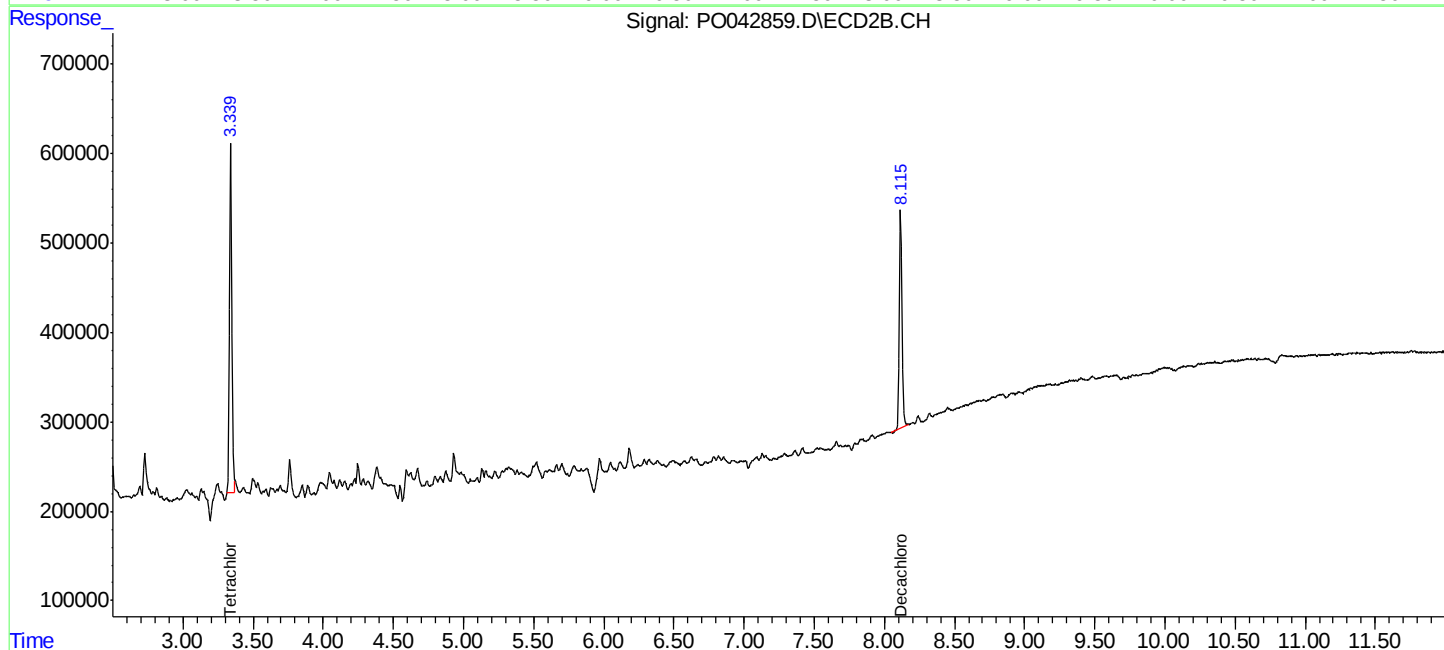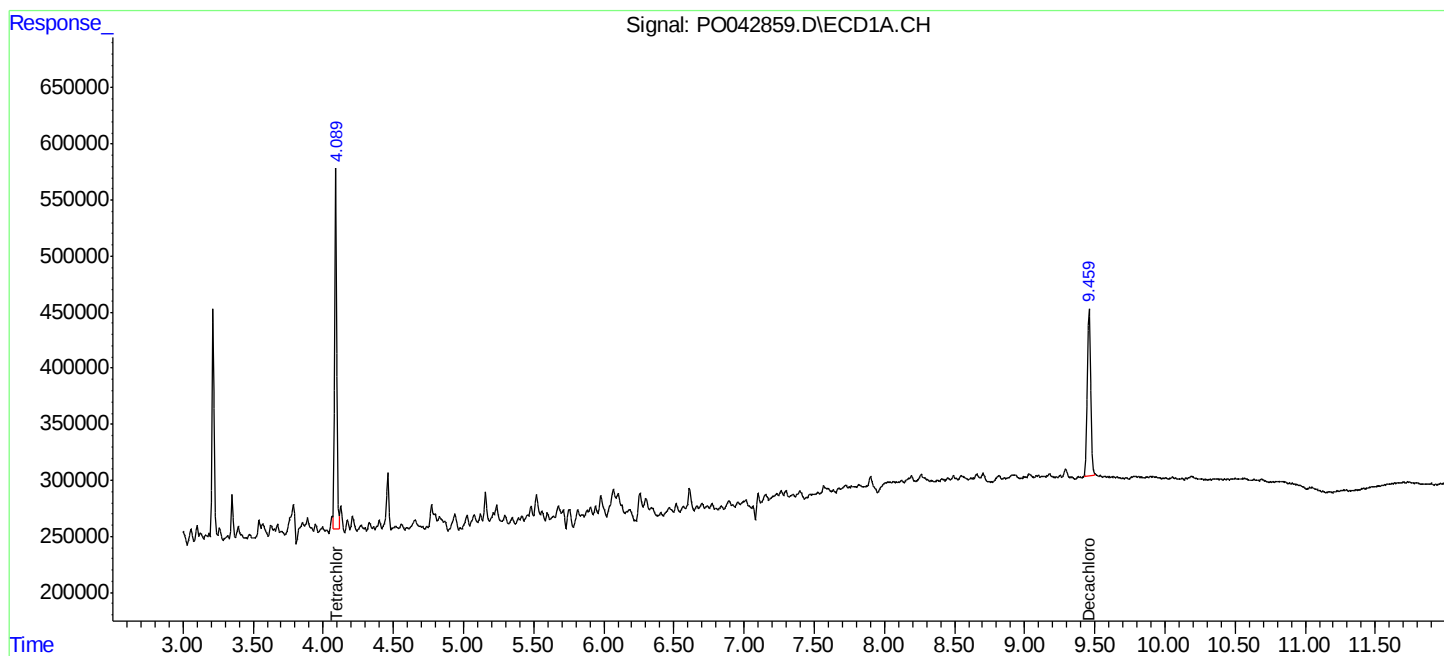

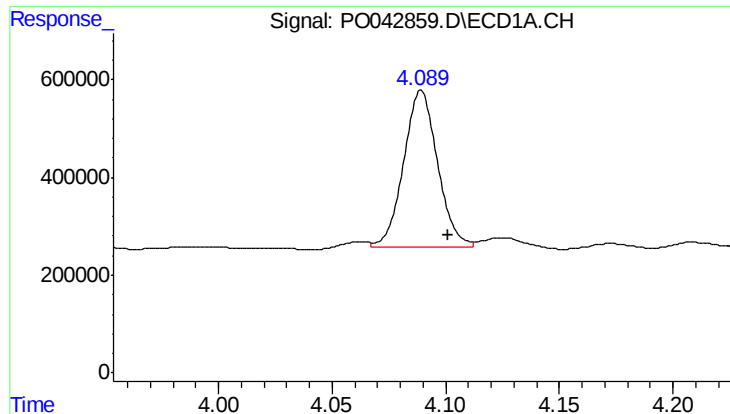


#1 Tetrachloro-m-xylene

R.T.: 4.089 min
Delta R.T.: -0.013 min
Response: 3356327
Conc: 13.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
030118-SIDI-F-D-M


Manual Integrations
APPROVED

ugo
3/9/2018 9:41:40 PM

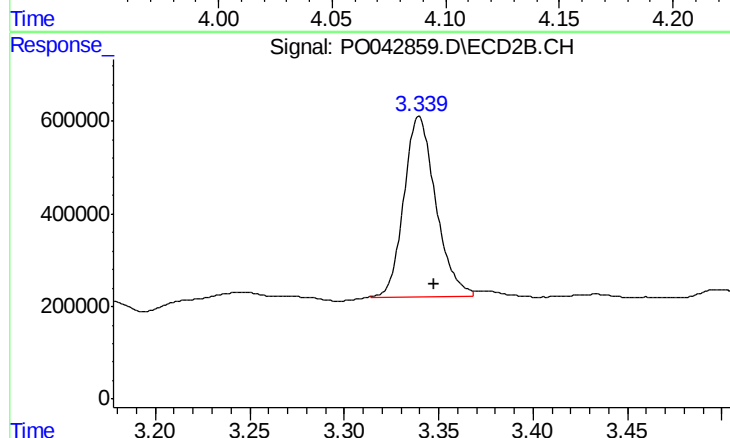


#1 Tetrachloro-m-xylene

R.T.: 3.339 min
Delta R.T.: -0.009 min
Response: 4606808
Conc: 12.47 ng/ml m

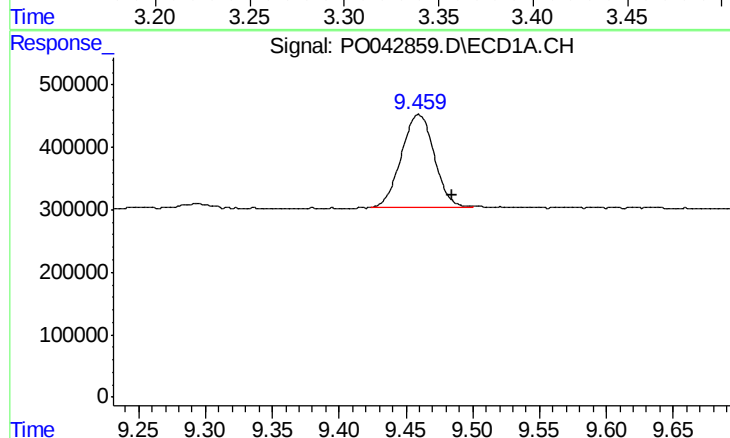

#2 Decachlorobiphenyl

R.T.: 9.459 min
Delta R.T.: -0.025 min
Response: 2550930
Conc: 10.09 ng/ml m

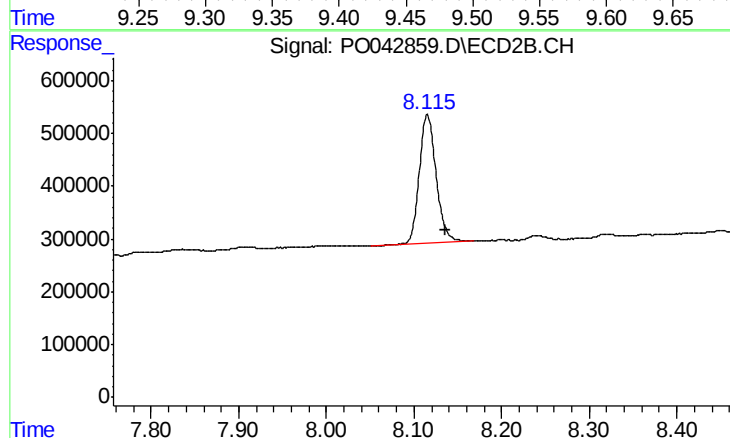

#2 Decachlorobiphenyl

R.T.: 8.115 min
Delta R.T.: -0.021 min
Response: 3230178
Conc: 8.38 ng/ml