

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030920\
 Data File : P0067007.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Mar 2020 9:30
 Operator : DD\AJ
 Sample : L1366-11 2X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 03-05-K

Manual Integrations
 APPROVED

Sohil
 3/11/2020 10:59:18 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 12:16:48 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 04 13:48:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.117	3.400	529648	483210	9.936	10.422
2) SA Decachlor...	9.576	8.275	526942	481891	9.571m	9.321m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030920\
Data File : P0067007.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Mar 2020 9:30
Operator : DD\AJ
Sample : L1366-11 2X
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
03-05-K


Manual Integrations
APPROVED

Sohil
3/11/2020 10:59:18 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 12:16:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 04 13:48:03 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

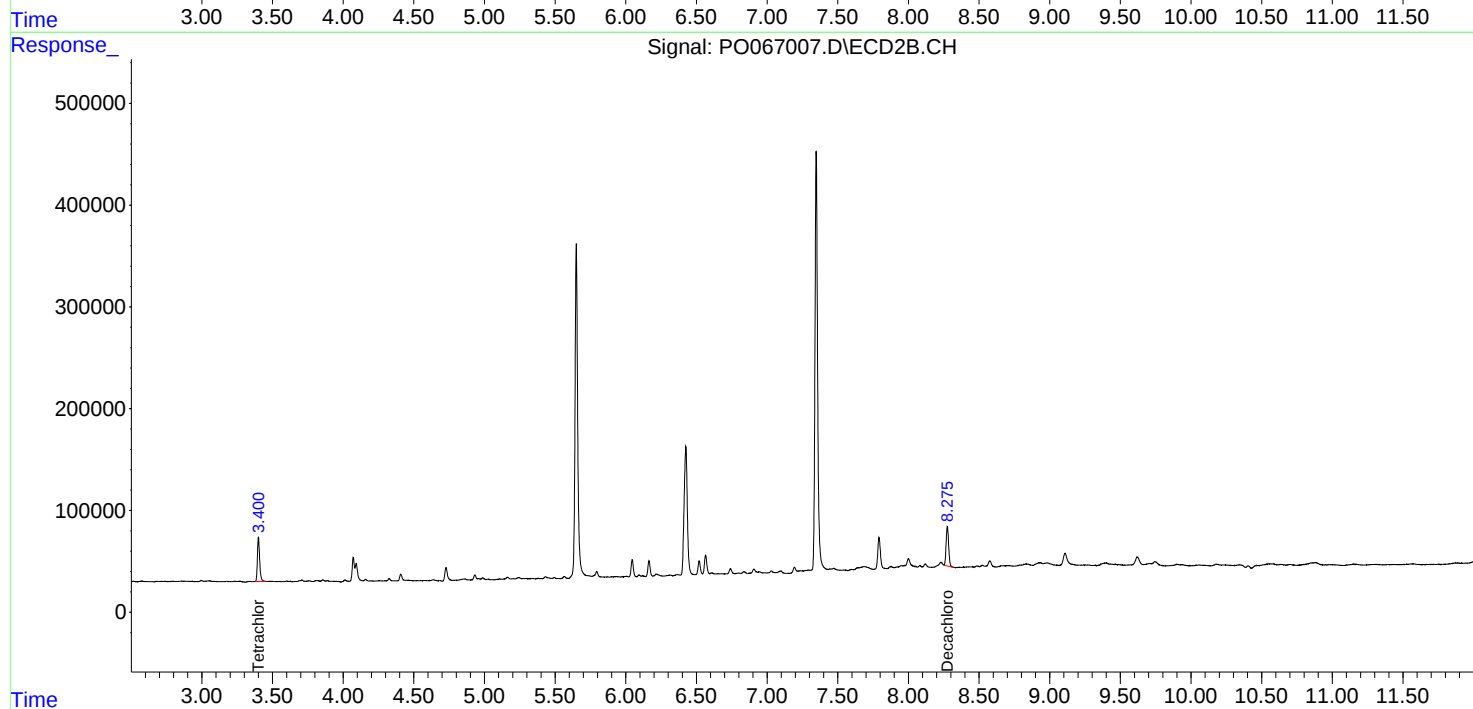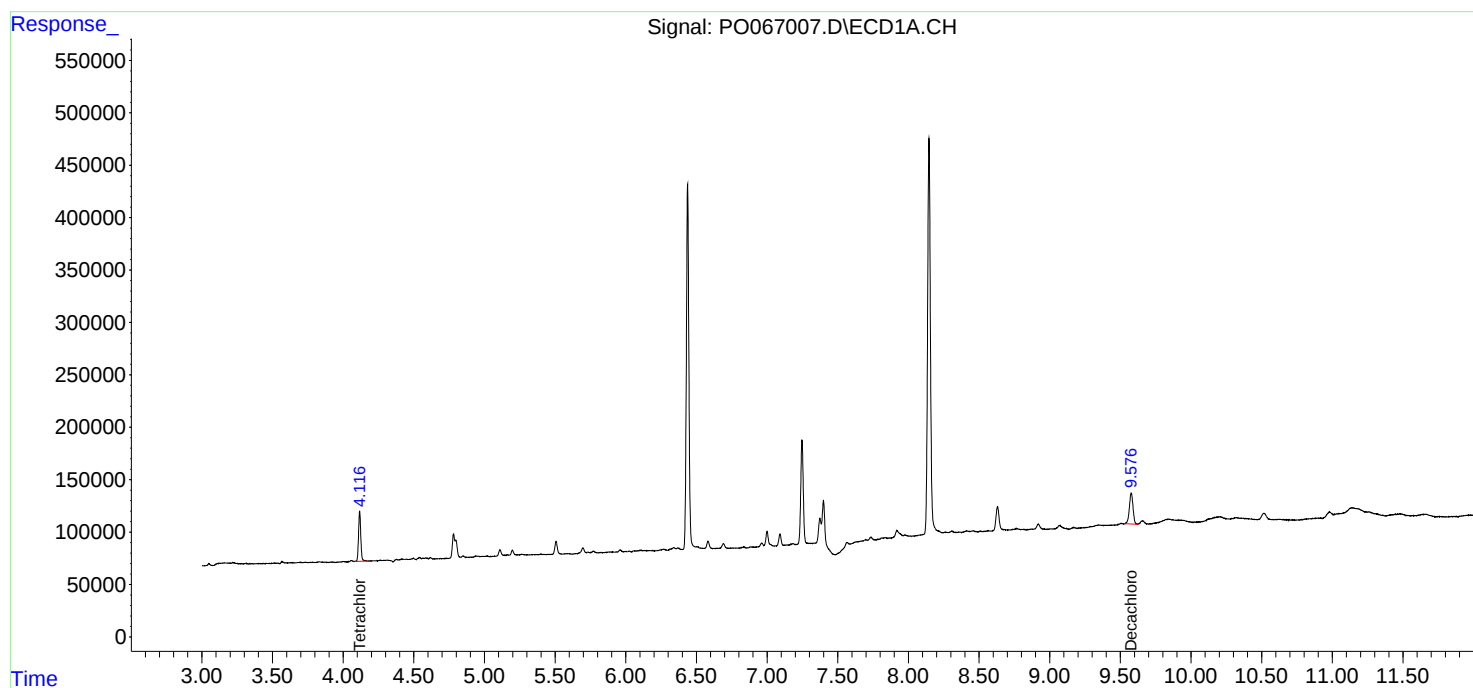

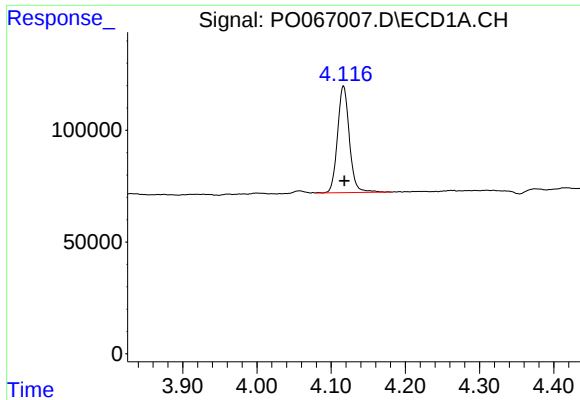


#1 Tetrachloro-m-xylene

R.T.: 4.117 min
Delta R.T.: -0.001 min
Response: 529648
Conc: 9.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
03-05-K


Manual Integrations
APPROVED

Sohil
3/11/2020 10:59:18 AM

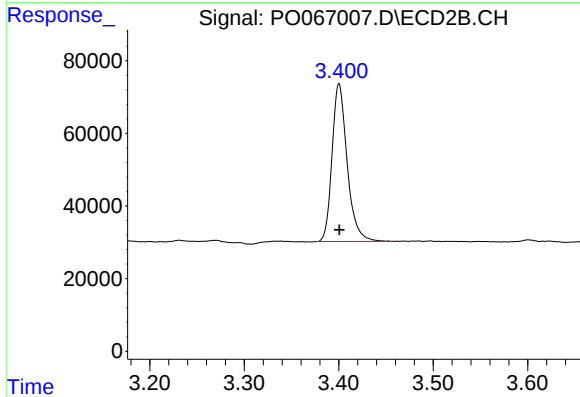


#1 Tetrachloro-m-xylene

R.T.: 3.400 min
Delta R.T.: 0.000 min
Response: 483210
Conc: 10.42 ng/ml

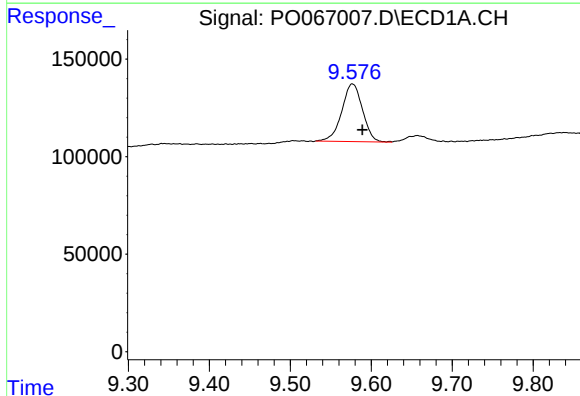

#2 Decachlorobiphenyl

R.T.: 9.576 min
Delta R.T.: -0.013 min
Response: 526942
Conc: 9.57 ng/ml m

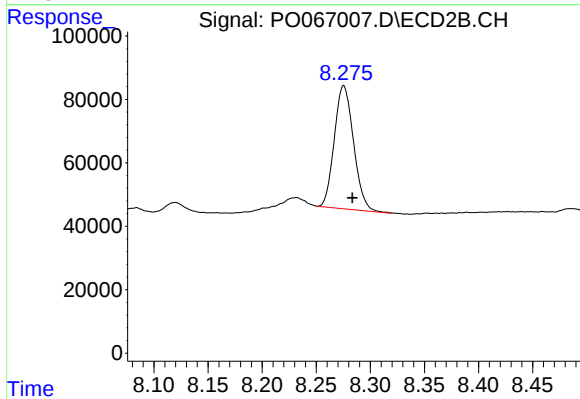

#2 Decachlorobiphenyl

R.T.: 8.275 min
Delta R.T.: -0.008 min
Response: 481891
Conc: 9.32 ng/ml m