

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030920\
 Data File : P0067012.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Mar 2020 10:54
 Operator : DD\AJ
 Sample : L1366-07 5X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 03-05-G

Manual Integrations
 APPROVED

Sohil
 3/11/2020 10:59:23 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 12:18:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 04 13:48:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.115	3.401	193397	176115	3.628m	3.799
2) SA Decachlor...	9.576	8.274	202867	184653	3.685m	3.572m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030920\
Data File : P0067012.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Mar 2020 10:54
Operator : DD\AJ
Sample : L1366-07 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
03-05-G


Manual Integrations
APPROVED

Sohil
3/11/2020 10:59:23 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 12:18:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 04 13:48:03 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

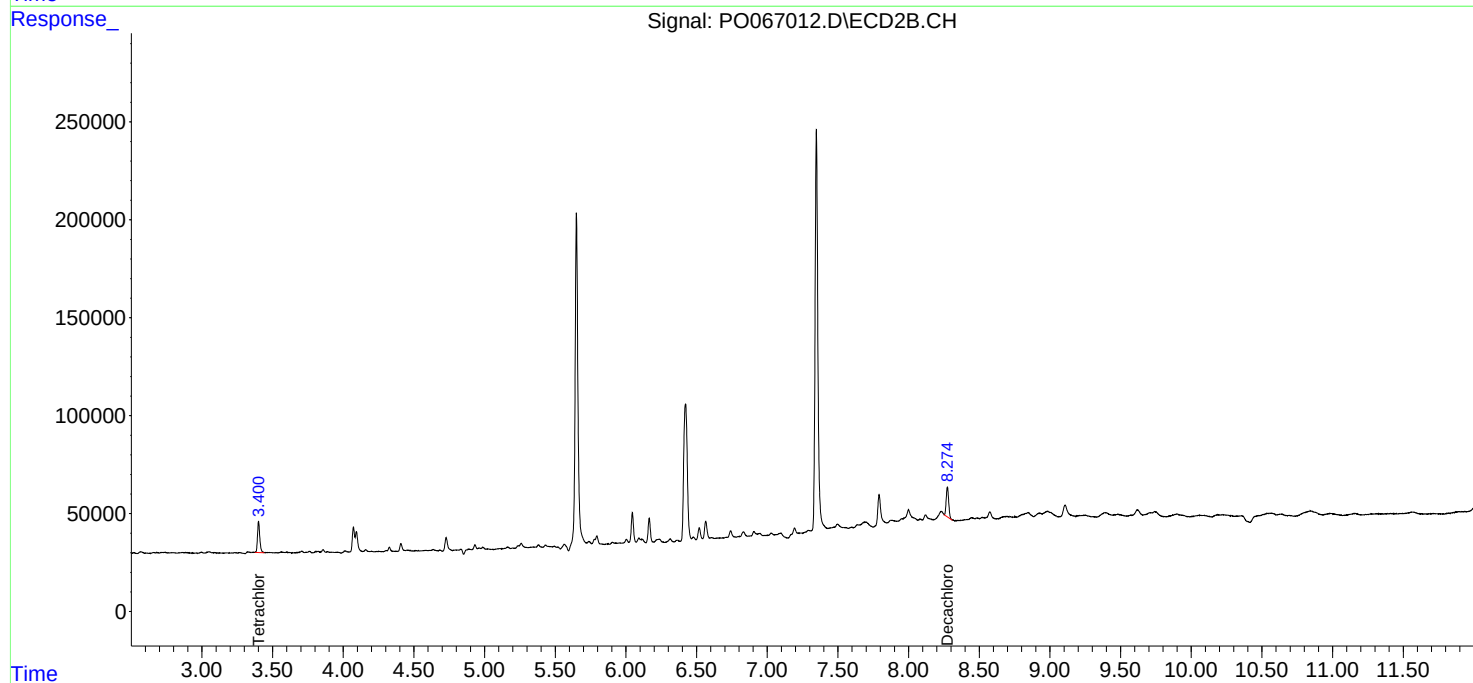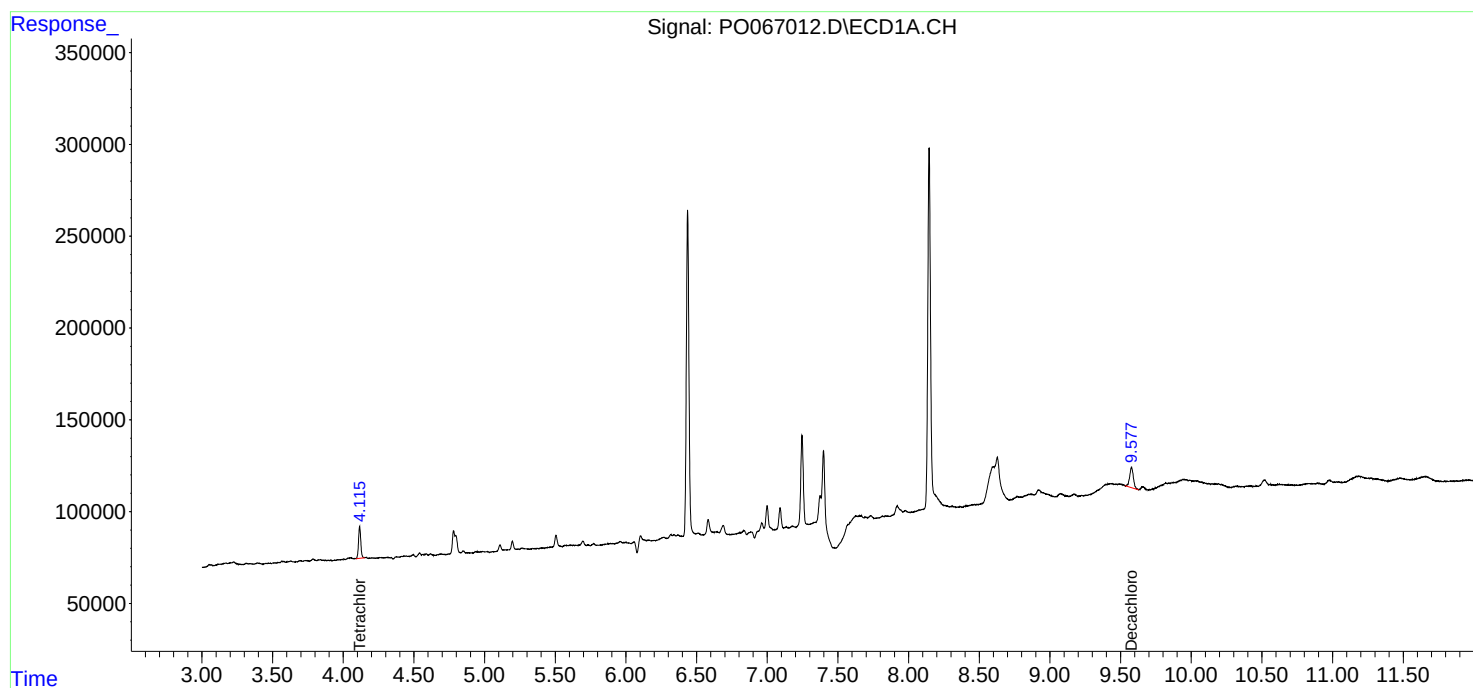

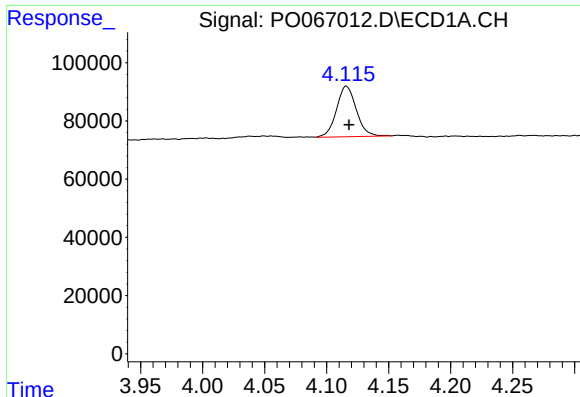


#1 Tetrachloro-m-xylene

R.T.: 4.115 min
Delta R.T.: -0.003 min
Response: 193397
Conc: 3.63 ng/ml m

Instrument :
ECD_O
ClientSampleId :
03-05-G


Manual Integrations
APPROVED

Sohil
3/11/2020 10:59:23 AM

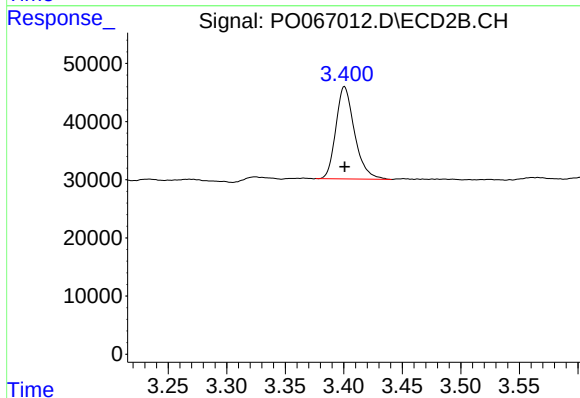


#1 Tetrachloro-m-xylene

R.T.: 3.401 min
Delta R.T.: 0.000 min
Response: 176115
Conc: 3.80 ng/ml

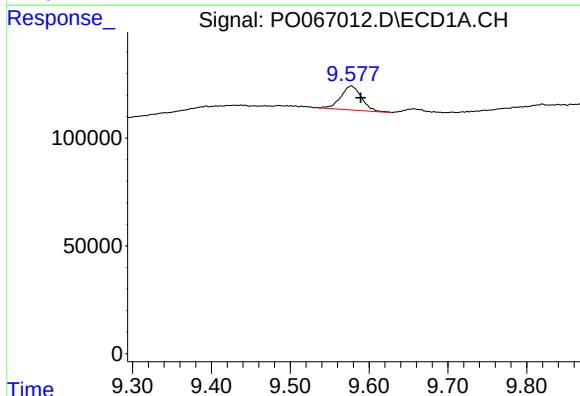

#2 Decachlorobiphenyl

R.T.: 9.576 min
Delta R.T.: -0.013 min
Response: 202867
Conc: 3.68 ng/ml m

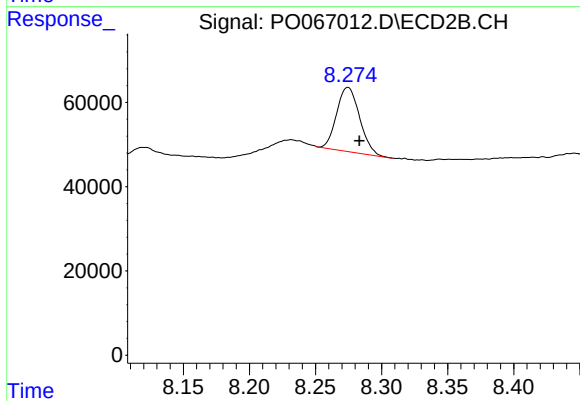

#2 Decachlorobiphenyl

R.T.: 8.274 min
Delta R.T.: -0.009 min
Response: 184653
Conc: 3.57 ng/ml m