

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030920\
 Data File : P0067016.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Mar 2020 12:10
 Operator : DD\AJ
 Sample : L1803-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 N38129

Manual Integrations
 APPROVED

Sohil
 3/11/2020 10:59:28 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 14:49:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 04 13:48:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.117	3.403	947491	849154	17.774	18.316
2) SA Decachlor...	9.574	8.274	599740	607550	10.893m	11.751m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030920\
Data File : P0067016.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Mar 2020 12:10
Operator : DD\AJ
Sample : L1803-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
N38129


Manual Integrations
APPROVED

Sohil
3/11/2020 10:59:28 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 14:49:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 04 13:48:03 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

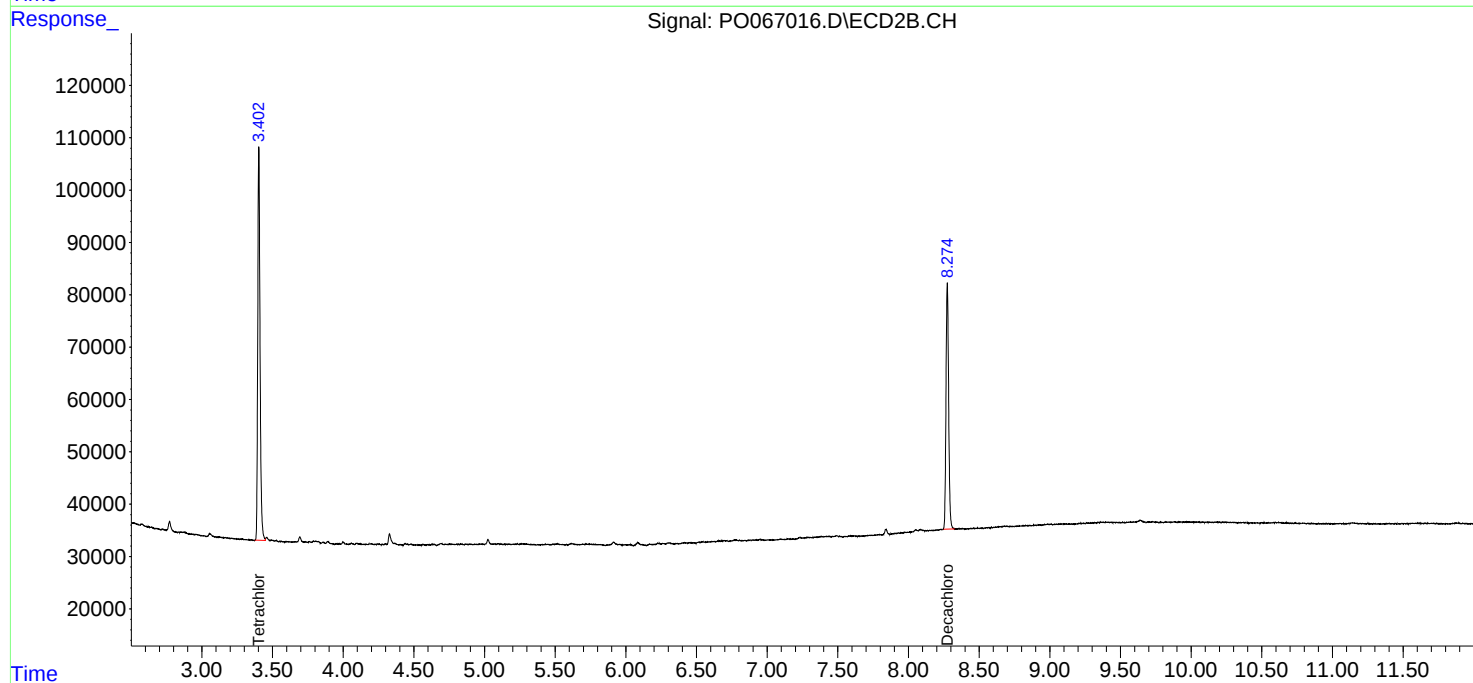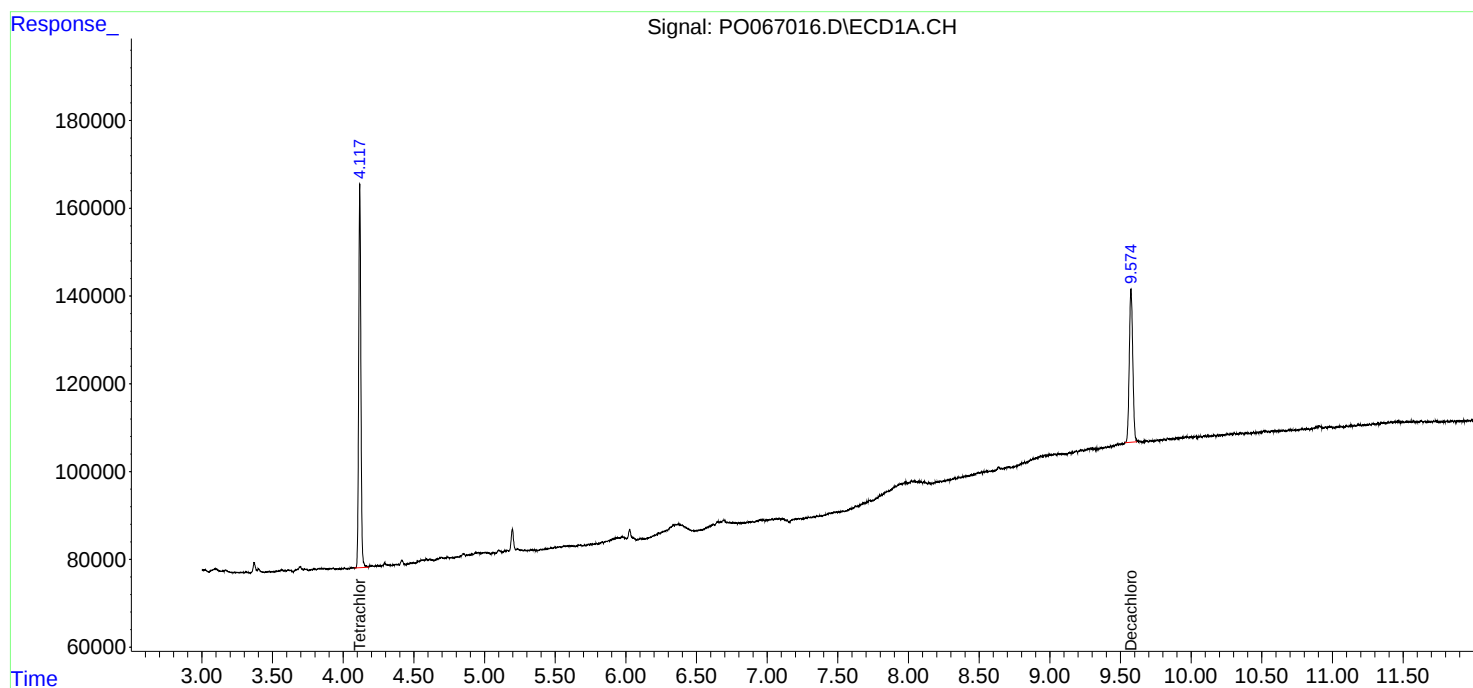

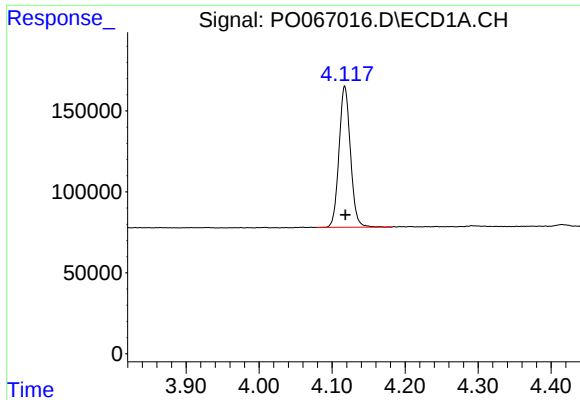


#1 Tetrachloro-m-xylene

R.T.: 4.117 min
Delta R.T.: 0.000 min
Response: 947491
Conc: 17.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
N38129


Manual Integrations
APPROVED

Sohil
3/11/2020 10:59:28 AM

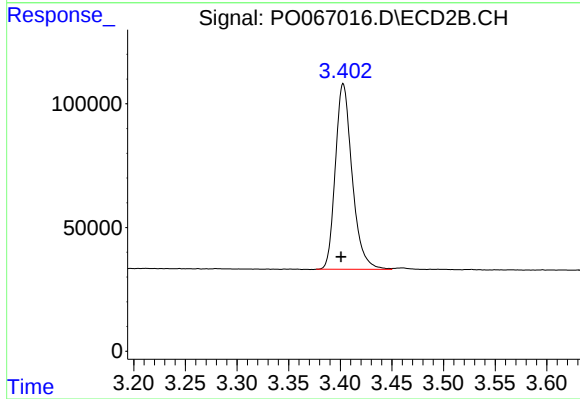


#1 Tetrachloro-m-xylene

R.T.: 3.403 min
Delta R.T.: 0.002 min
Response: 849154
Conc: 18.32 ng/ml

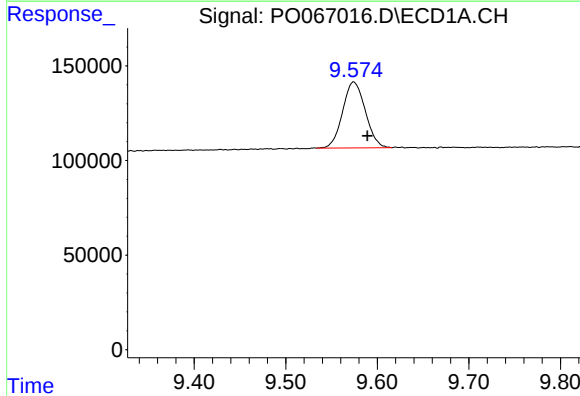

#2 Decachlorobiphenyl

R.T.: 9.574 min
Delta R.T.: -0.015 min
Response: 599740
Conc: 10.89 ng/ml m

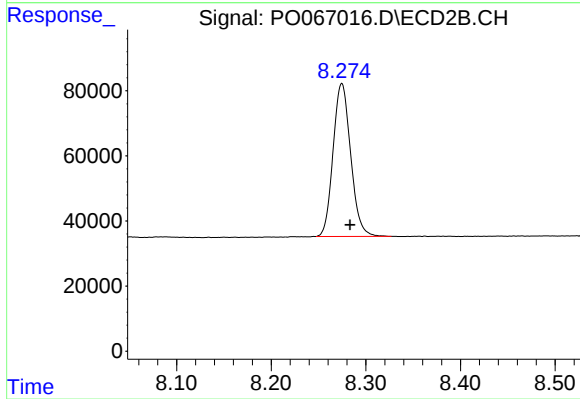

#2 Decachlorobiphenyl

R.T.: 8.274 min
Delta R.T.: -0.009 min
Response: 607550
Conc: 11.75 ng/ml m