

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030920\
 Data File : P0067037.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Mar 2020 23:02
 Operator : DD\AJ
 Sample : L1841-37 100X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WALL-FLASHING-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 00:34:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 04 13:48:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.116	3.400	12107	9306	0.227	0.201
2)	SA Decachlor...	9.592	8.275	13125	11440	0.238	0.221

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030920\
Data File : P0067037.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Mar 2020 23:02
Operator : DD\AJ
Sample : L1841-37 100X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
WALL-FLASHING-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 00:34:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 04 13:48:03 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

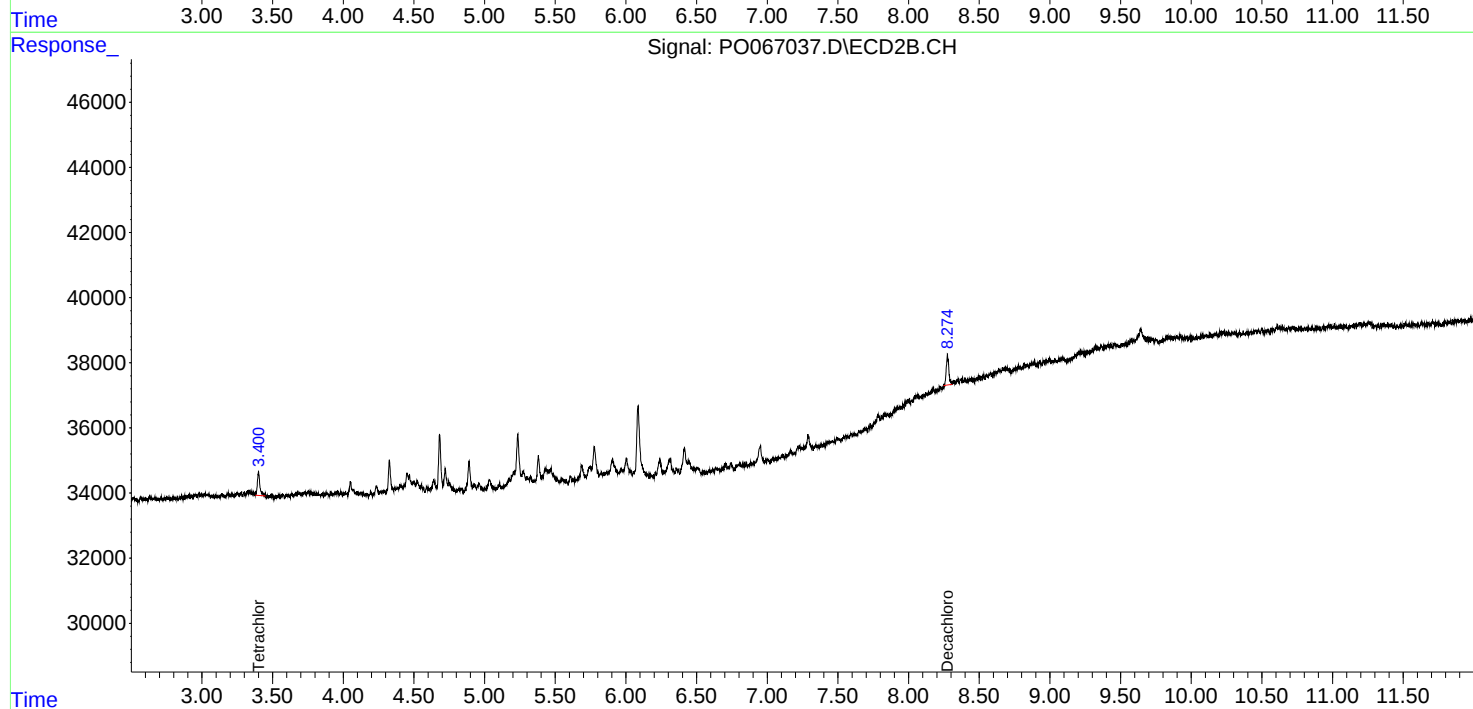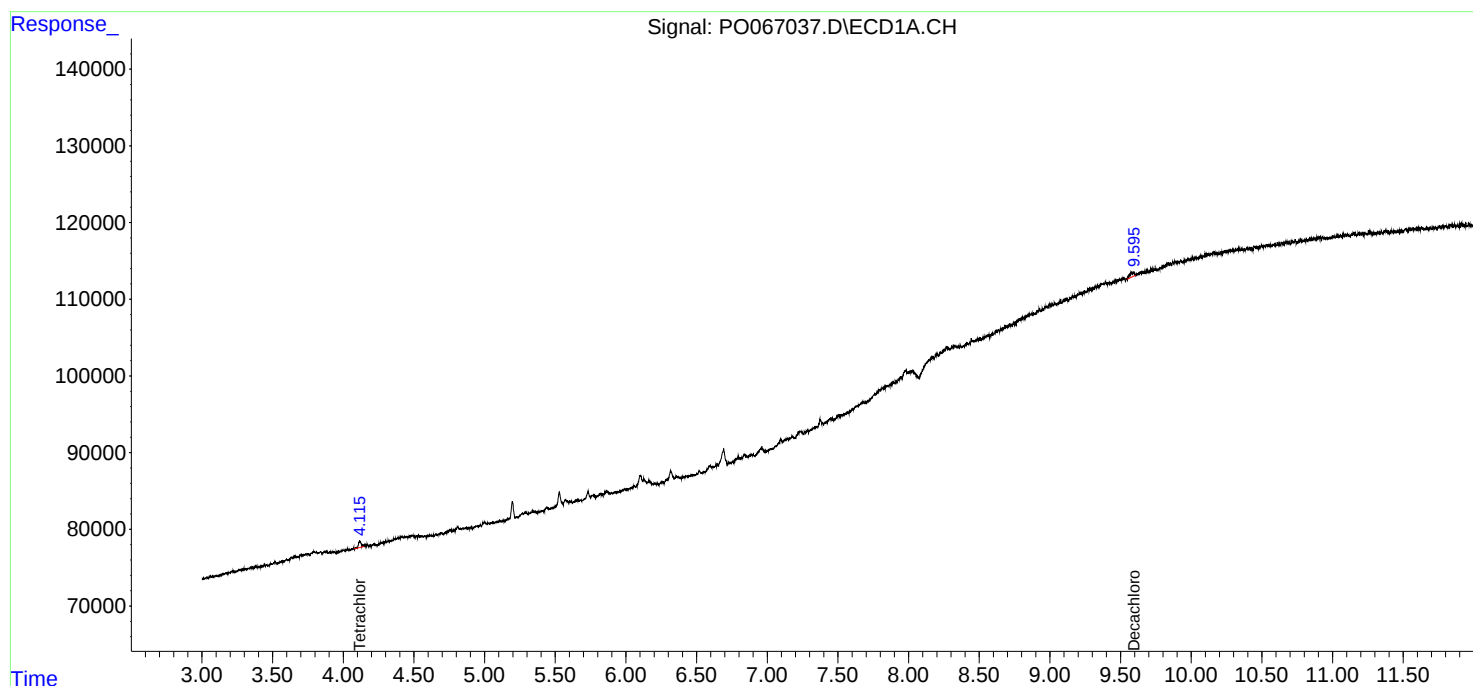


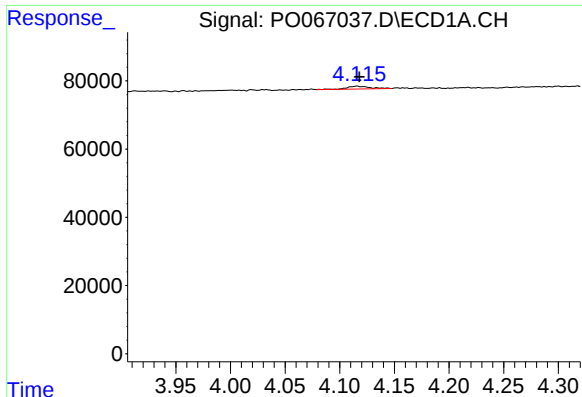

#1 Tetrachloro-m-xylene


R.T.: 4.116 min
Delta R.T.: -0.002 min
Response: 12107
Conc: 0.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
WALL-FLASHING-A

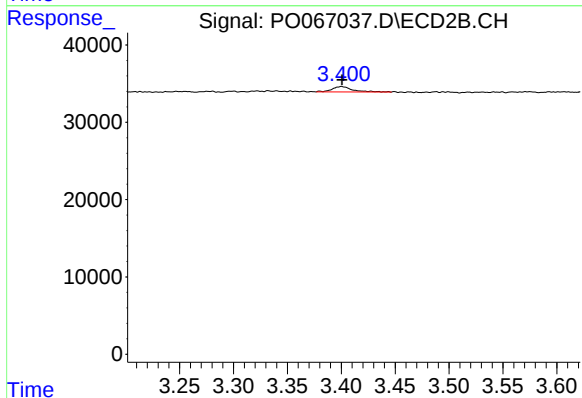


#1 Tetrachloro-m-xylene

R.T.: 3.400 min
Delta R.T.: 0.000 min
Response: 9306
Conc: 0.20 ng/ml

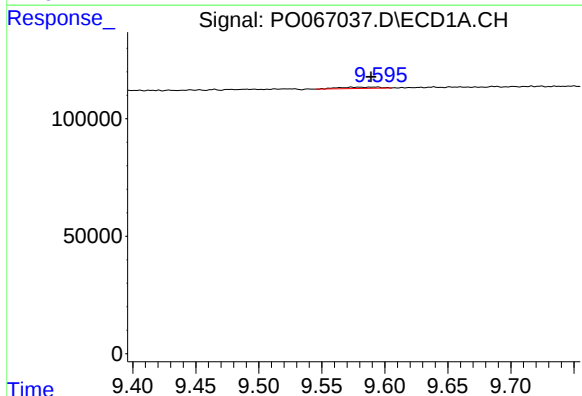

#2 Decachlorobiphenyl

R.T.: 9.592 min
Delta R.T.: 0.003 min
Response: 13125
Conc: 0.24 ng/ml

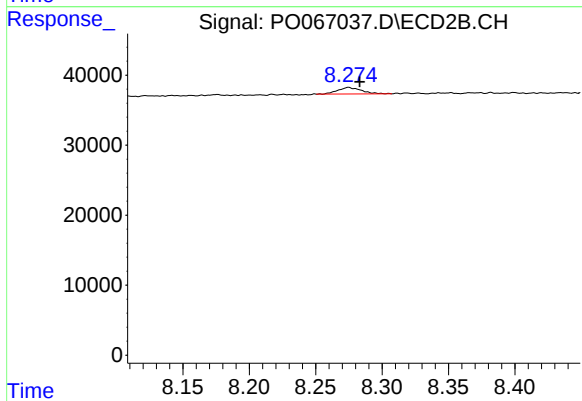

#2 Decachlorobiphenyl

R.T.: 8.275 min
Delta R.T.: -0.008 min
Response: 11440
Conc: 0.22 ng/ml