

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031020\
 Data File : P0067072.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Mar 2020 17:46
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 01:46:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 04 13:48:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.115	3.400	1195849	1008623	22.433	21.755
2)	SA Decachlor...	9.578	8.276	966924	959220	17.562	18.553

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031020\
Data File : P0067072.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Mar 2020 17:46
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 01:46:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 04 13:48:03 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

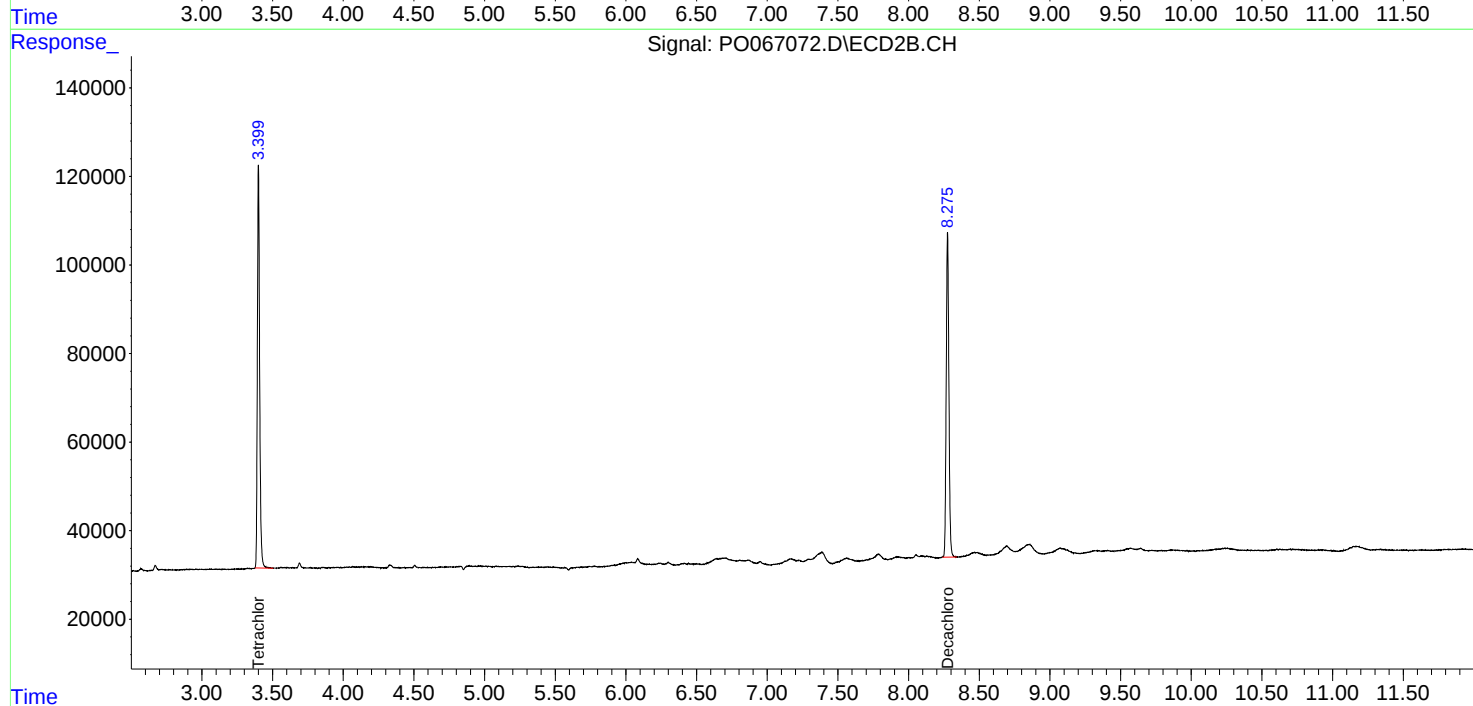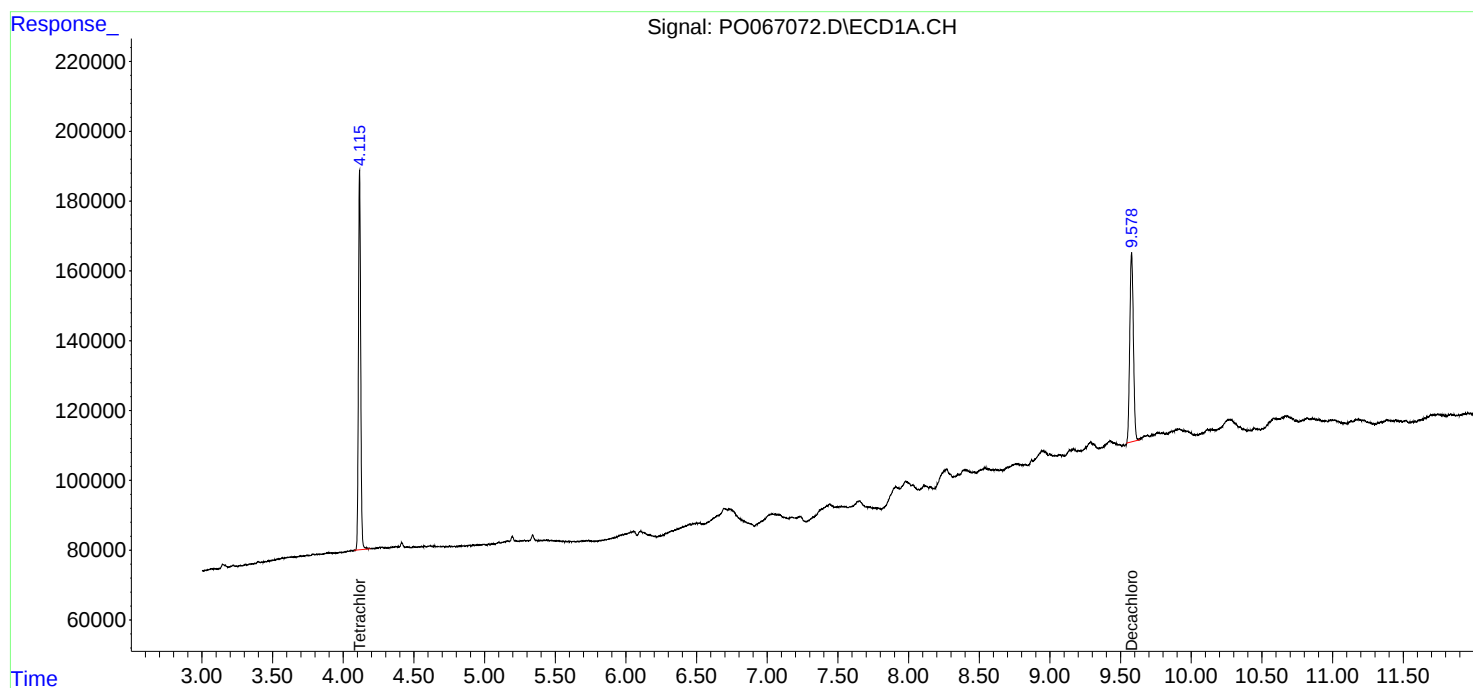


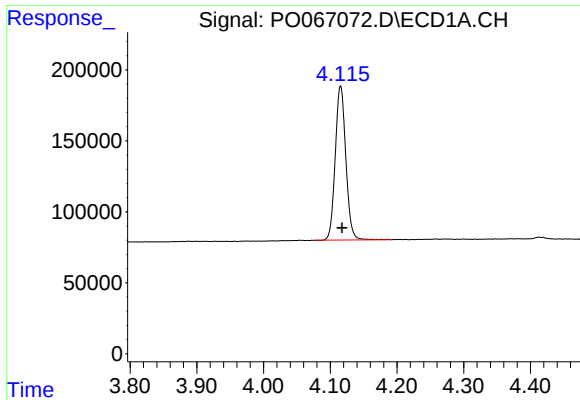

#1 Tetrachloro-m-xylene


R.T.: 4.115 min
Delta R.T.: -0.003 min
Response: 1195849
Conc: 22.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

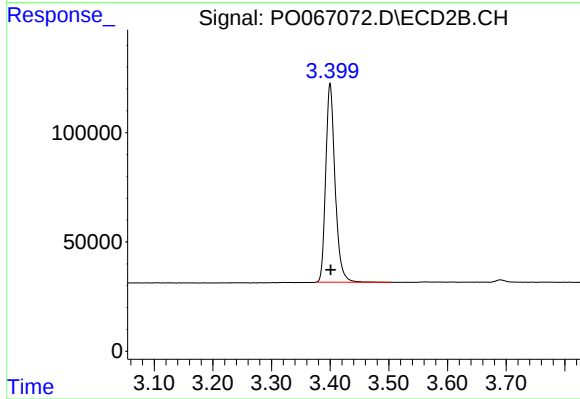


#1 Tetrachloro-m-xylene

R.T.: 3.400 min
Delta R.T.: 0.000 min
Response: 1008623
Conc: 21.76 ng/ml

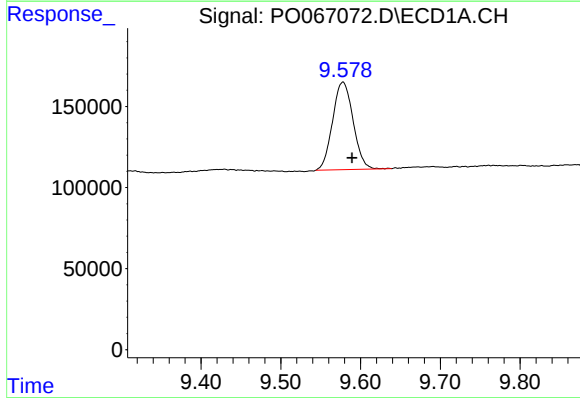

#2 Decachlorobiphenyl

R.T.: 9.578 min
Delta R.T.: -0.011 min
Response: 966924
Conc: 17.56 ng/ml

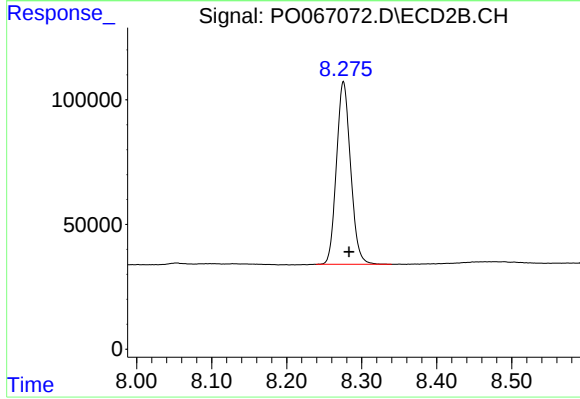

#2 Decachlorobiphenyl

R.T.: 8.276 min
Delta R.T.: -0.008 min
Response: 959220
Conc: 18.55 ng/ml