

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031020\
 Data File : P0067083.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Mar 2020 20:56
 Operator : DD\AJ
 Sample : L1852-19
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-3-D

Manual Integrations
 APPROVED

Sohil
 3/16/2020 9:13:57 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 01:52:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 04 13:48:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.115	3.399	1075250	898779	20.170	19.386
2) SA Decachlor...	9.576	8.275	902199	849695	16.386m	16.435

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031020\
Data File : P0067083.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Mar 2020 20:56
Operator : DD\AJ
Sample : L1852-19
Misc :
ALS Vial : 40 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-3-D


Manual Integrations
APPROVED

Sohil
3/16/2020 9:13:57 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 01:52:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 04 13:48:03 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

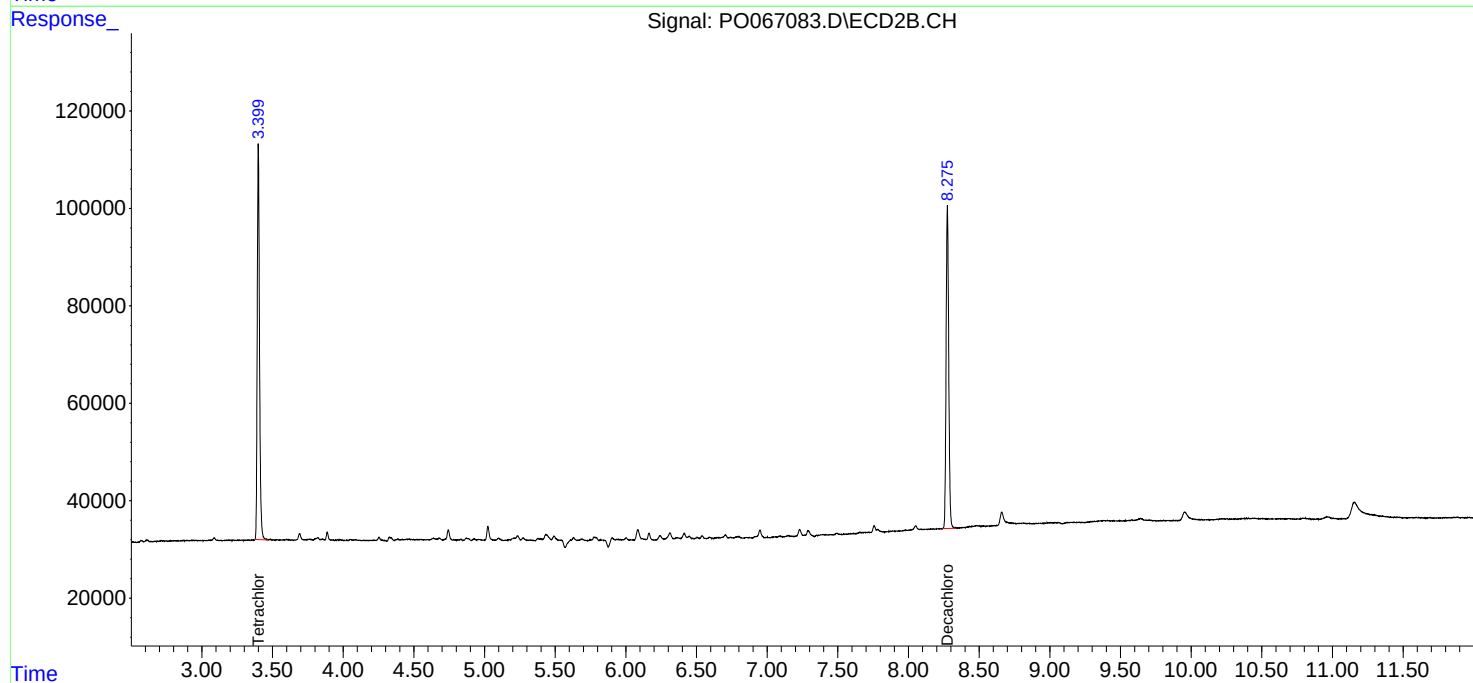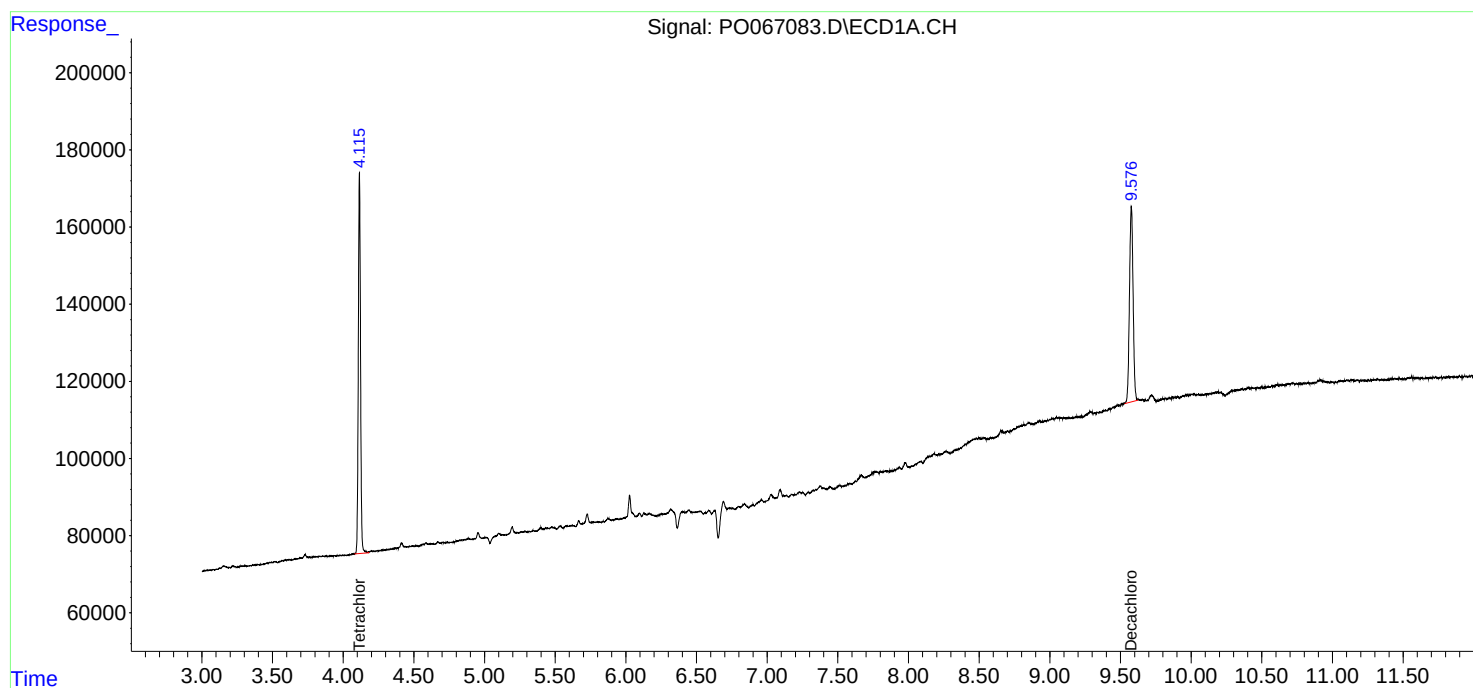

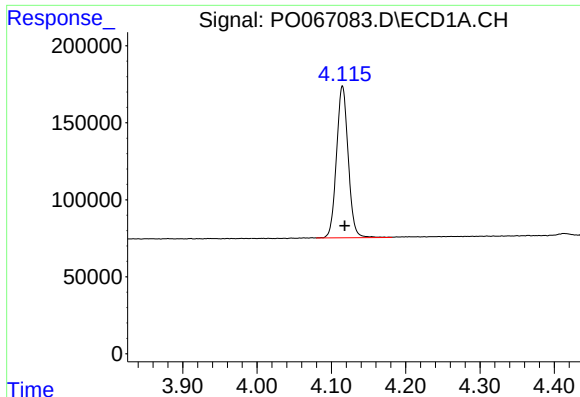


#1 Tetrachloro-m-xylene

R.T.: 4.115 min
Delta R.T.: -0.003 min
Response: 1075250
Conc: 20.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3-D


Manual Integrations
APPROVED

Sohil
3/16/2020 9:13:57 AM

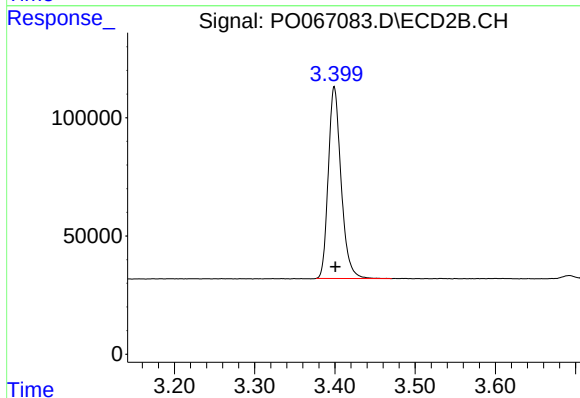


#1 Tetrachloro-m-xylene

R.T.: 3.399 min
Delta R.T.: -0.001 min
Response: 898779
Conc: 19.39 ng/ml

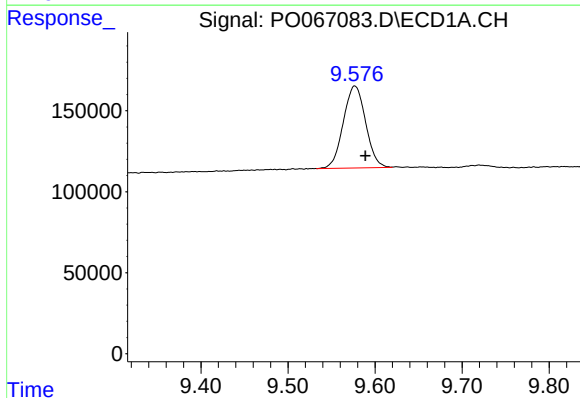

#2 Decachlorobiphenyl

R.T.: 9.576 min
Delta R.T.: -0.013 min
Response: 902199
Conc: 16.39 ng/ml m

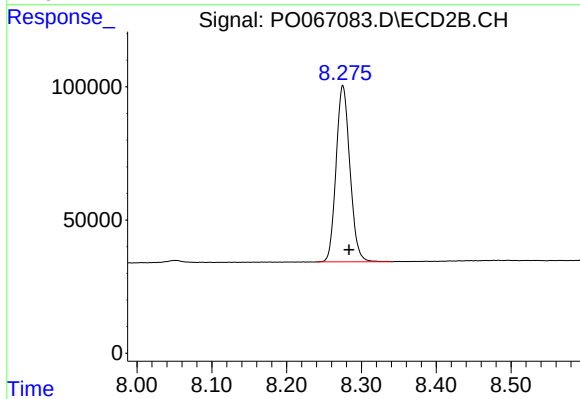

#2 Decachlorobiphenyl

R.T.: 8.275 min
Delta R.T.: -0.008 min
Response: 849695
Conc: 16.43 ng/ml