

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031119\
Data File : P0054321.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Mar 2019 19:21
Operator : SM/SJ
Sample : K1785-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SD3-0.0-0.5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 00:55:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031119.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 11 14:40:27 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.023	3.112	59239162	4692381	17.237	16.755
2) SA Decachlor...	9.332	7.673	6099526	1359747	4.842	4.833

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031119\
Data File : P0054321.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Mar 2019 19:21
Operator : SM/SJ
Sample : K1785-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SD3-0.0-0.5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 00:55:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031119.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 11 14:40:27 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

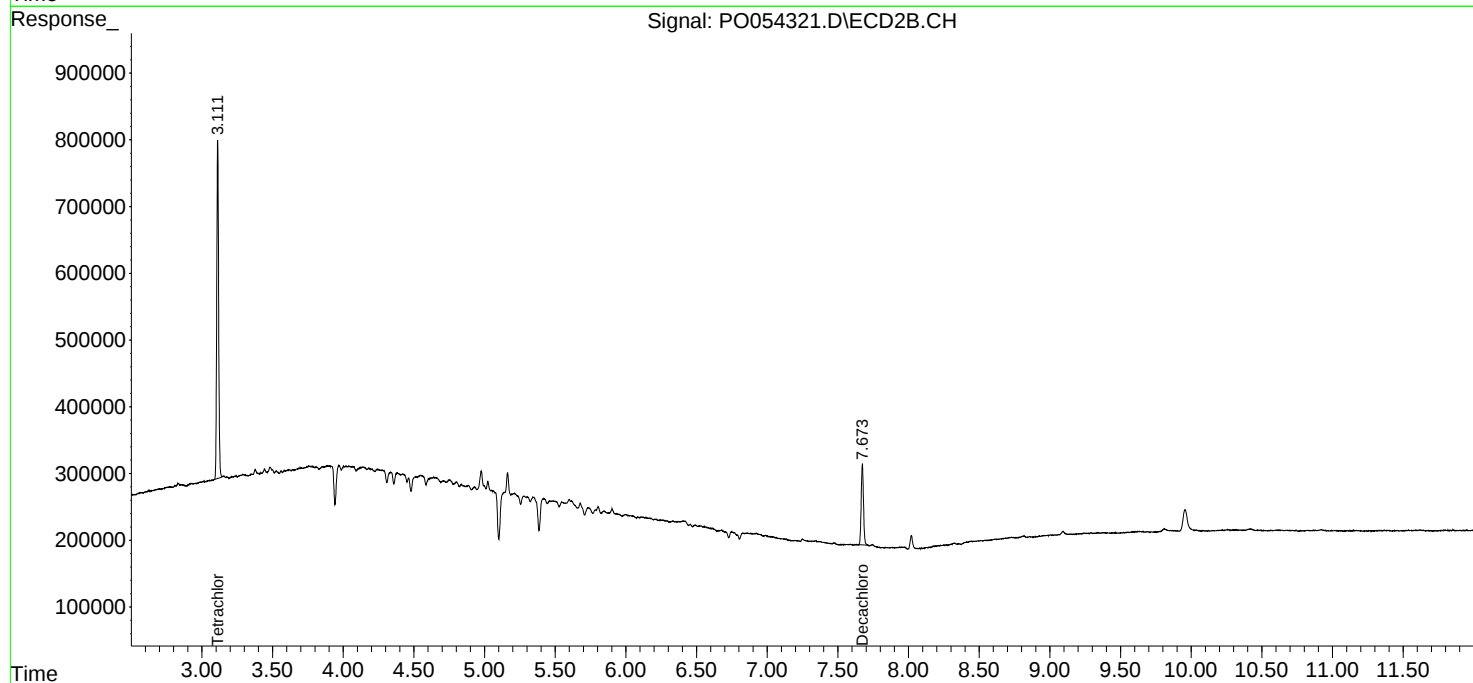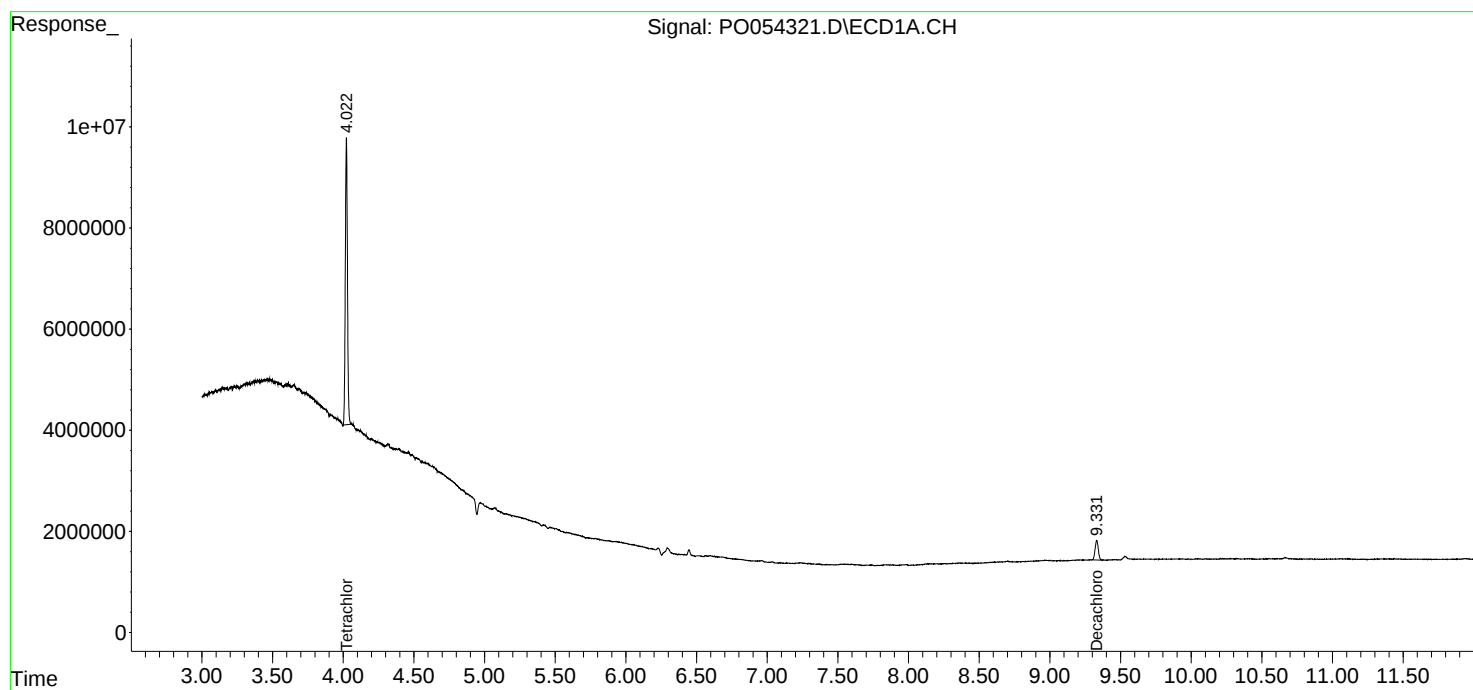


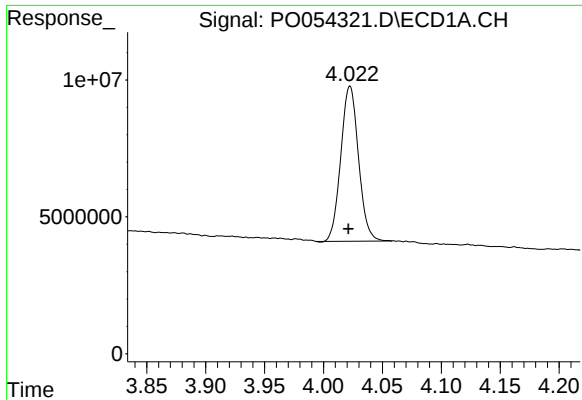

#1 Tetrachloro-m-xylene


R.T.: 4.023 min
Delta R.T.: 0.002 min
Response: 59239162
Conc: 17.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
SD3-0.0-0.5

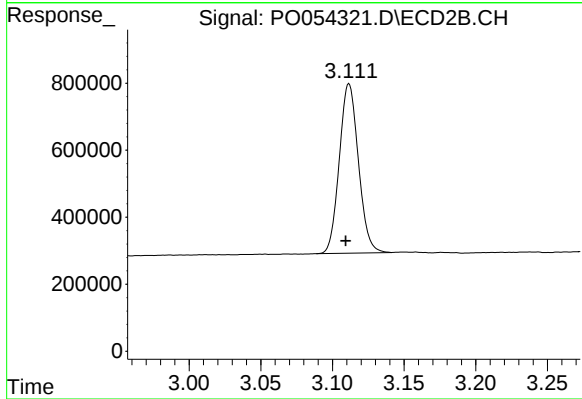


#1 Tetrachloro-m-xylene

R.T.: 3.112 min
Delta R.T.: 0.002 min
Response: 4692381
Conc: 16.76 ng/ml

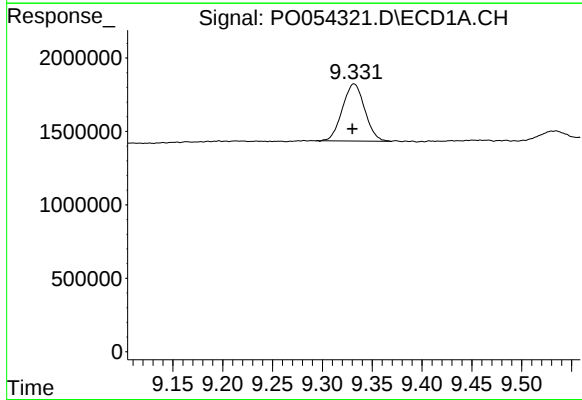

#2 Decachlorobiphenyl

R.T.: 9.332 min
Delta R.T.: 0.001 min
Response: 6099526
Conc: 4.84 ng/ml

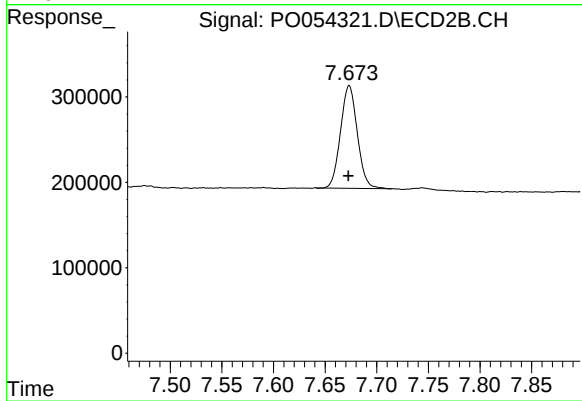

#2 Decachlorobiphenyl

R.T.: 7.673 min
Delta R.T.: 0.000 min
Response: 1359747
Conc: 4.83 ng/ml