

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031119\
 Data File : P0054324.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Mar 2019 20:12
 Operator : SM/SJ
 Sample : K1785-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 2019-03-05-DUP-SD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 00:59:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 11 14:40:27 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.022	3.111	78380815	5214131	22.807	18.618
2) SA Decachlor...	9.332	7.673	8168610	1928955	6.485	6.856

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031119\
Data File : P0054324.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Mar 2019 20:12
Operator : SM/SJ
Sample : K1785-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
2019-03-05-DUP-SD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 00:59:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031119.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 11 14:40:27 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

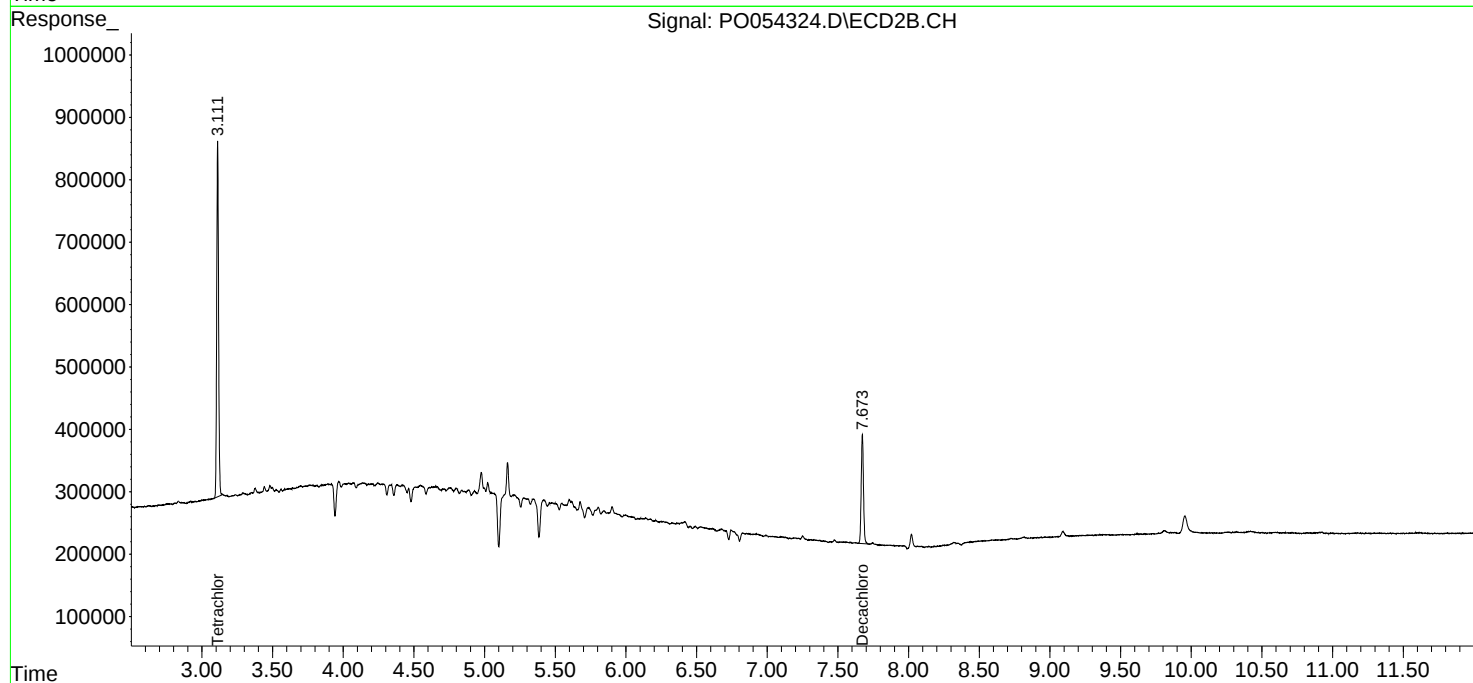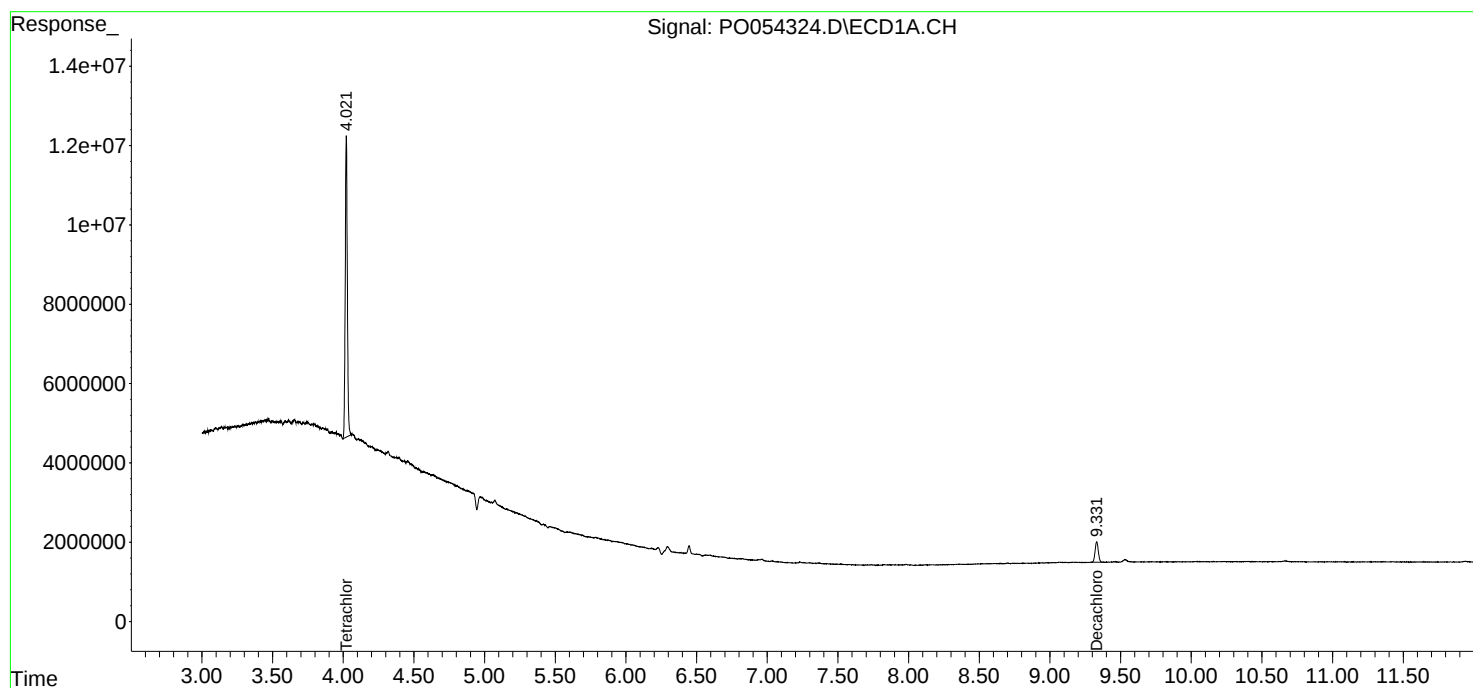


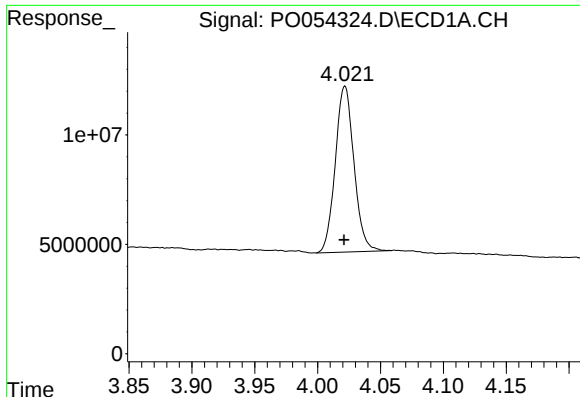

#1 Tetrachloro-m-xylene


R.T.: 4.022 min
Delta R.T.: 0.000 min
Response: 78380815
Conc: 22.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
2019-03-05-DUP-SD

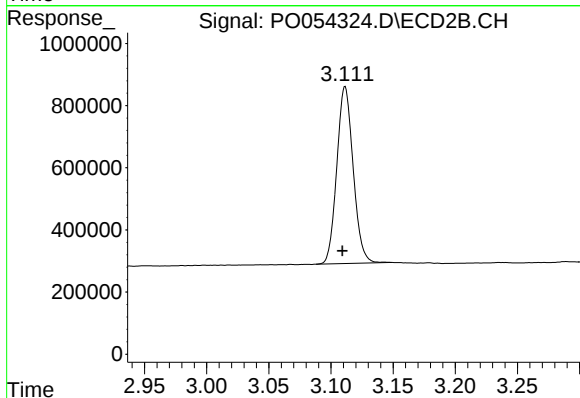


#1 Tetrachloro-m-xylene

R.T.: 3.111 min
Delta R.T.: 0.002 min
Response: 5214131
Conc: 18.62 ng/ml

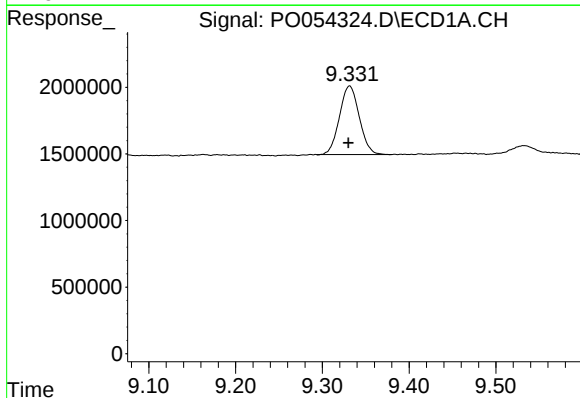

#2 Decachlorobiphenyl

R.T.: 9.332 min
Delta R.T.: 0.001 min
Response: 8168610
Conc: 6.49 ng/ml

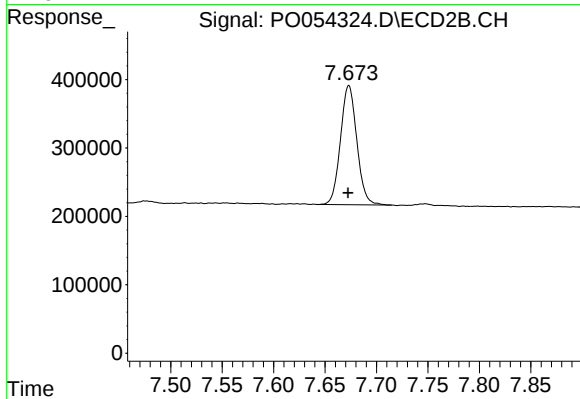

#2 Decachlorobiphenyl

R.T.: 7.673 min
Delta R.T.: 0.000 min
Response: 1928955
Conc: 6.86 ng/ml