

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031119\
 Data File : P0054336.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Mar 2019 23:35
 Operator : SM/SJ
 Sample : K1837-09
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MR-MH-07-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 01:03:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 11 14:40:27 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.021	3.110	90512140	5931633	26.337	21.180
2) SA Decachlor...	9.328	7.671	21700537	5051612	17.228	17.955

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031119\
Data File : P0054336.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Mar 2019 23:35
Operator : SM/SJ
Sample : K1837-09
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MR-MH-07-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 01:03:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031119.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 11 14:40:27 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

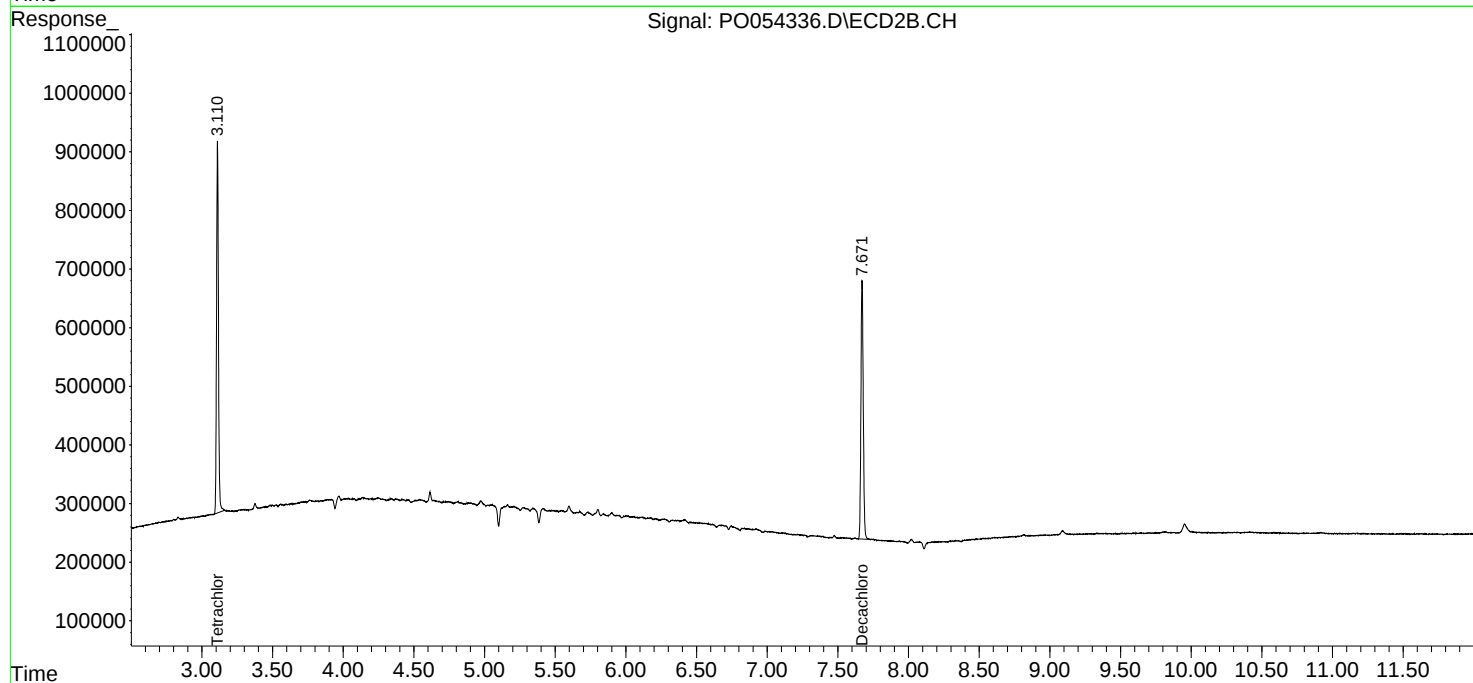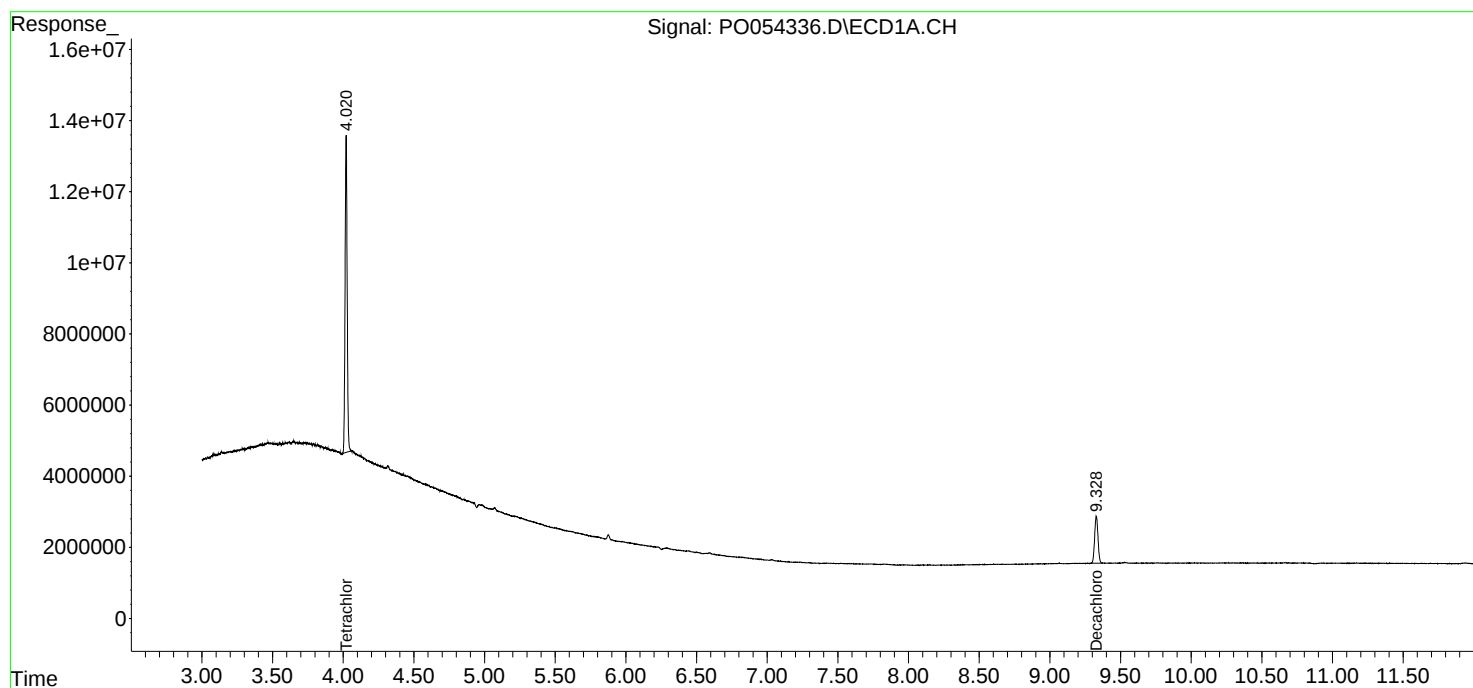


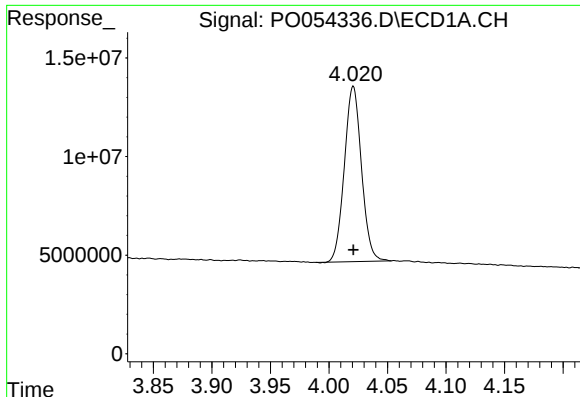

#1 Tetrachloro-m-xylene


R.T.: 4.021 min
Delta R.T.: 0.000 min
Response: 90512140
Conc: 26.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
MR-MH-07-COMP

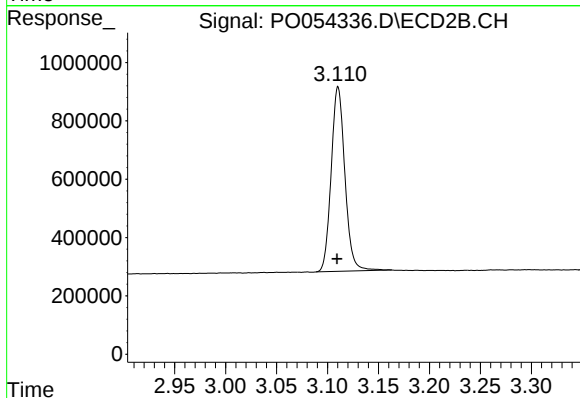


#1 Tetrachloro-m-xylene

R.T.: 3.110 min
Delta R.T.: 0.001 min
Response: 5931633
Conc: 21.18 ng/ml

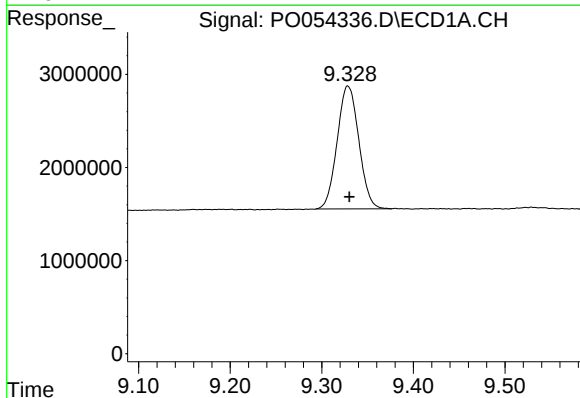

#2 Decachlorobiphenyl

R.T.: 9.328 min
Delta R.T.: -0.002 min
Response: 21700537
Conc: 17.23 ng/ml

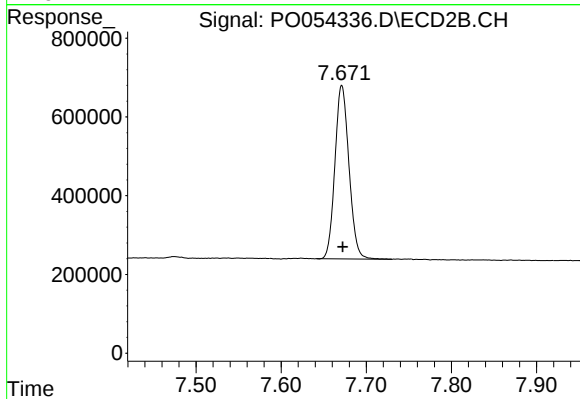

#2 Decachlorobiphenyl

R.T.: 7.671 min
Delta R.T.: -0.001 min
Response: 5051612
Conc: 17.95 ng/ml