

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031120\
 Data File : P0067154.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Mar 2020 3:33
 Operator : DD\AJ
 Sample : L1867-11
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DUP-6

Manual Integrations
 APPROVED

Sohil
 3/16/2020 4:36:39 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 08:21:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 11 15:01:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.112	3.396	703110	843168	22.493	21.548
2) SA Decachlor...	9.572	8.273	509805	739333	14.035	15.184m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031120\
Data File : P0067154.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Mar 2020 3:33
Operator : DD\AJ
Sample : L1867-11
Misc :
ALS Vial : 45 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
DUP-6


Manual Integrations
APPROVED

Sohil
3/16/2020 4:36:39 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 08:21:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031120.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 11 15:01:31 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

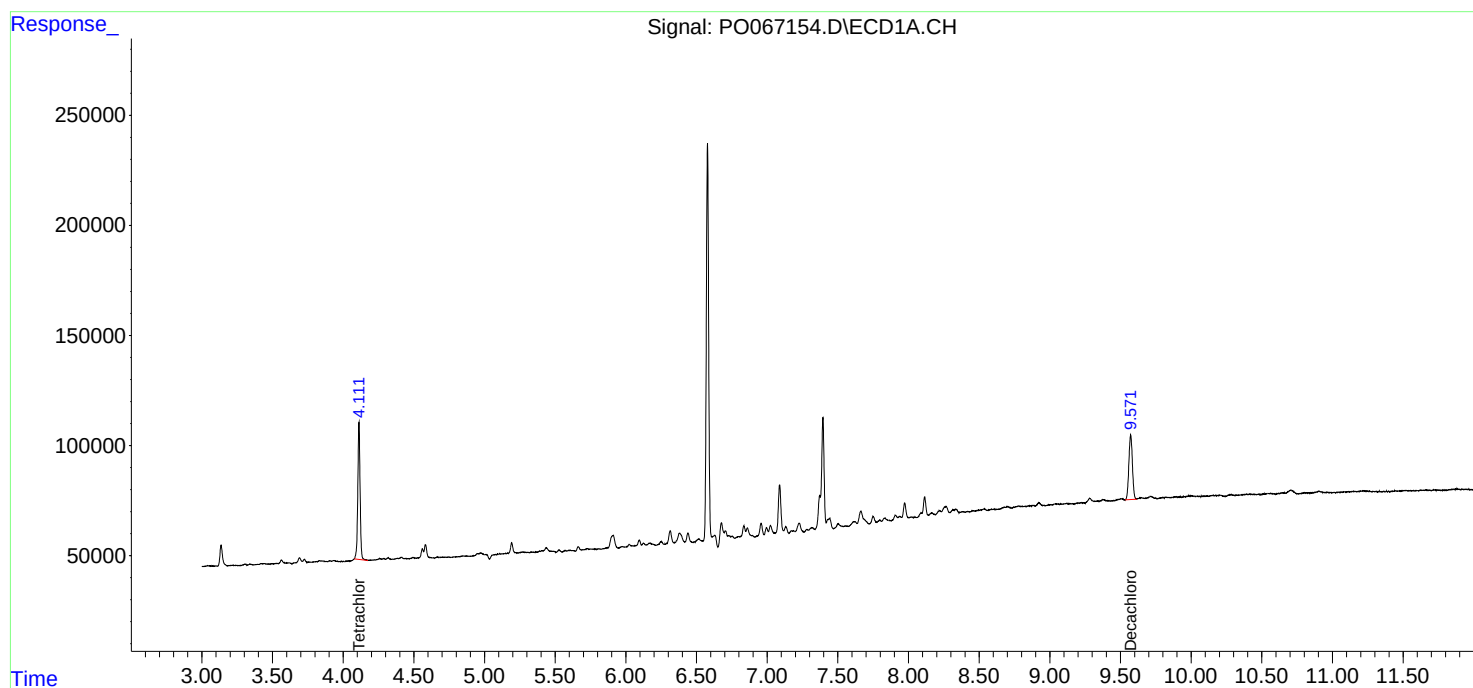

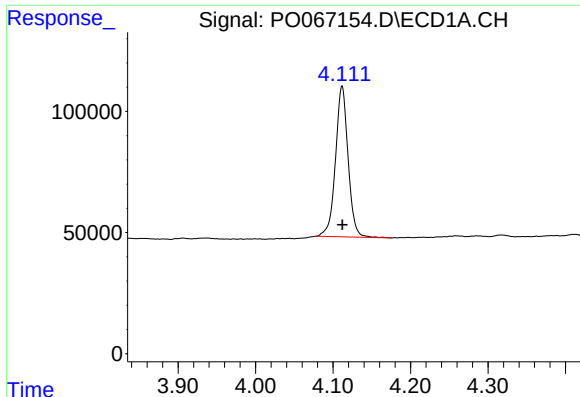


#1 Tetrachloro-m-xylene

R.T.: 4.112 min
Delta R.T.: 0.000 min
Response: 703110
Conc: 22.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
DUP-6


Manual Integrations
APPROVED

Sohil
3/16/2020 4:36:39 PM

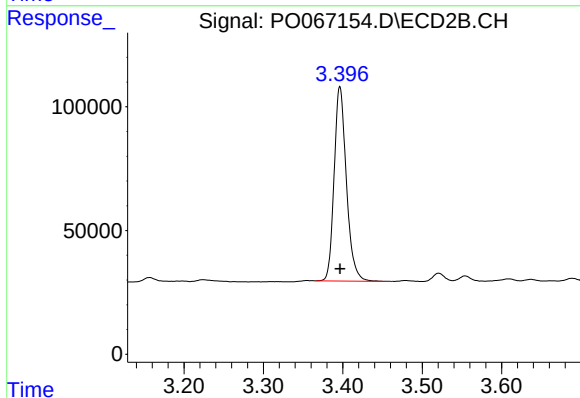


#1 Tetrachloro-m-xylene

R.T.: 3.396 min
Delta R.T.: 0.000 min
Response: 843168
Conc: 21.55 ng/ml

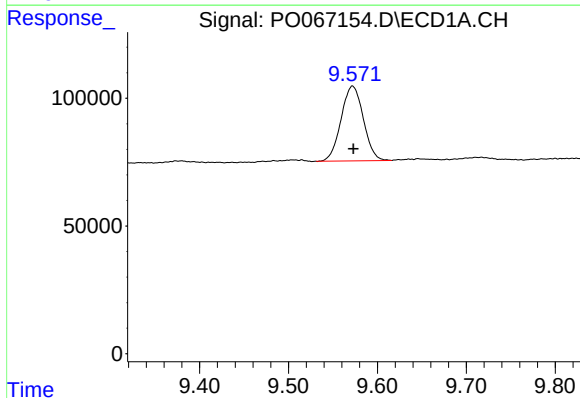

#2 Decachlorobiphenyl

R.T.: 9.572 min
Delta R.T.: -0.001 min
Response: 509805
Conc: 14.03 ng/ml

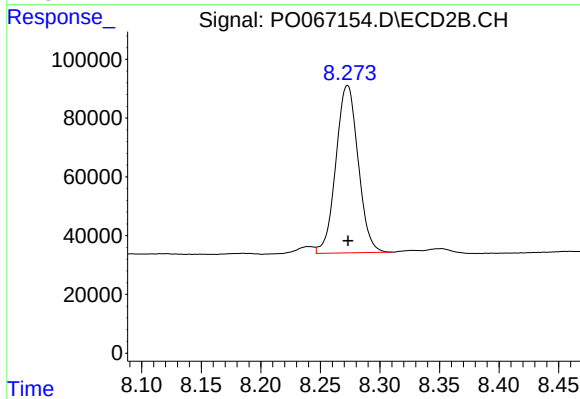

#2 Decachlorobiphenyl

R.T.: 8.273 min
Delta R.T.: 0.000 min
Response: 739333
Conc: 15.18 ng/ml m