

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031219\
Data File : P0054345.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Mar 2019 11:41
Operator : SM/SJ
Sample : K1785-02RE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SD3-0.0-0.5RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 01:10:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031119.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 11 14:40:27 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.017	3.107	48690591	3595563	14.168	12.839
2) SA Decachlor...	9.322	7.667	6577668	1642764	5.222	5.839

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031219\
Data File : P0054345.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Mar 2019 11:41
Operator : SM/SJ
Sample : K1785-02RE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SD3-0.0-0.5RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 01:10:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031119.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 11 14:40:27 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

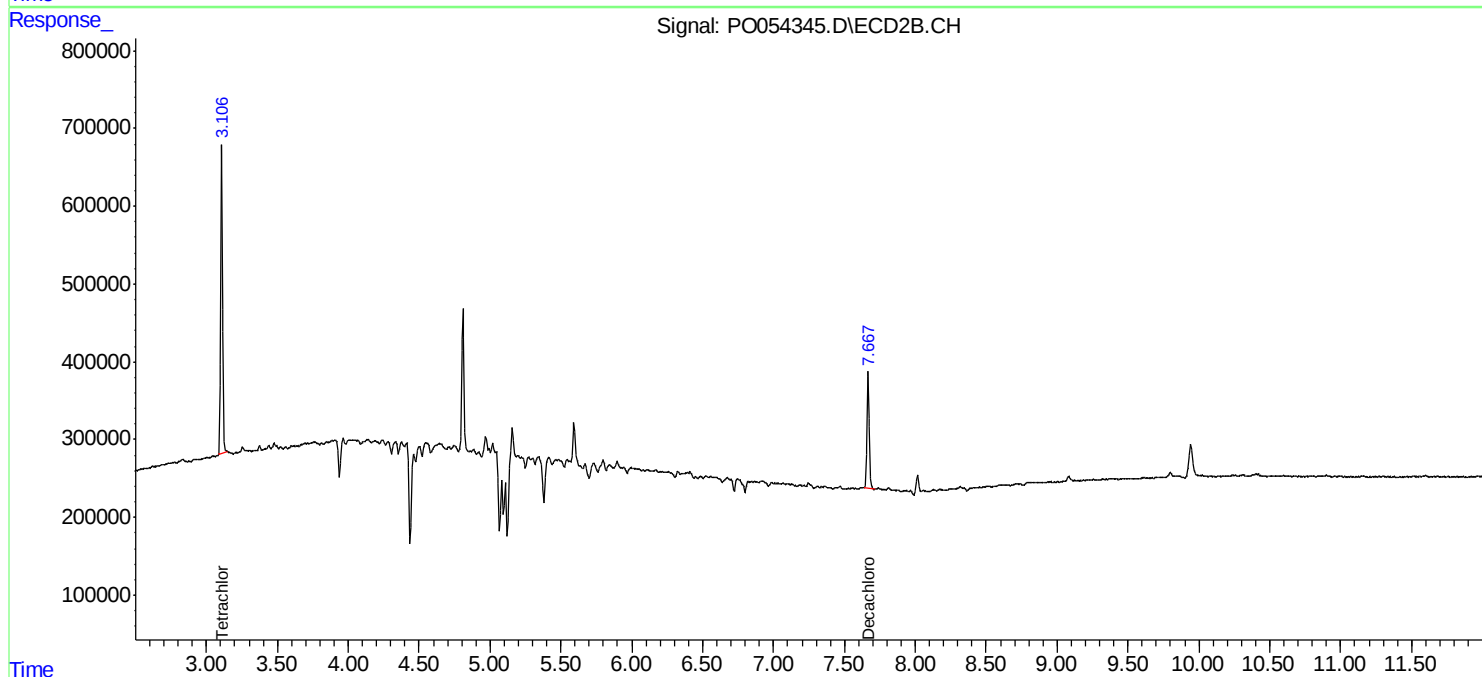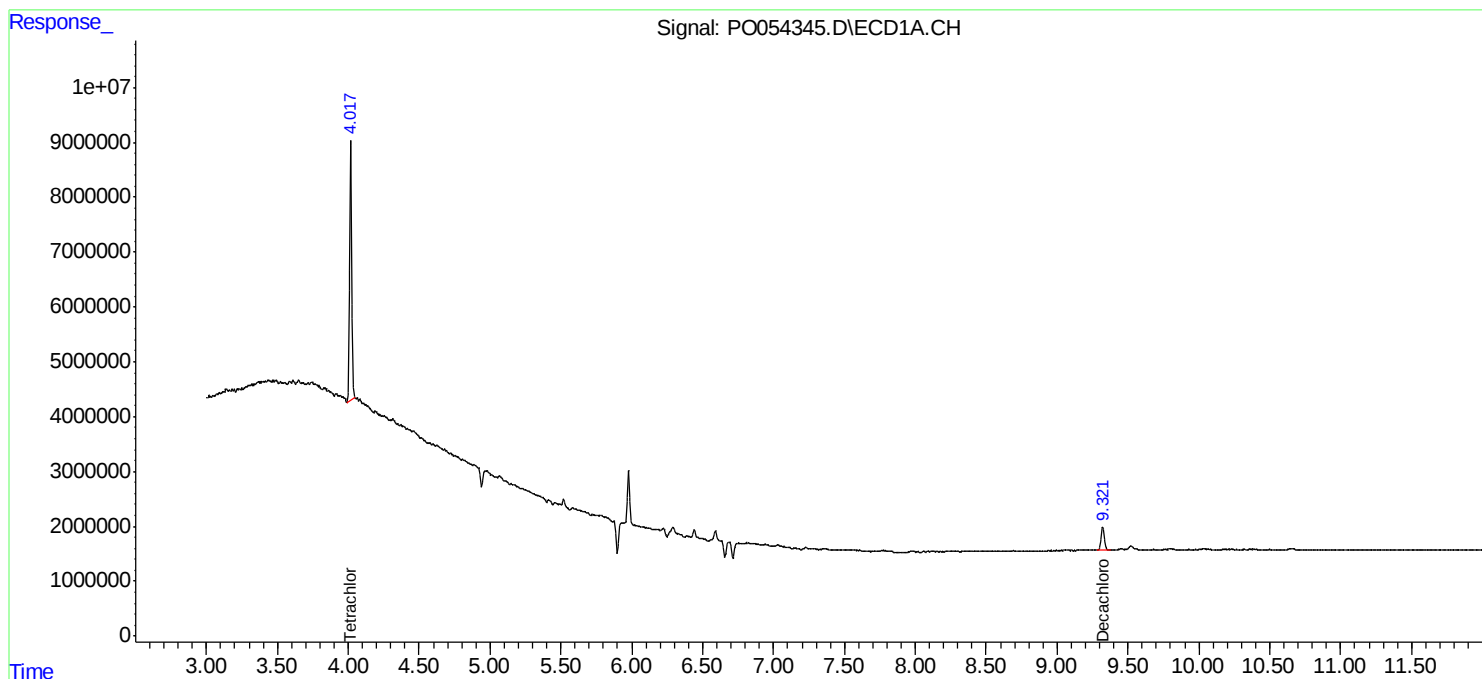


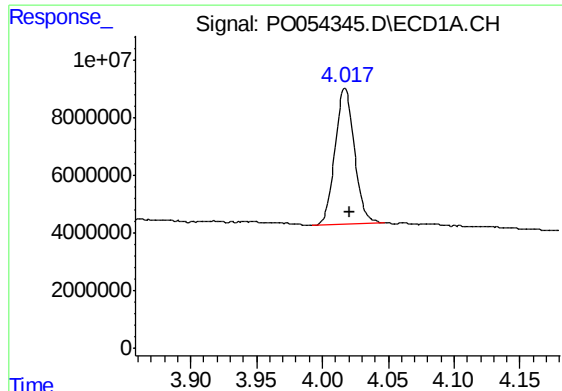

#1 Tetrachloro-m-xylene


R.T.: 4.017 min
Delta R.T.: -0.004 min
Response: 48690591
Conc: 14.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
SD3-0.0-0.5RE

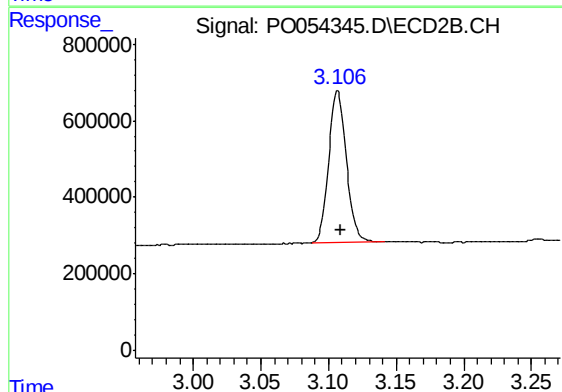


#1 Tetrachloro-m-xylene

R.T.: 3.107 min
Delta R.T.: -0.003 min
Response: 3595563
Conc: 12.84 ng/ml

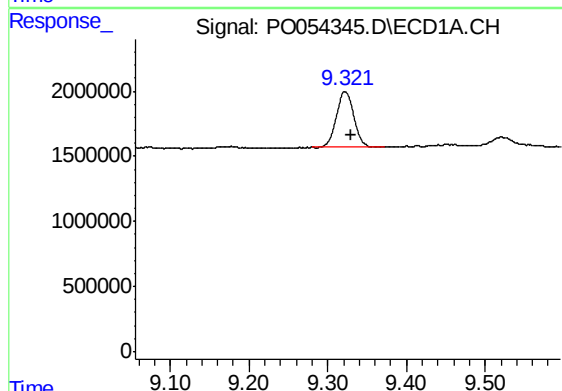

#2 Decachlorobiphenyl

R.T.: 9.322 min
Delta R.T.: -0.008 min
Response: 6577668
Conc: 5.22 ng/ml

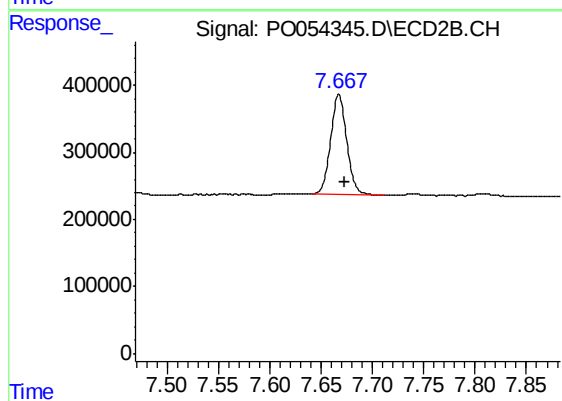

#2 Decachlorobiphenyl

R.T.: 7.667 min
Delta R.T.: -0.005 min
Response: 1642764
Conc: 5.84 ng/ml