

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031219\
 Data File : P0054346.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Mar 2019 11:58
 Operator : SM/SJ
 Sample : K1785-03RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 2019-03-05-DUP-SDRE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 01:11:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 11 14:40:27 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.017	3.107	56752377	4108372	16.513	14.670
2) SA Decachlor...	9.320	7.667	8124454	2030237	6.450	7.216

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031219\
Data File : P0054346.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Mar 2019 11:58
Operator : SM/SJ
Sample : K1785-03RE
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
2019-03-05-DUP-SDRE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 01:11:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031119.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 11 14:40:27 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

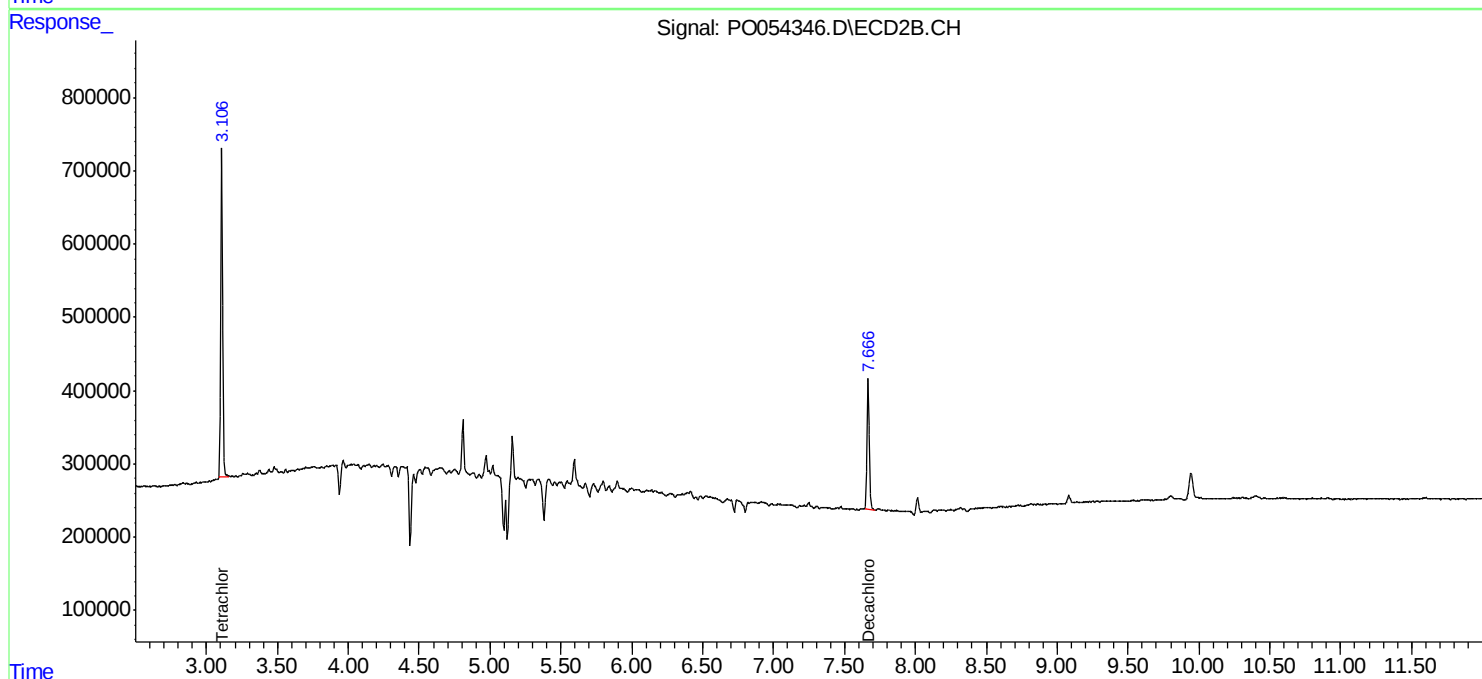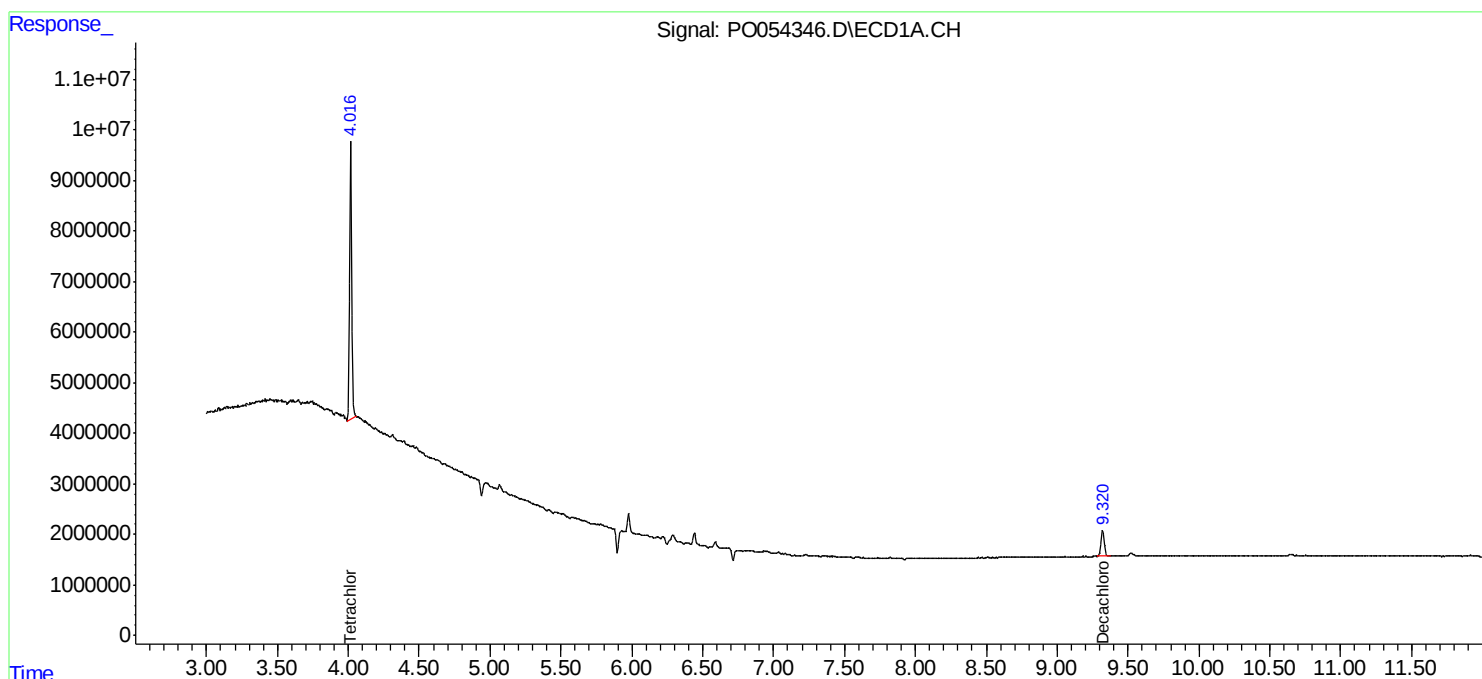


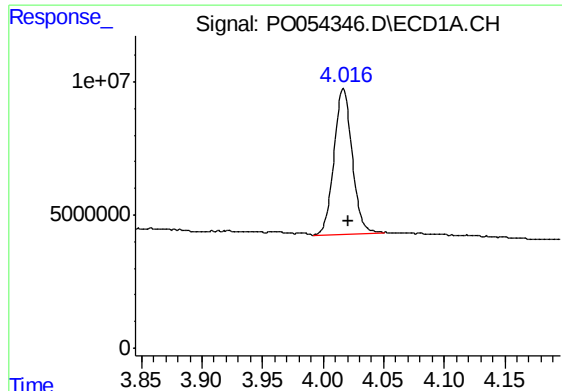

#1 Tetrachloro-m-xylene


R.T.: 4.017 min
Delta R.T.: -0.004 min
Response: 56752377
Conc: 16.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
2019-03-05-DUP-SDRE

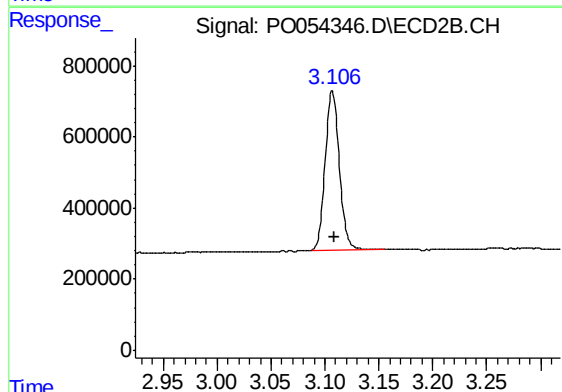


#1 Tetrachloro-m-xylene

R.T.: 3.107 min
Delta R.T.: -0.002 min
Response: 4108372
Conc: 14.67 ng/ml

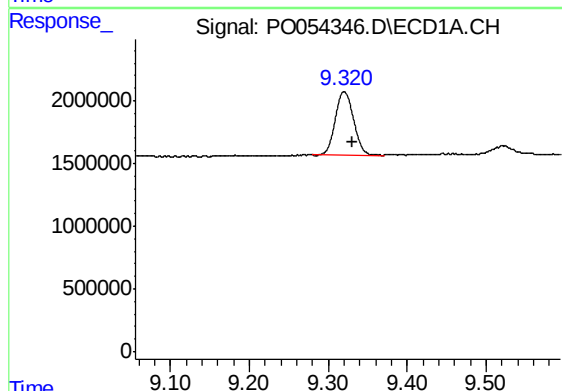

#2 Decachlorobiphenyl

R.T.: 9.320 min
Delta R.T.: -0.010 min
Response: 8124454
Conc: 6.45 ng/ml

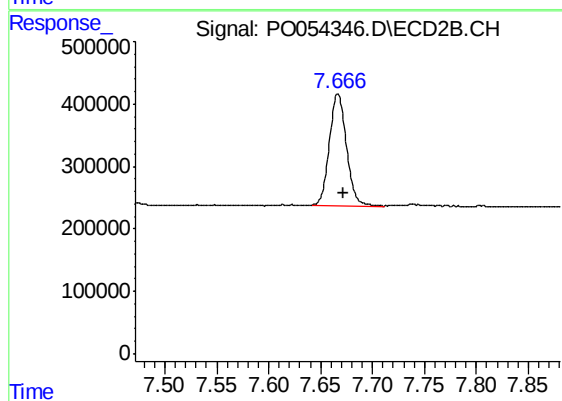

#2 Decachlorobiphenyl

R.T.: 7.667 min
Delta R.T.: -0.006 min
Response: 2030237
Conc: 7.22 ng/ml