

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031320\
 Data File : P0067206.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Mar 2020 8:48
 Operator : DD\AJ
 Sample : L1870-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S10-01-A

Manual Integrations
 APPROVED

Sohil
 3/17/2020 2:02:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 12:20:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 11 15:01:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.112	3.398	547525	666937	17.516	17.044
2) SA Decachlor...	9.572	8.273	329918	580560	9.083	11.923m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031320\
Data File : P0067206.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Mar 2020 8:48
Operator : DD\AJ
Sample : L1870-05
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
S10-01-A


Manual Integrations
APPROVED

Sohil
3/17/2020 2:02:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 12:20:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031120.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 11 15:01:31 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

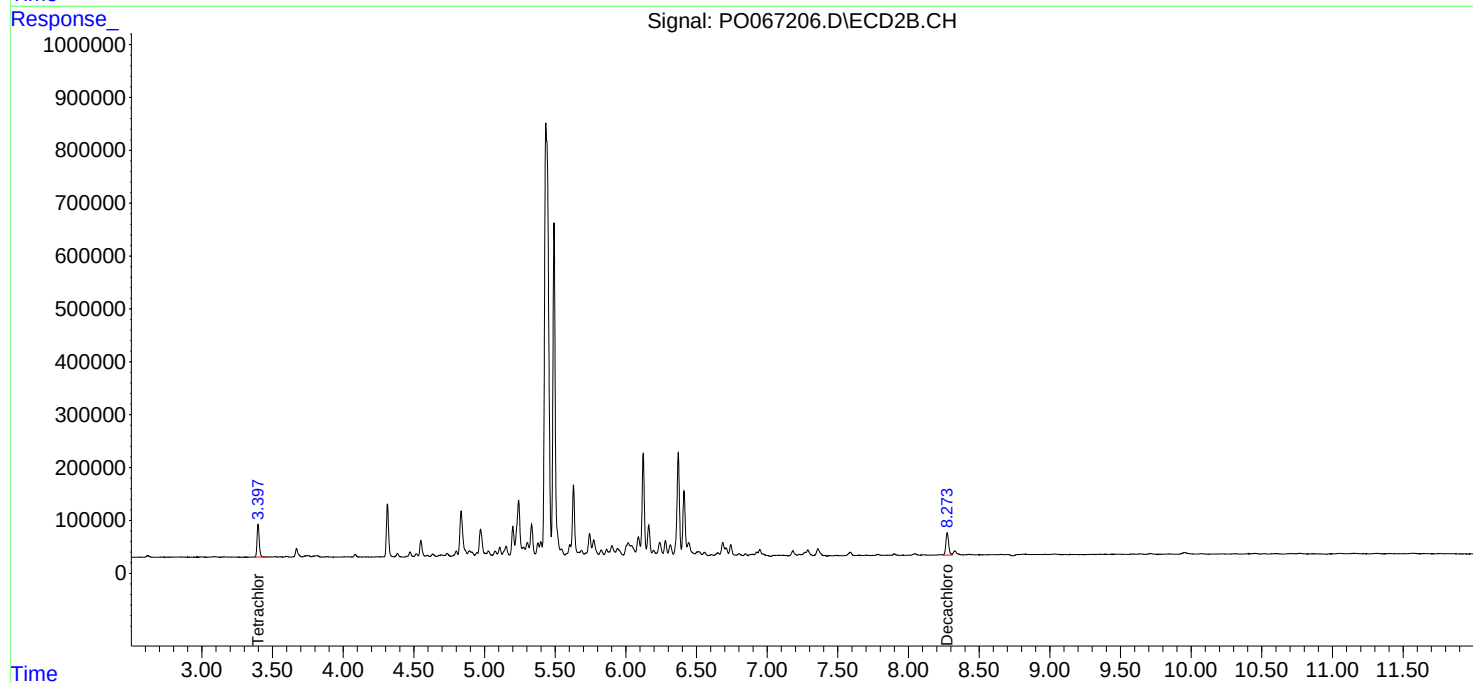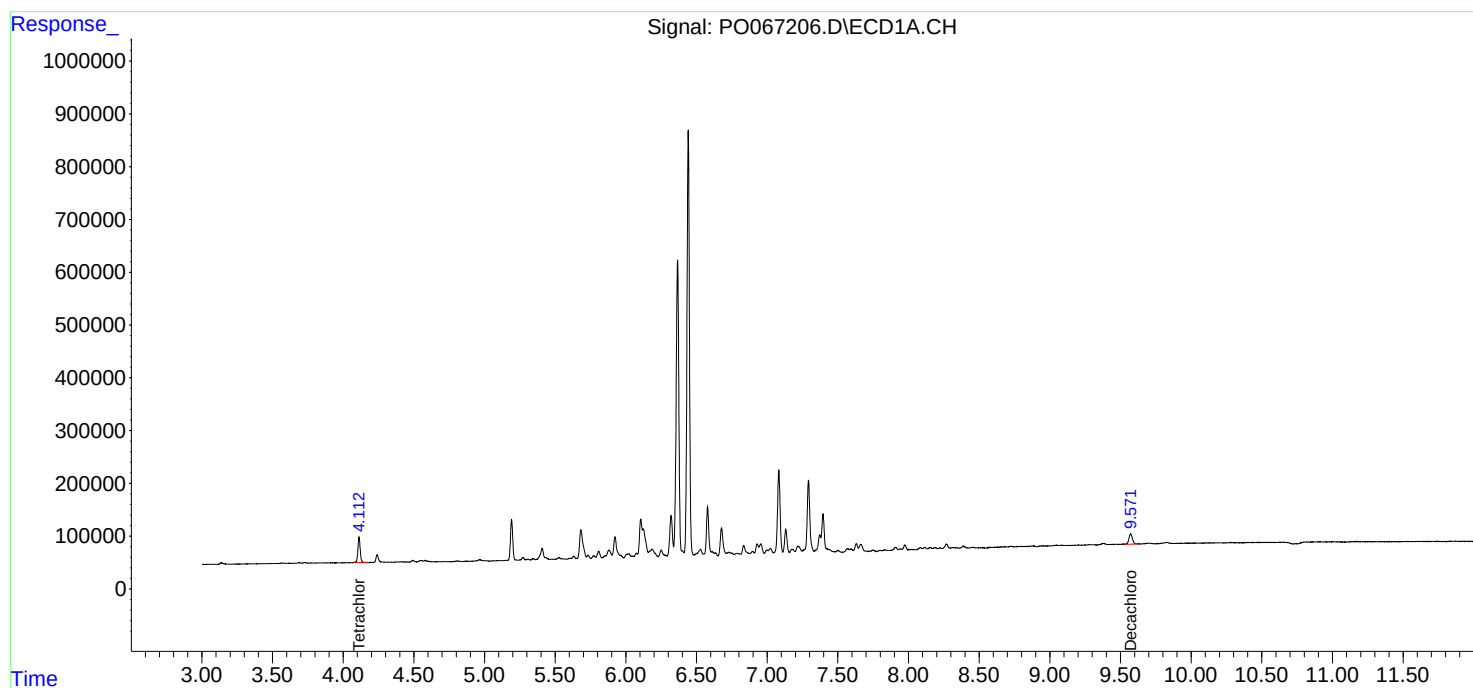

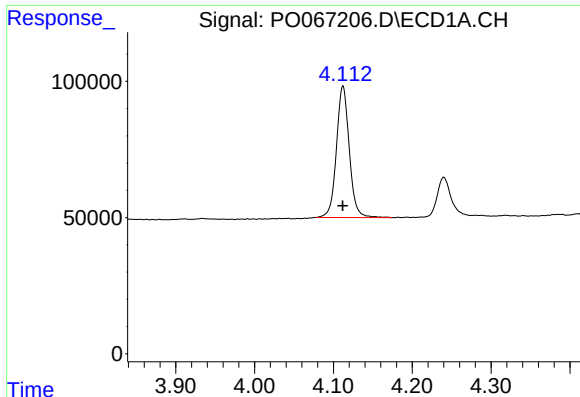


#1 Tetrachloro-m-xylene

R.T.: 4.112 min
Delta R.T.: 0.000 min
Response: 547525
Conc: 17.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
S10-01-A


Manual Integrations
APPROVED

Sohil
3/17/2020 2:02:25 PM

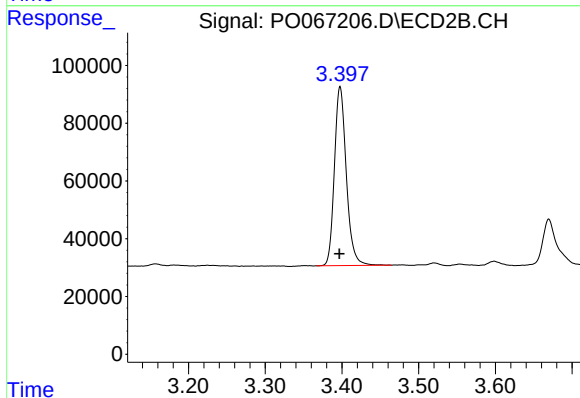


#1 Tetrachloro-m-xylene

R.T.: 3.398 min
Delta R.T.: 0.000 min
Response: 666937
Conc: 17.04 ng/ml

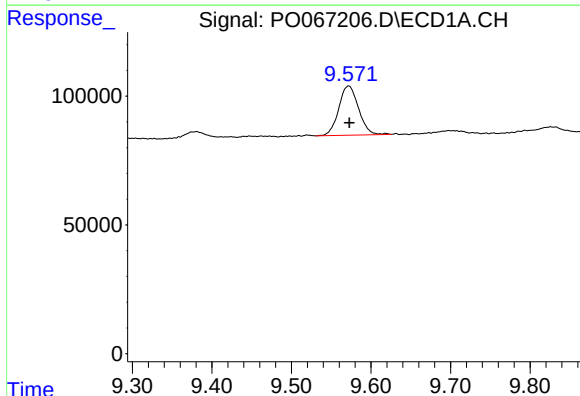

#2 Decachlorobiphenyl

R.T.: 9.572 min
Delta R.T.: -0.001 min
Response: 329918
Conc: 9.08 ng/ml

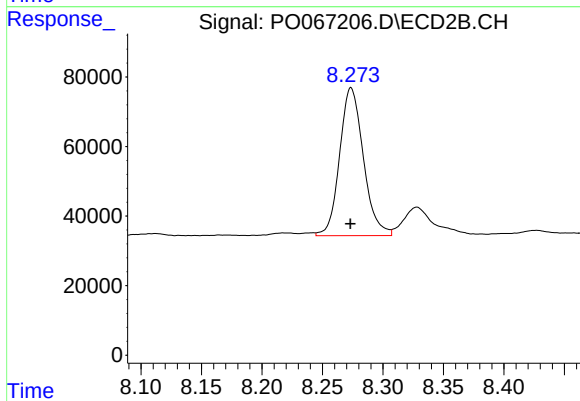

#2 Decachlorobiphenyl

R.T.: 8.273 min
Delta R.T.: 0.000 min
Response: 580560
Conc: 11.92 ng/ml m