

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031320\
 Data File : P0067213.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Mar 2020 14:15
 Operator : DD\AJ
 Sample : L1907-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-9-SA

Manual Integrations
 APPROVED

Sohil
 3/17/2020 2:02:31 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 16:54:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 11 15:01:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.111	3.398	772103	1007980	24.700	25.759
2) SA Decachlor...	9.572	8.273	632008	866380	17.399m	17.794

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031320\
Data File : P0067213.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Mar 2020 14:15
Operator : DD\AJ
Sample : L1907-06
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TP-9-SA


Manual Integrations
APPROVED

Sohil
3/17/2020 2:02:31 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 16:54:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031120.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 11 15:01:31 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

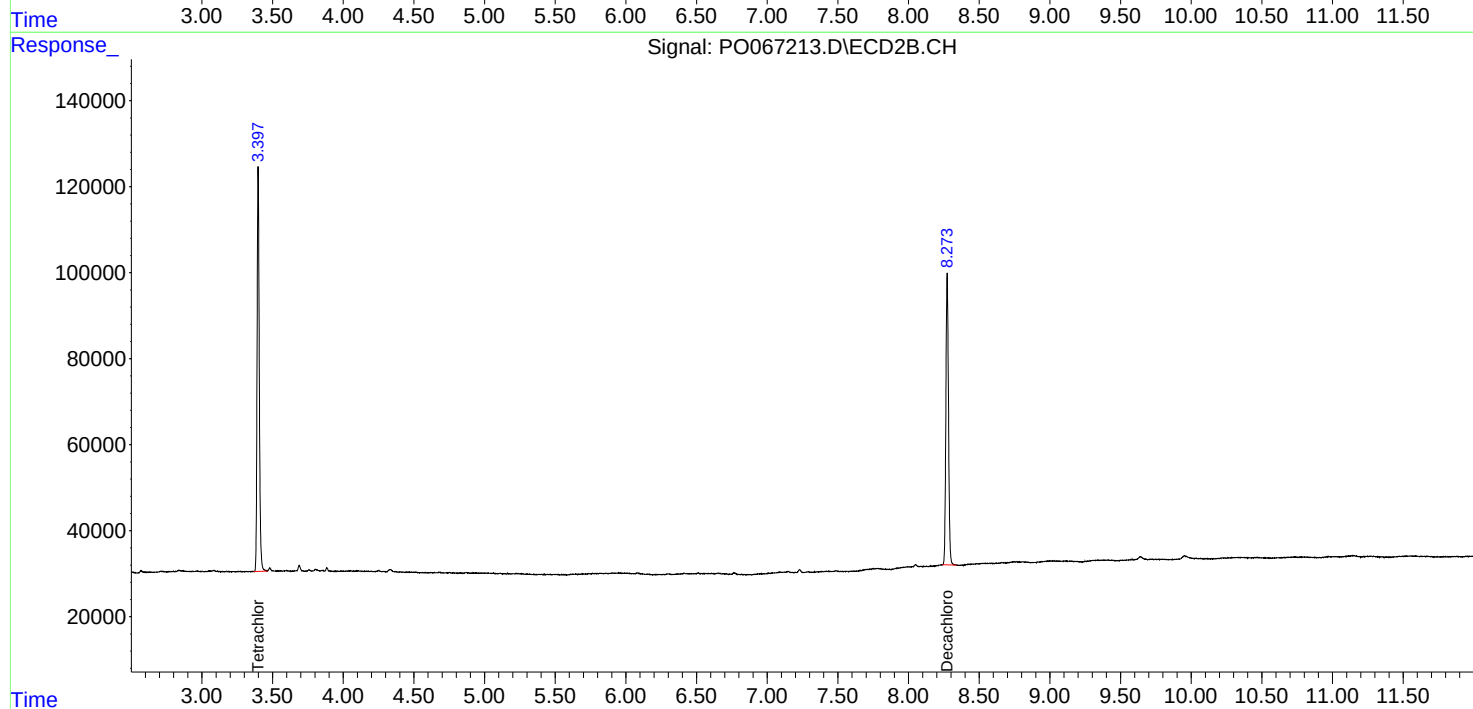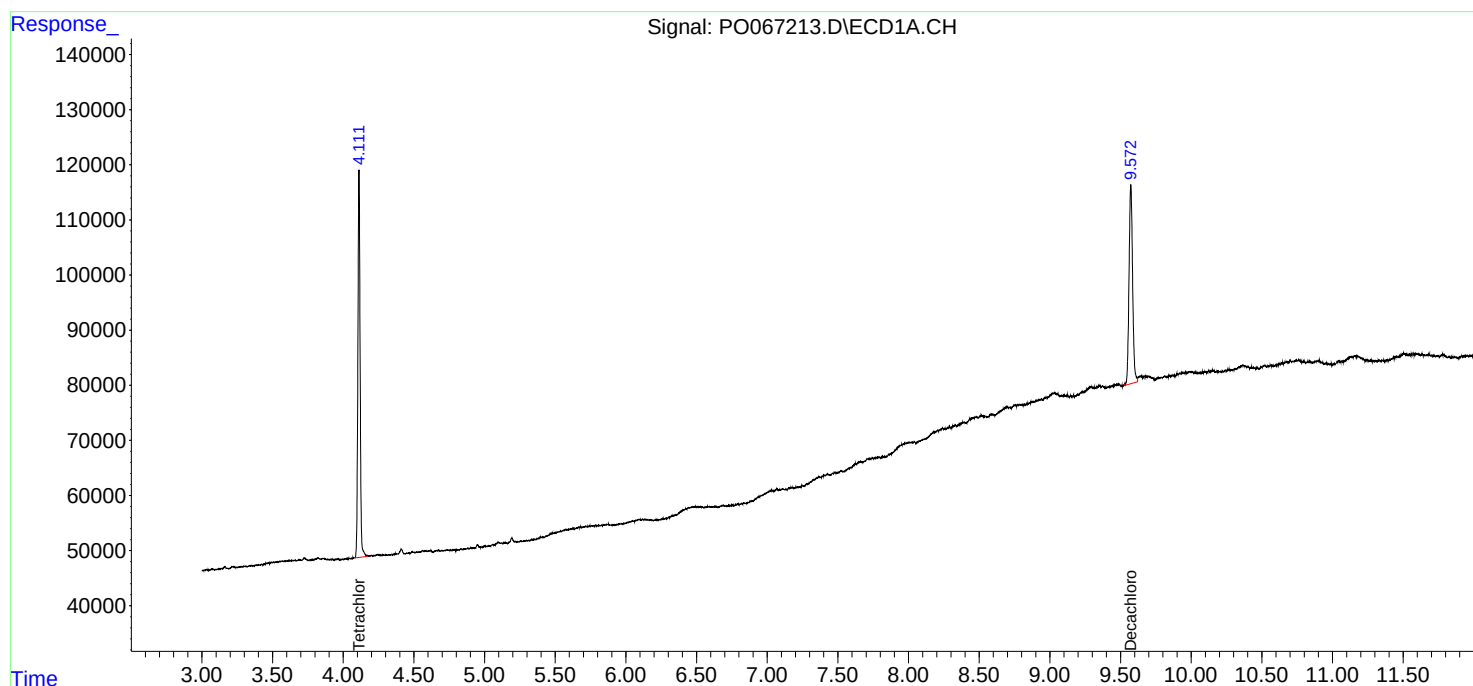

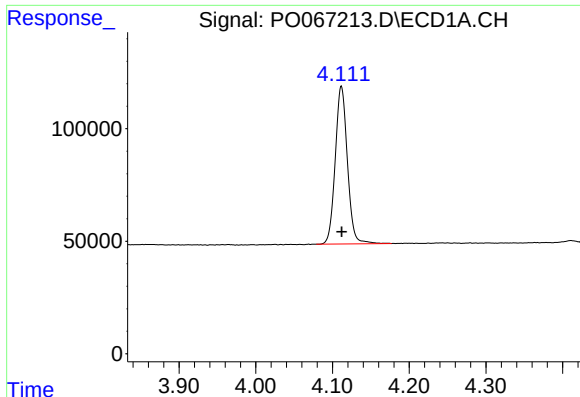


#1 Tetrachloro-m-xylene

R.T.: 4.111 min
Delta R.T.: 0.000 min
Response: 772103
Conc: 24.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-9-SA


Manual Integrations
APPROVED

Sohil
3/17/2020 2:02:31 PM

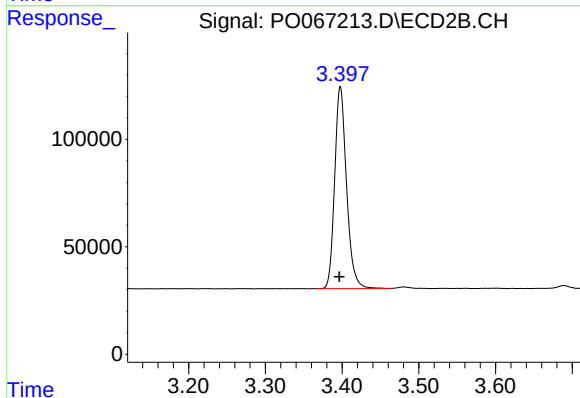


#1 Tetrachloro-m-xylene

R.T.: 3.398 min
Delta R.T.: 0.001 min
Response: 1007980
Conc: 25.76 ng/ml

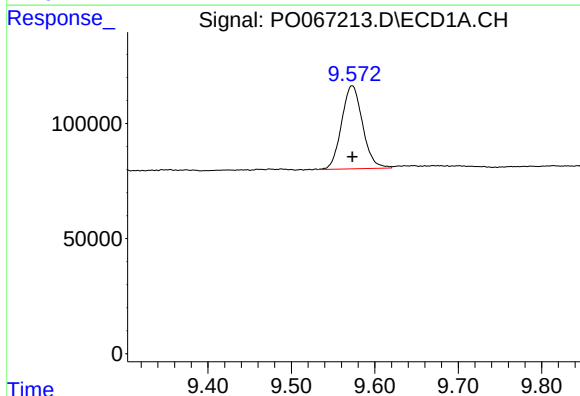

#2 Decachlorobiphenyl

R.T.: 9.572 min
Delta R.T.: 0.000 min
Response: 632008
Conc: 17.40 ng/ml m

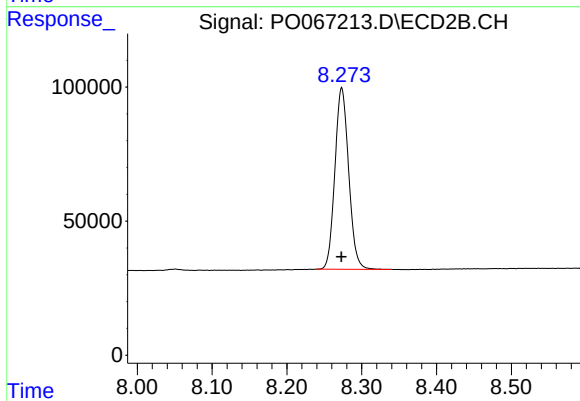

#2 Decachlorobiphenyl

R.T.: 8.273 min
Delta R.T.: 0.000 min
Response: 866380
Conc: 17.79 ng/ml