

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031320\
 Data File : P0067228.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Mar 2020 18:29
 Operator : DD\AJ
 Sample : L1913-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MK-031220-2-5-COMP-B3

Manual Integrations
 APPROVED

Sohil
 3/16/2020 4:41:05 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 18:50:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 11 15:01:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.111	3.397	683581	806832	21.868	20.619
2)	SA Decachlor...	9.571	8.273	669174	915462	18.422m	18.802

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031320\
Data File : P0067228.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Mar 2020 18:29
Operator : DD\AJ
Sample : L1913-07
Misc :
ALS Vial : 26 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
MK-031220-2-5-COMP-B3


Manual Integrations
APPROVED

Sohil
3/16/2020 4:41:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 18:50:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031120.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 11 15:01:31 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

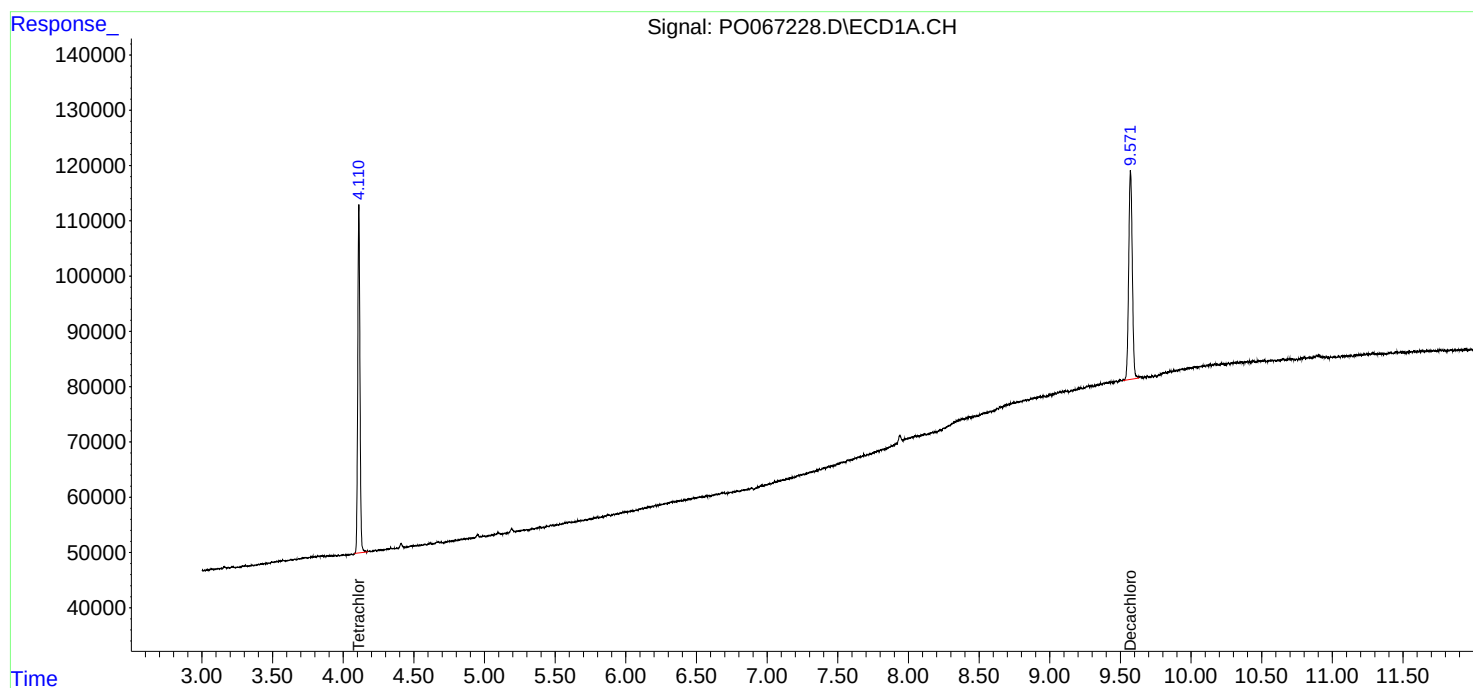

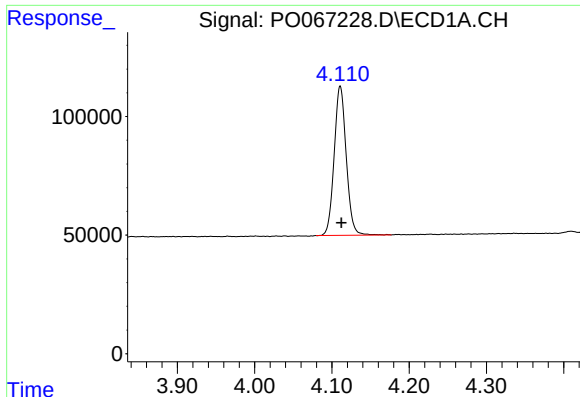


#1 Tetrachloro-m-xylene

R.T.: 4.111 min
Delta R.T.: -0.001 min
Response: 683581
Conc: 21.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
MK-031220-2-5-COMP-B3


Manual Integrations
APPROVED

Sohil
3/16/2020 4:41:05 PM

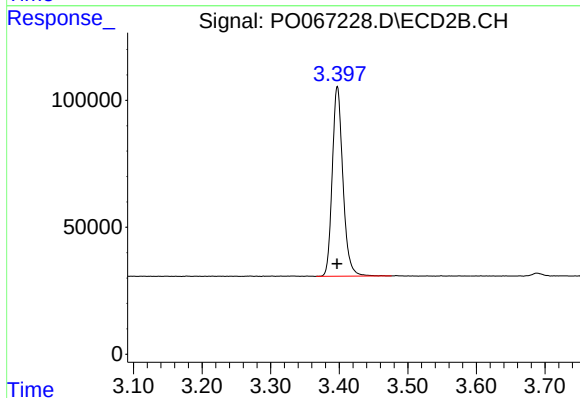


#1 Tetrachloro-m-xylene

R.T.: 3.397 min
Delta R.T.: 0.000 min
Response: 806832
Conc: 20.62 ng/ml

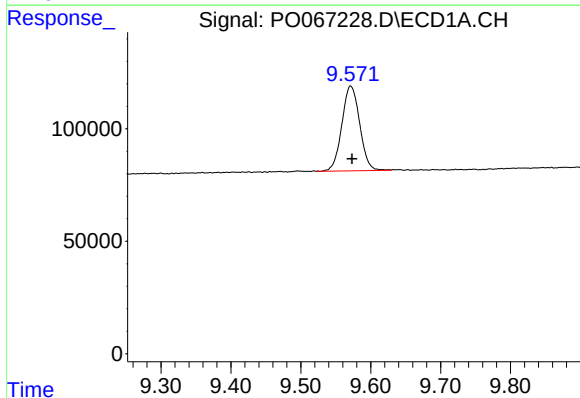

#2 Decachlorobiphenyl

R.T.: 9.571 min
Delta R.T.: -0.003 min
Response: 669174
Conc: 18.42 ng/ml m

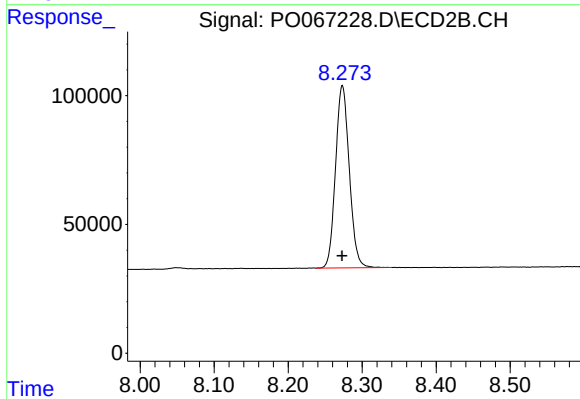

#2 Decachlorobiphenyl

R.T.: 8.273 min
Delta R.T.: 0.000 min
Response: 915462
Conc: 18.80 ng/ml