

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031519\
 Data File : P0054420.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Mar 2019 16:01
 Operator : SM/SJ
 Sample : PB117906BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB117906BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 22:52:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 15 05:00:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.025	3.105	107.1E6	3705823	21.746	14.585 #
2) SA Decachlor...	9.338	7.671	28474082	5560968	20.670	18.803

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031519\
Data File : P0054420.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Mar 2019 16:01
Operator : SM/SJ
Sample : PB117906BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB117906BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 22:52:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031419.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 15 05:00:00 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

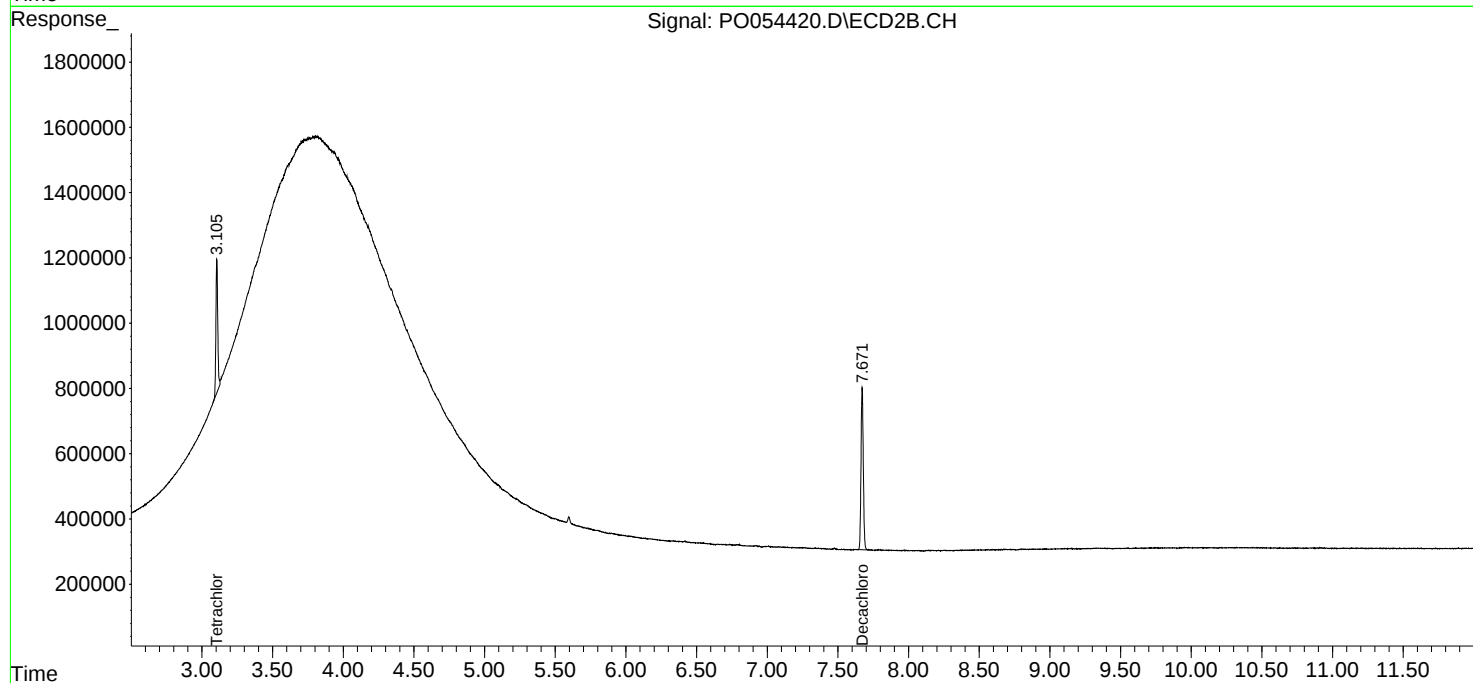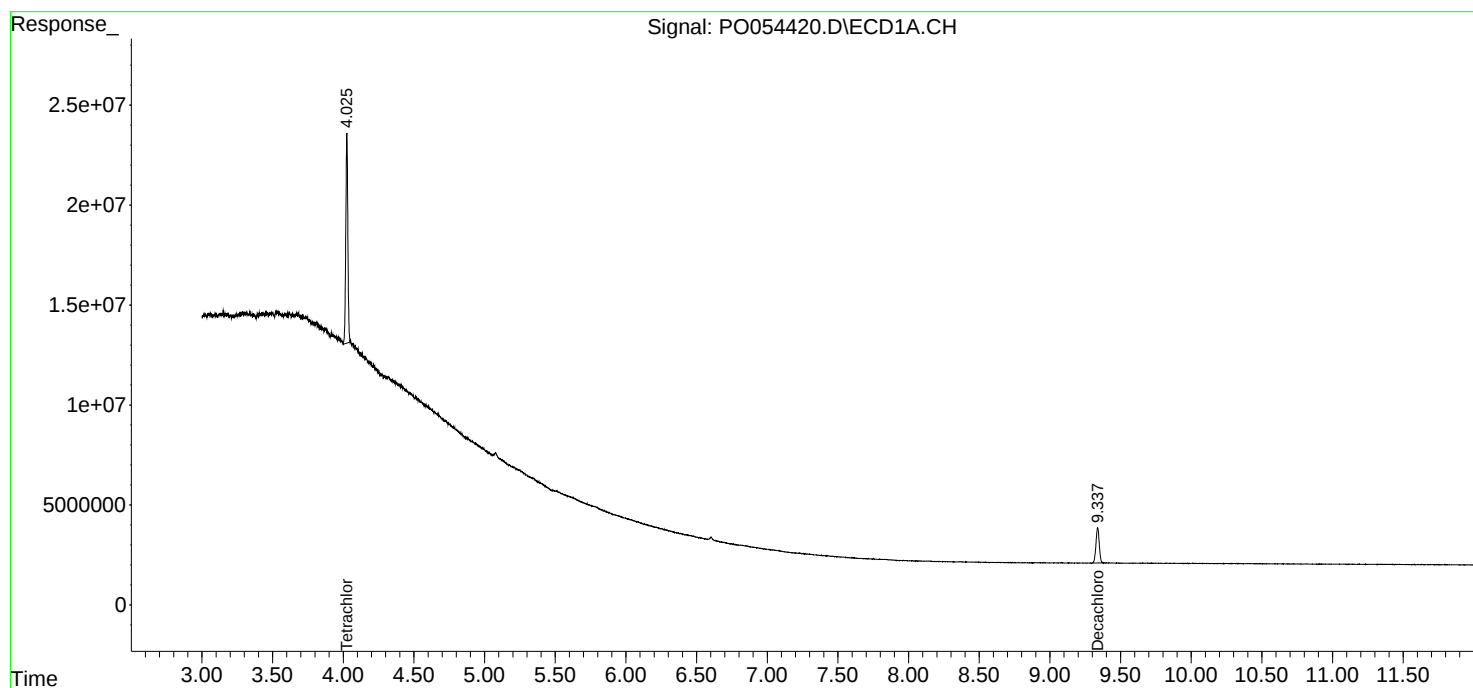


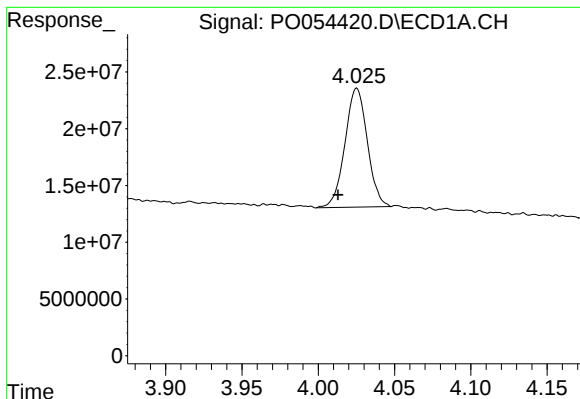

#1 Tetrachloro-m-xylene


R.T.: 4.025 min
Delta R.T.: 0.012 min
Response: 107095038
Conc: 21.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB117906BL

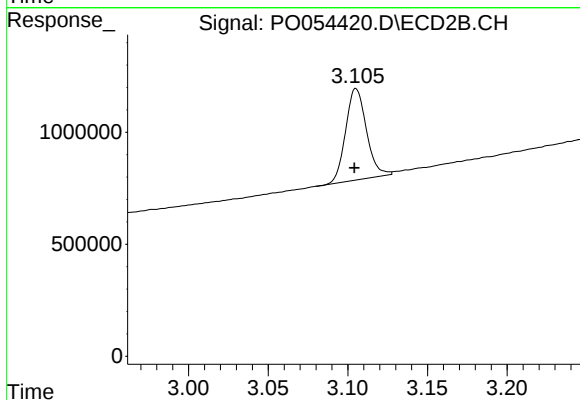


#1 Tetrachloro-m-xylene

R.T.: 3.105 min
Delta R.T.: 0.000 min
Response: 3705823
Conc: 14.58 ng/ml

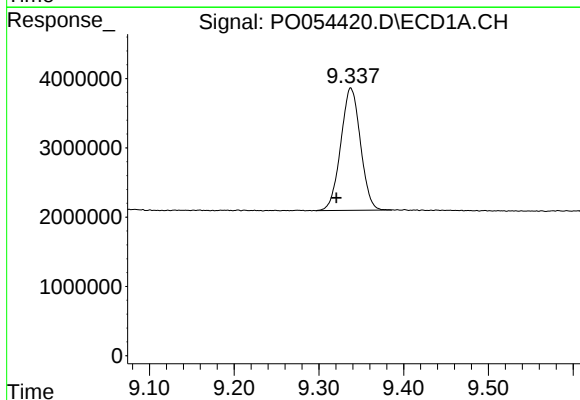

#2 Decachlorobiphenyl

R.T.: 9.338 min
Delta R.T.: 0.017 min
Response: 28474082
Conc: 20.67 ng/ml

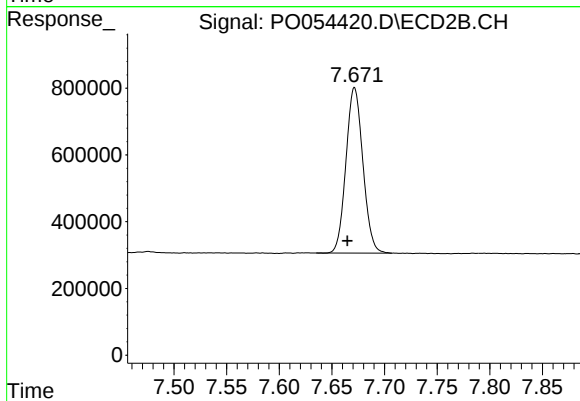

#2 Decachlorobiphenyl

R.T.: 7.671 min
Delta R.T.: 0.007 min
Response: 5560968
Conc: 18.80 ng/ml