

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031519\
 Data File : P0054426.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Mar 2019 17:43
 Operator : SM/SJ
 Sample : K1866-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MR-MH-15-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 22:54:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 15 05:00:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.014	3.104	106.0E6	4784803	21.514	18.831
2) SA Decachlor...	9.321	7.667	28511974	5970747	20.697	20.189

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031519\
Data File : P0054426.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Mar 2019 17:43
Operator : SM/SJ
Sample : K1866-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MR-MH-15-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 22:54:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031419.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 15 05:00:00 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

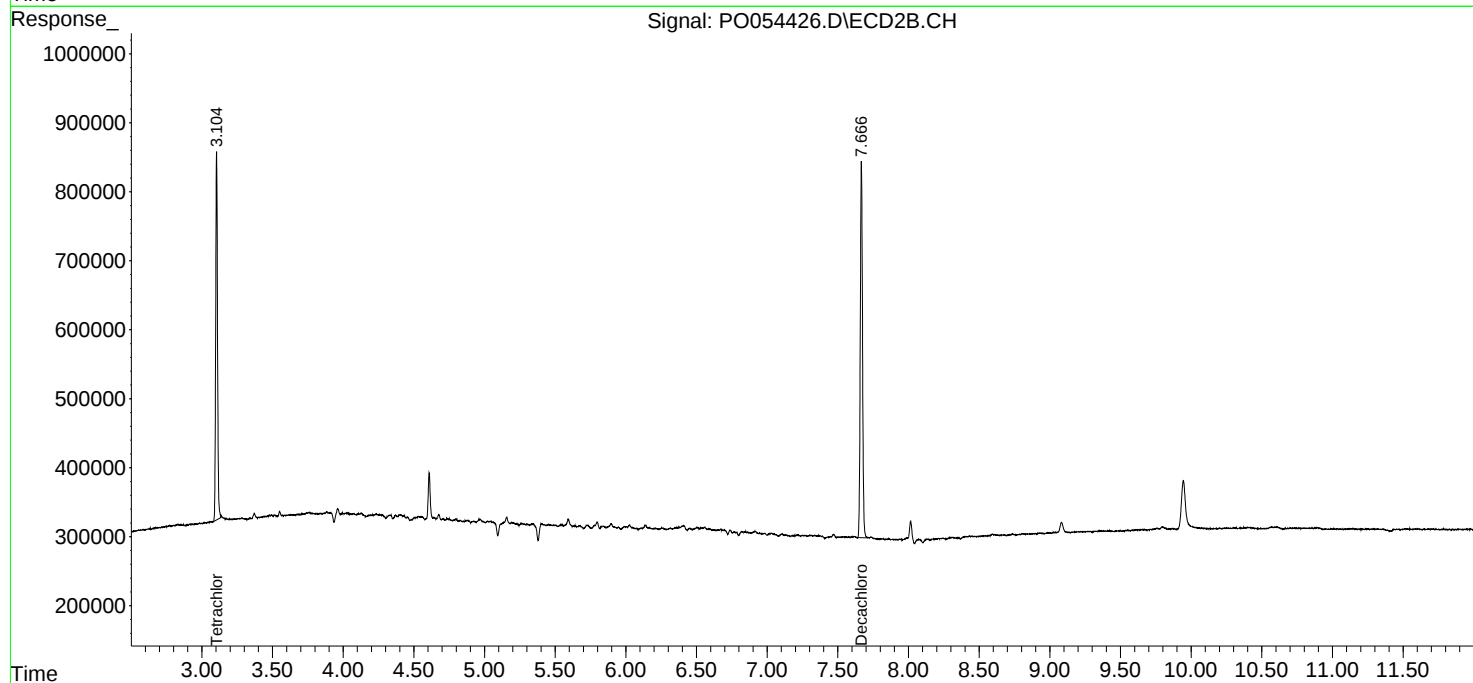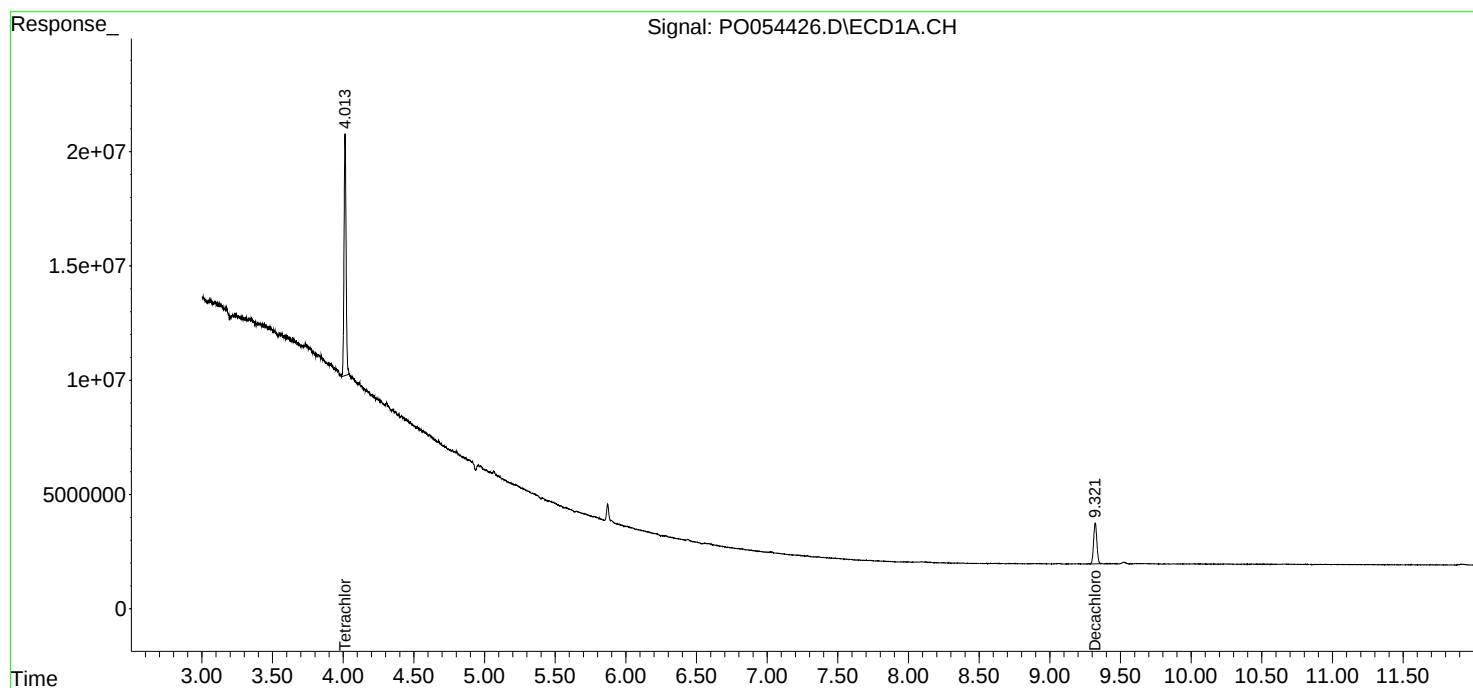


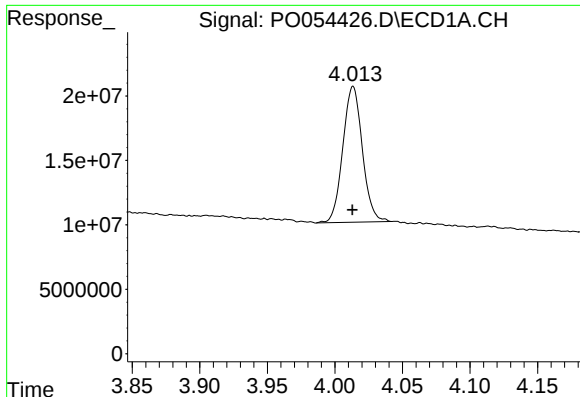

#1 Tetrachloro-m-xylene


R.T.: 4.014 min
Delta R.T.: 0.000 min
Response: 105954883
Conc: 21.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
MR-MH-15-COMP

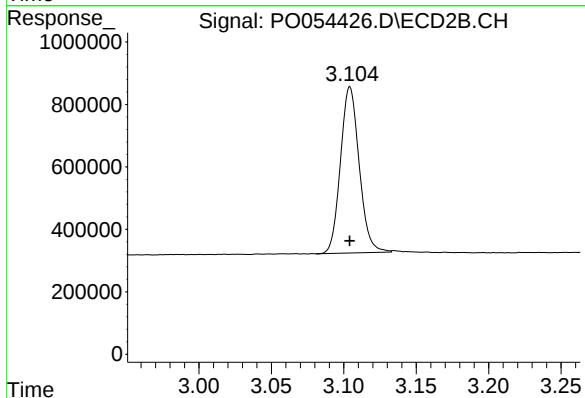


#1 Tetrachloro-m-xylene

R.T.: 3.104 min
Delta R.T.: 0.000 min
Response: 4784803
Conc: 18.83 ng/ml

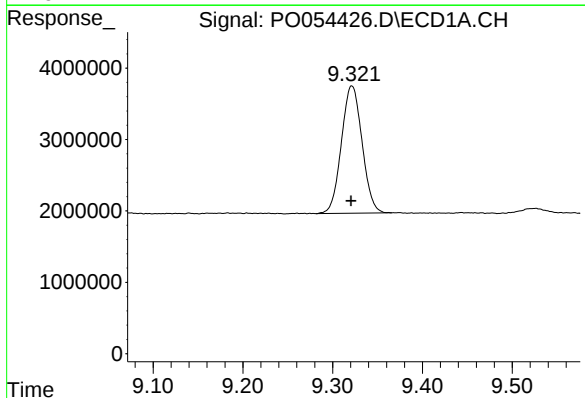

#2 Decachlorobiphenyl

R.T.: 9.321 min
Delta R.T.: 0.000 min
Response: 28511974
Conc: 20.70 ng/ml

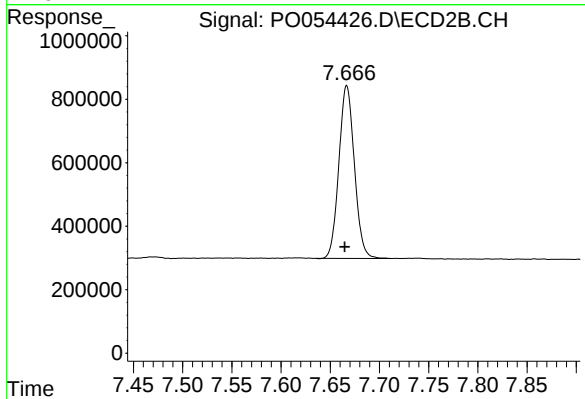

#2 Decachlorobiphenyl

R.T.: 7.667 min
Delta R.T.: 0.002 min
Response: 5970747
Conc: 20.19 ng/ml