

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031519\
 Data File : P0054436.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Mar 2019 20:32
 Operator : SM/SJ
 Sample : K1897-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-1

Manual Integrations
 APPROVED

Sohil
 3/19/2019 8:51:26 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 22:58:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 15 05:00:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.013	3.103	95906733	4174514	19.474	16.429
2) SA Decachlor...	9.320	7.665	20809235	3888423	15.106m	13.148

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031519\
Data File : P0054436.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Mar 2019 20:32
Operator : SM/SJ
Sample : K1897-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-1


Manual Integrations
APPROVED

Sohil
3/19/2019 8:51:26 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 22:58:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031419.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 15 05:00:00 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

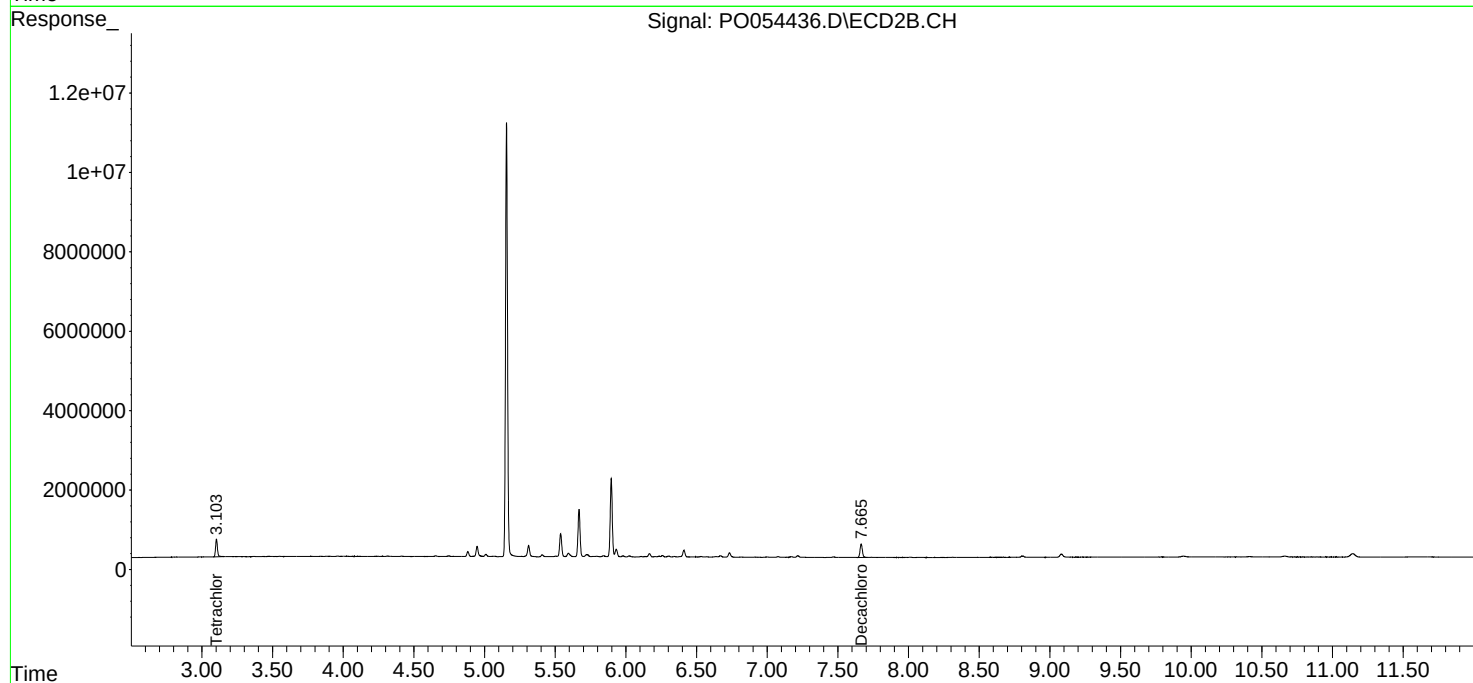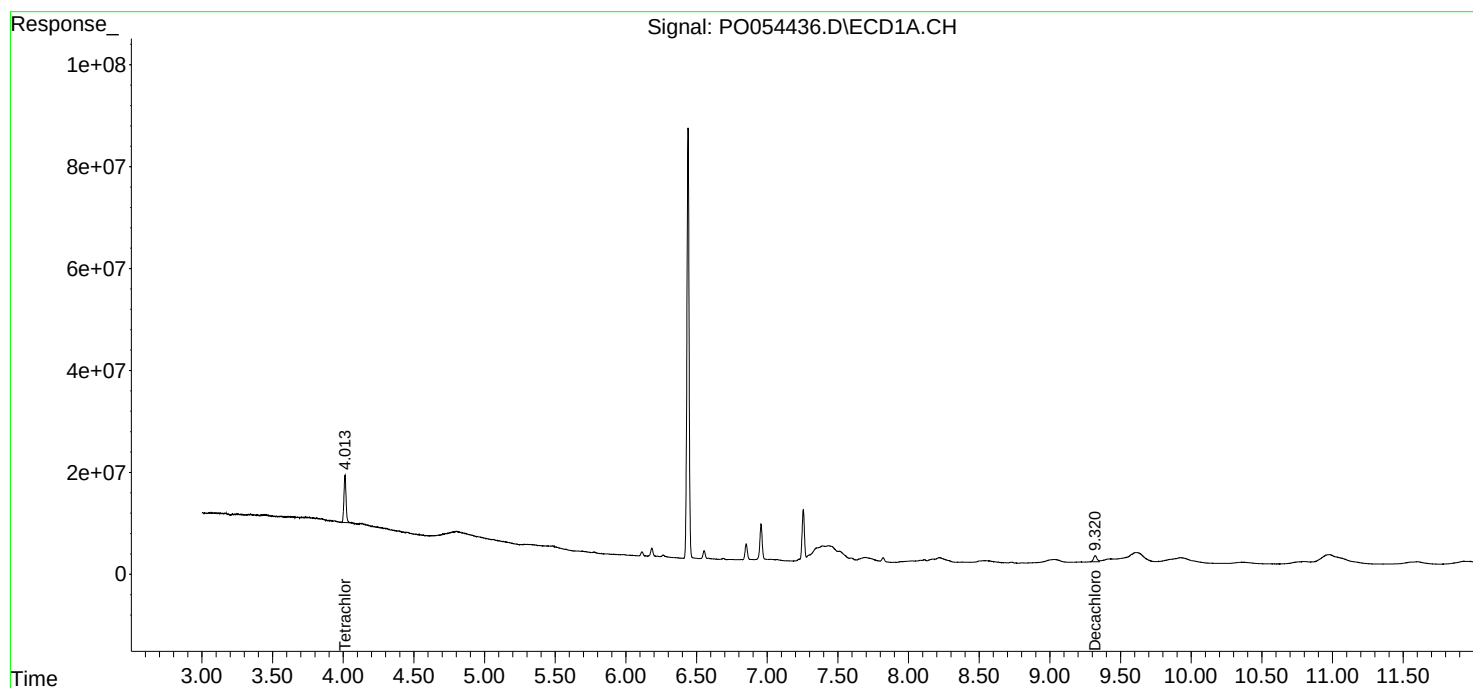

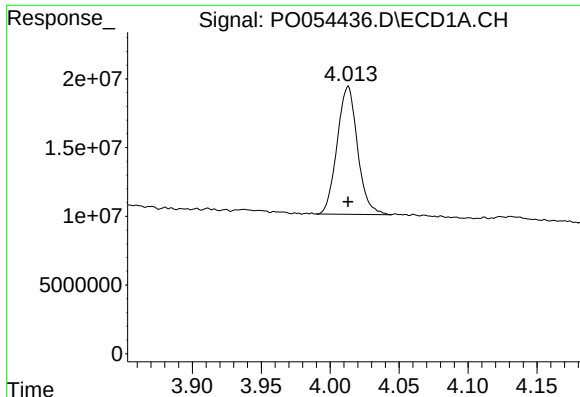


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 95906733
Conc: 19.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-1


Manual Integrations
APPROVED

Sohil
3/19/2019 8:51:26 AM

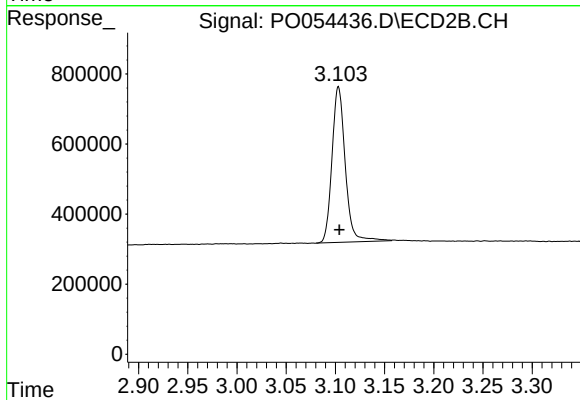


#1 Tetrachloro-m-xylene

R.T.: 3.103 min
Delta R.T.: 0.000 min
Response: 4174514
Conc: 16.43 ng/ml

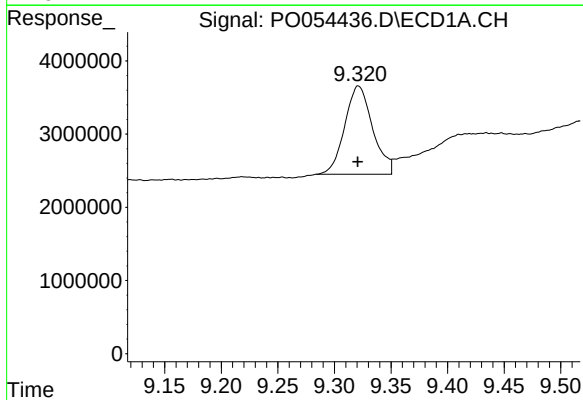

#2 Decachlorobiphenyl

R.T.: 9.320 min
Delta R.T.: 0.000 min
Response: 20809235
Conc: 15.11 ng/ml m

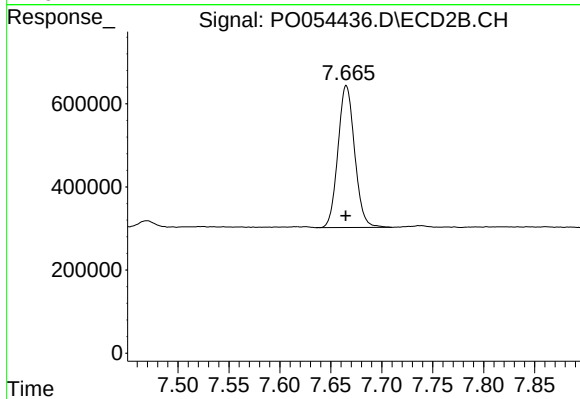

#2 Decachlorobiphenyl

R.T.: 7.665 min
Delta R.T.: 0.000 min
Response: 3888423
Conc: 13.15 ng/ml