

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031519\
Data File : P0054450.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Mar 2019 00:29
Operator : SM/SJ
Sample : K1900-11
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BP-DUP02-20190313

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 03:40:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031419.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 15 05:00:00 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.012	3.104	93892347	4756280	19.065	18.719
2) SA Decachlor...	9.319	7.664	28512490	6148758	20.698	20.791

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031519\
Data File : P0054450.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Mar 2019 00:29
Operator : SM/SJ
Sample : K1900-11
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BP-DUP02-20190313

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 03:40:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031419.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 15 05:00:00 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

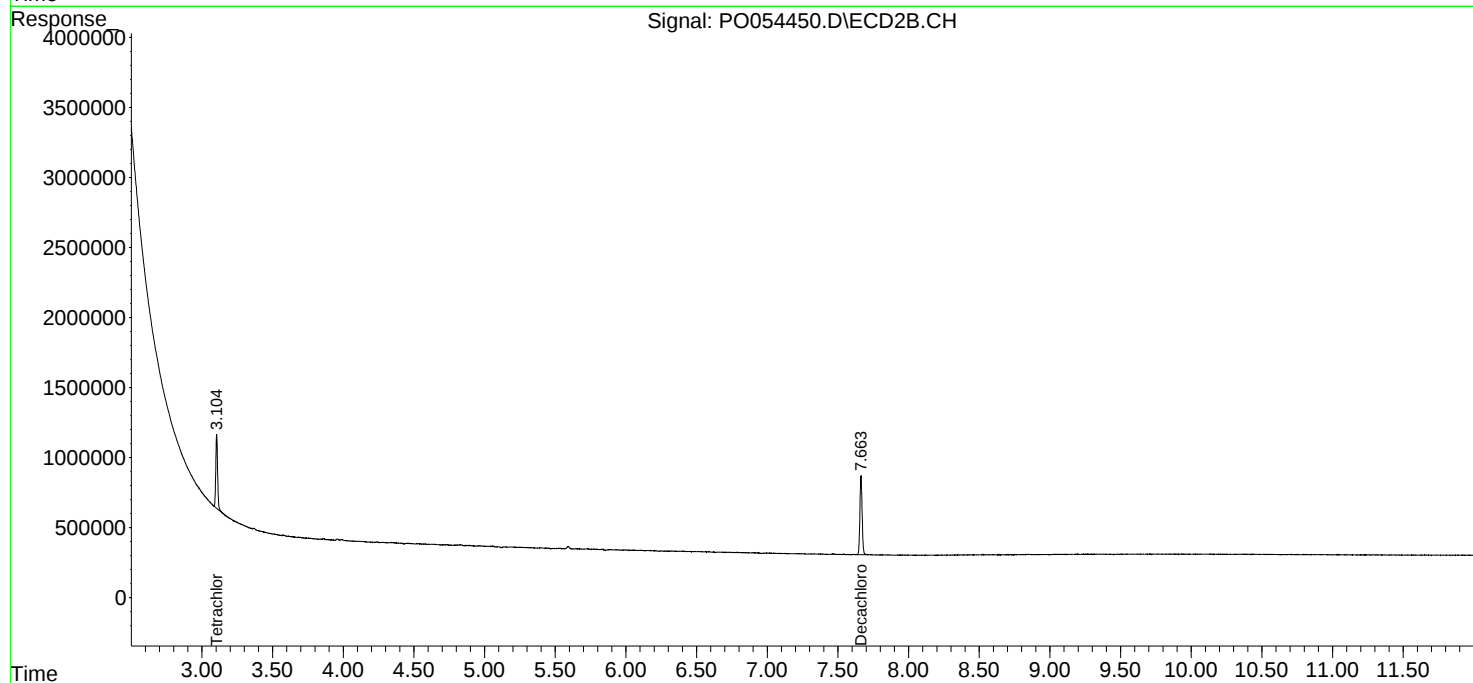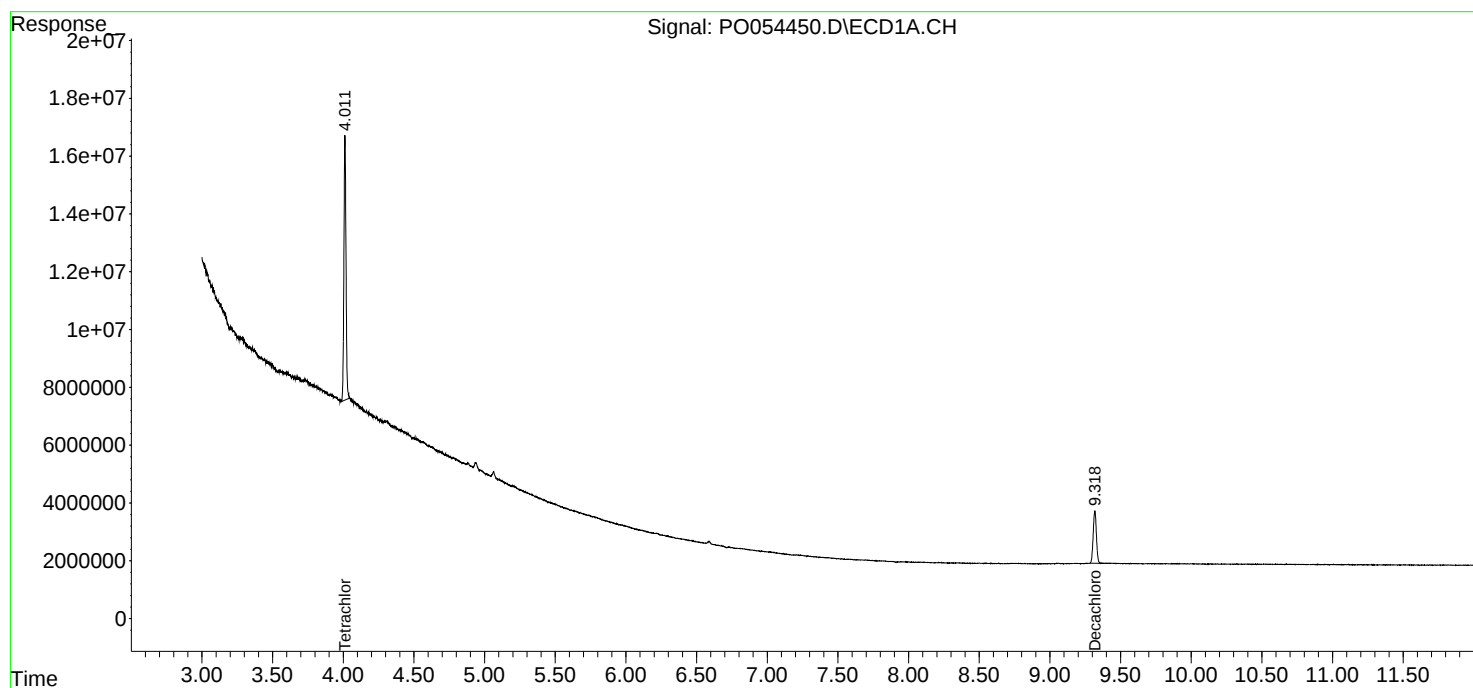


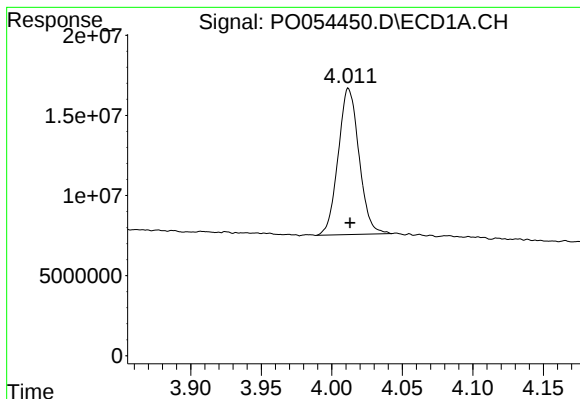

#1 Tetrachloro-m-xylene


R.T.: 4.012 min
Delta R.T.: -0.001 min
Response: 93892347
Conc: 19.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
BP-DUP02-20190313

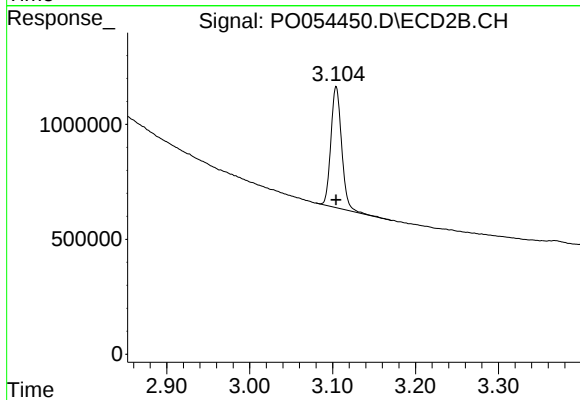


#1 Tetrachloro-m-xylene

R.T.: 3.104 min
Delta R.T.: 0.000 min
Response: 4756280
Conc: 18.72 ng/ml

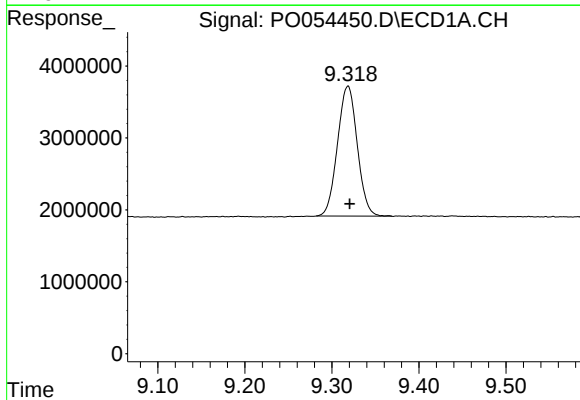

#2 Decachlorobiphenyl

R.T.: 9.319 min
Delta R.T.: -0.002 min
Response: 28512490
Conc: 20.70 ng/ml

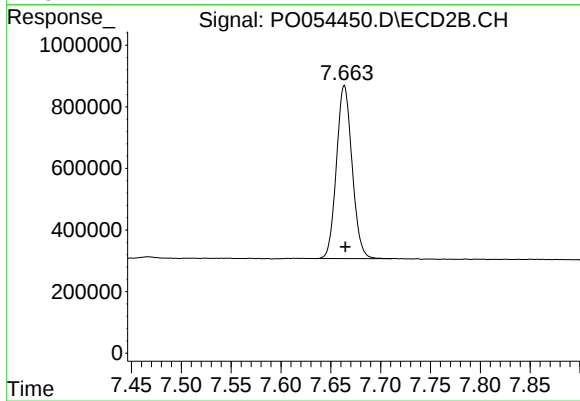

#2 Decachlorobiphenyl

R.T.: 7.664 min
Delta R.T.: -0.001 min
Response: 6148758
Conc: 20.79 ng/ml