

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031620\
 Data File : P0067289.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Mar 2020 20:43
 Operator : DD\AJ
 Sample : L1942-17
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 04:19:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 17 02:39:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.107	3.397	611556	272286	23.160	17.135 #
2)	SA Decachlor...	9.559	8.269	614519	533624	17.473	15.397
Target Compounds							
30)	L6 AR-1254-5	7.297	0.000	434781	0	274.384	N.D. #
32)	L7 AR-1260-2	7.089	0.000	825597	0	350.278	N.D. #
35)	L7 AR-1260-5	0.000	6.988	0	825	N.D.	0.254 #
37)	L8 AR-1262-2	0.000	6.988	0	825	N.D.	0.295 #
40)	L8 AR-1262-5	0.000	7.761	0	3270	N.D.	3.107 #
43)	L9 AR-1268-3	0.000	7.544	0	1325	N.D.	0.470 #
44)	L9 AR-1268-4	0.000	7.761	0	3270	N.D.	2.599 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031620\
Data File : P0067289.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Mar 2020 20:43
Operator : DD\AJ
Sample : L1942-17
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 04:19:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031620.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 17 02:39:09 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

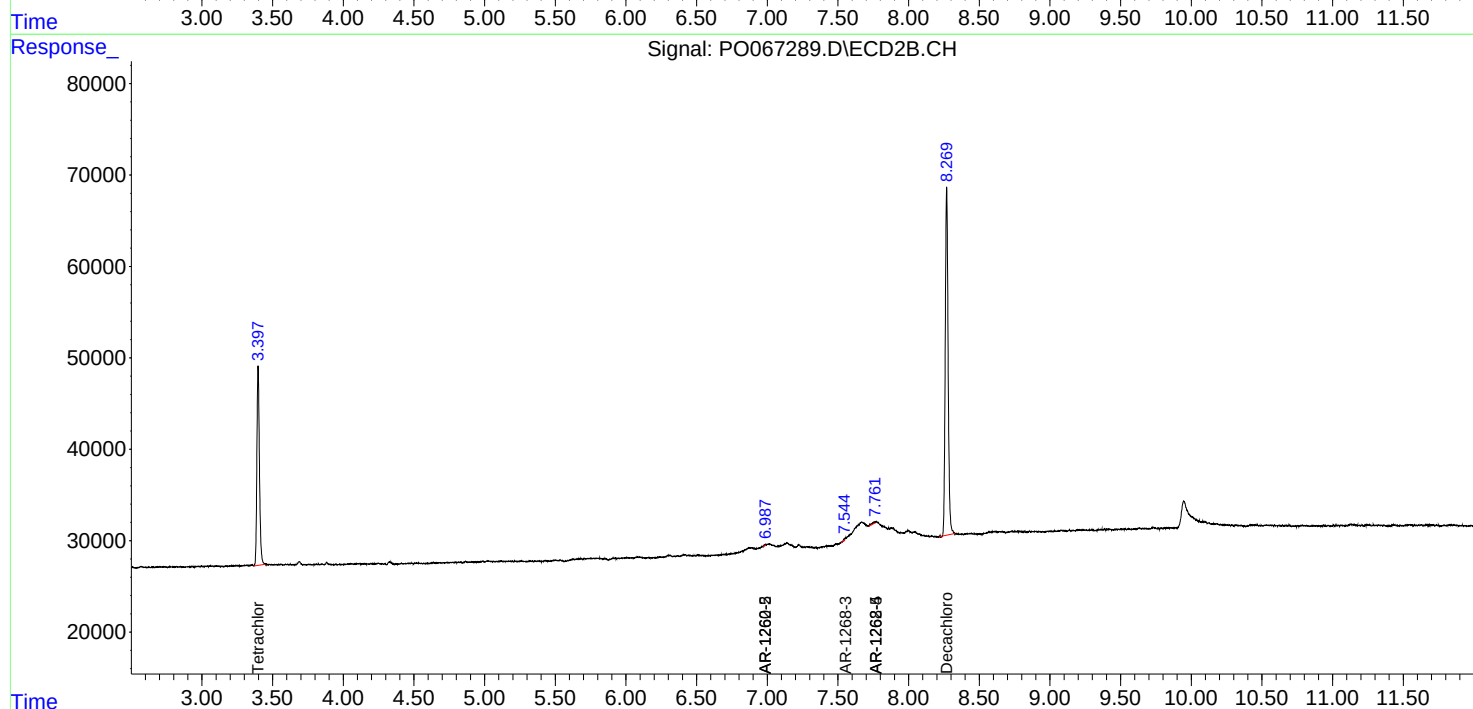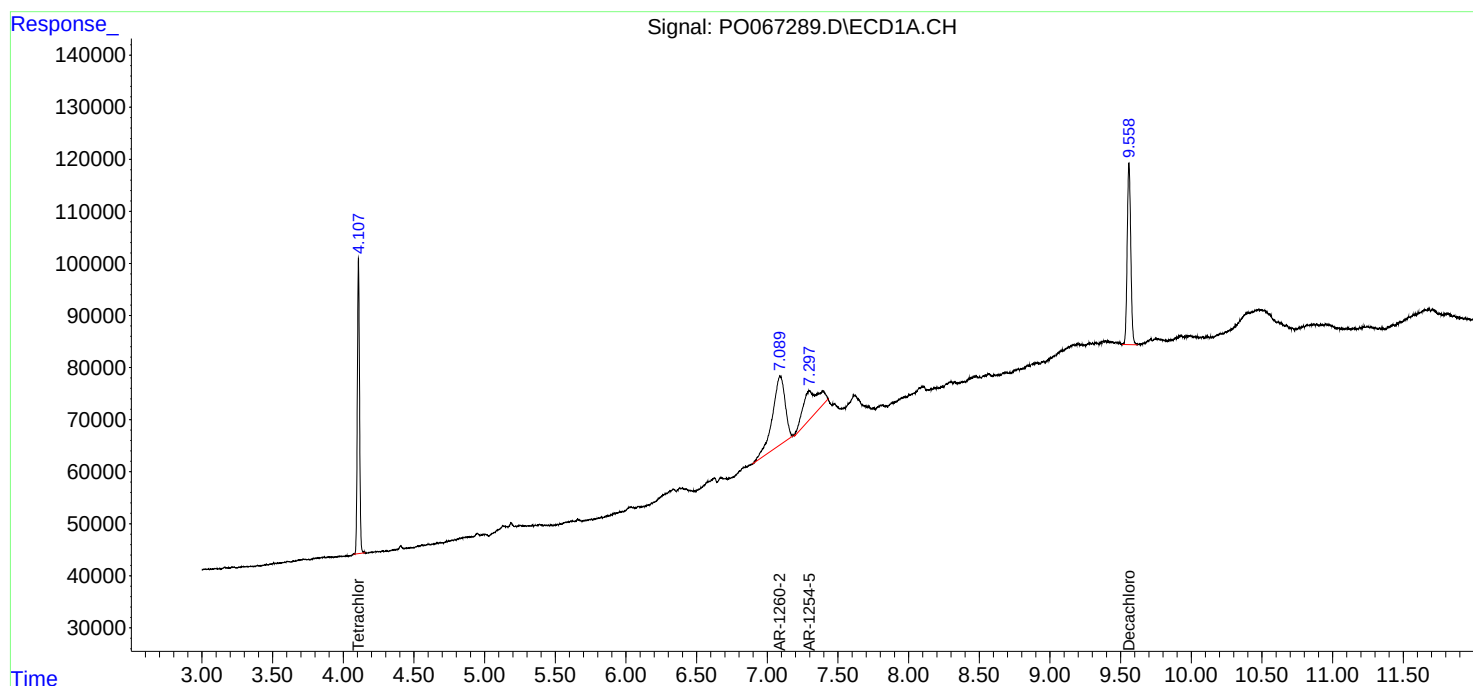


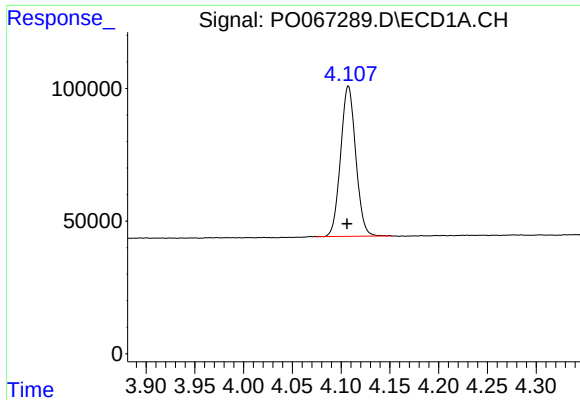

#1 Tetrachloro-m-xylene


R.T.: 4.107 min
Delta R.T.: 0.002 min
Response: 611556
Conc: 23.16 ng/ml

Instrument :
ECD_O
ClientSampleId :

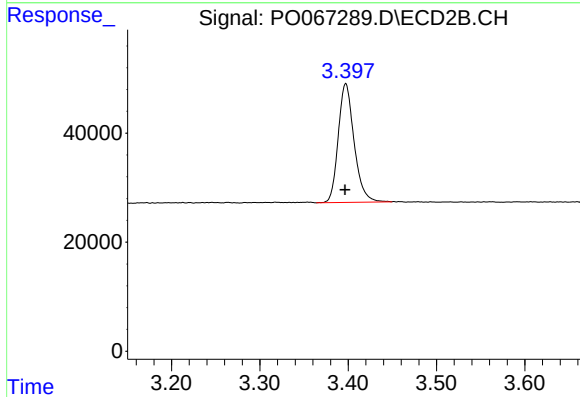


#1 Tetrachloro-m-xylene

R.T.: 3.397 min
Delta R.T.: 0.000 min
Response: 272286
Conc: 17.14 ng/ml

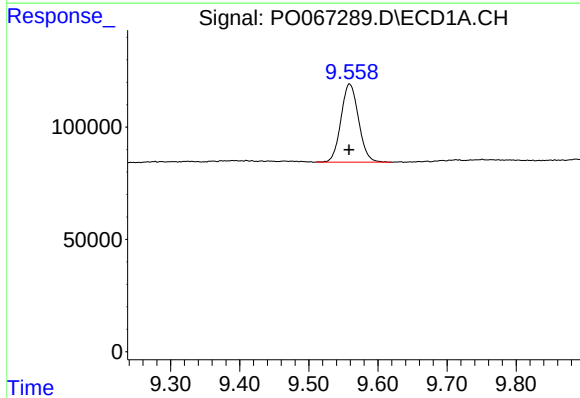


#2 Decachlorobiphenyl

R.T.: 9.559 min
Delta R.T.: 0.000 min
Response: 614519
Conc: 17.47 ng/ml

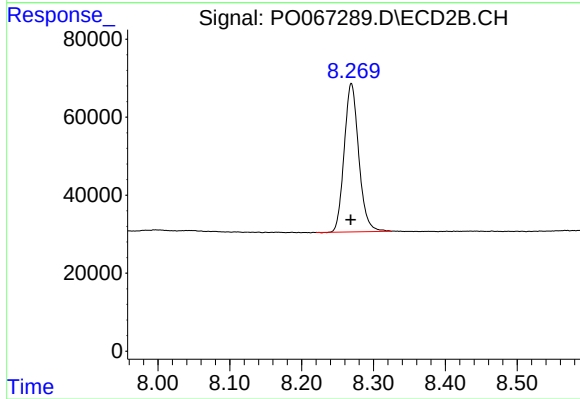

#2 Decachlorobiphenyl


R.T.: 8.269 min
Delta R.T.: 0.000 min
Response: 533624
Conc: 15.40 ng/ml

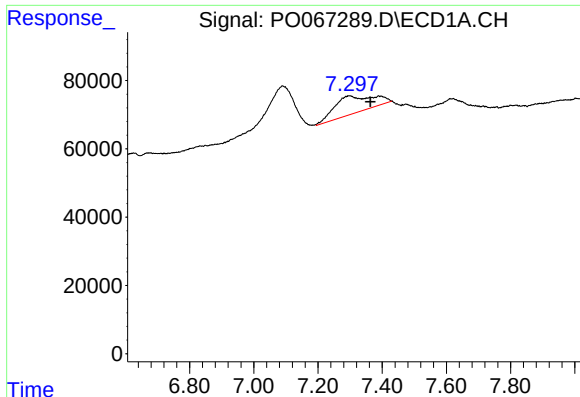

#30 AR-1254-5


R.T.: 7.297 min
Delta R.T.: -0.067 min
Response: 434781
Conc: 274.38 ng/ml

Instrument :
ECD_O
ClientSampleId :

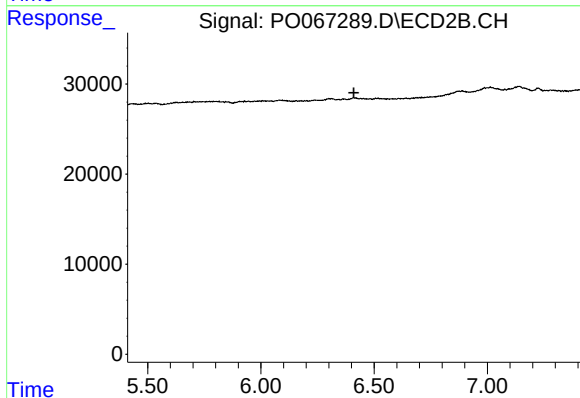


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 6.410 min
Response: 0
Conc: N.D.

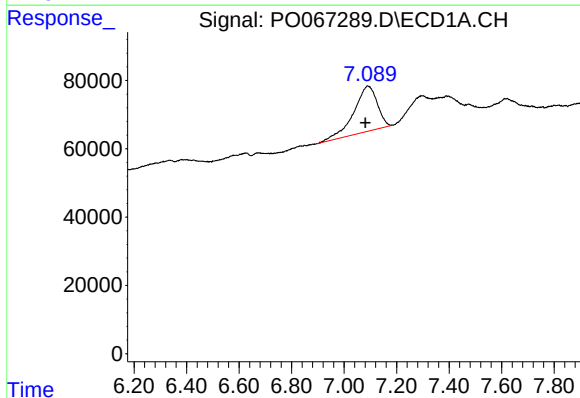


#32 AR-1260-2

R.T.: 7.089 min
Delta R.T.: 0.007 min
Response: 825597
Conc: 350.28 ng/ml

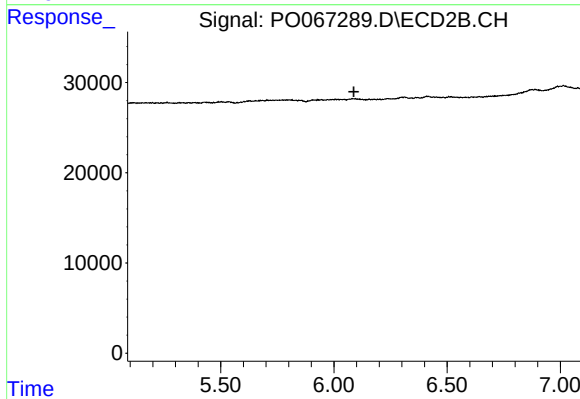

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.088 min
Response: 0
Conc: N.D.

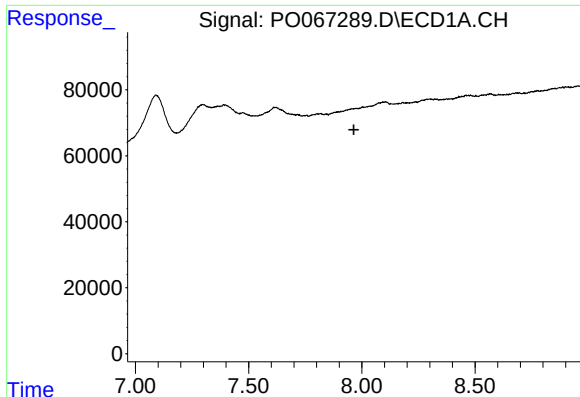

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 7.965 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

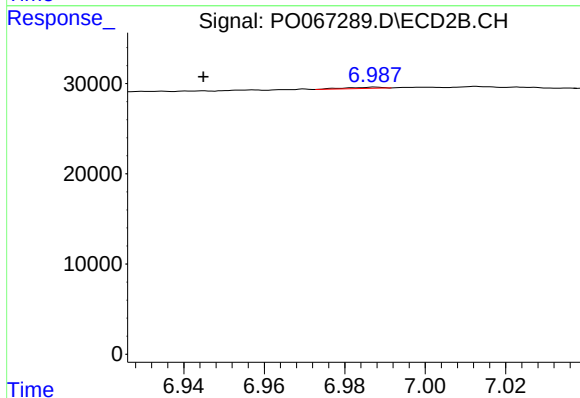


#35 AR-1260-5

R.T.: 6.988 min
Delta R.T.: 0.043 min
Response: 825
Conc: 0.25 ng/ml

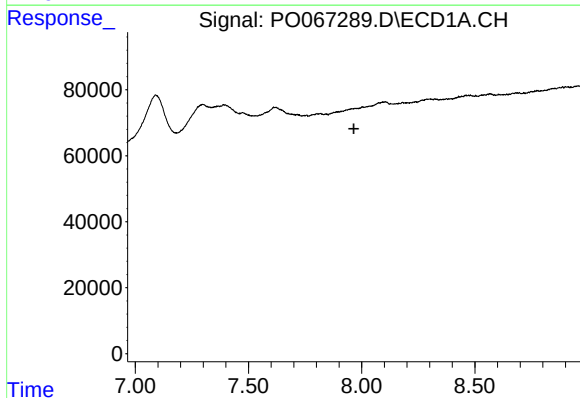


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T.: 7.966 min
Response: 0
Conc: N.D.

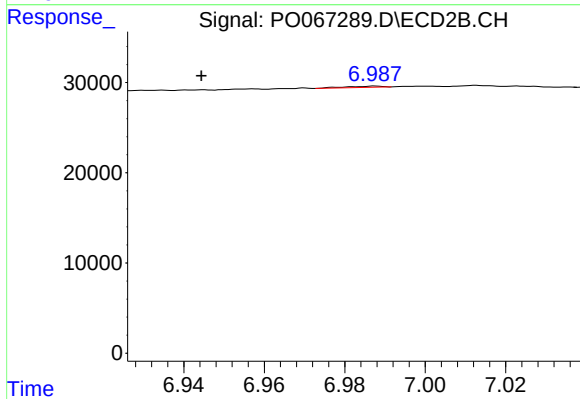

#37 AR-1262-2


R.T.: 6.988 min
Delta R.T.: 0.043 min
Response: 825
Conc: 0.30 ng/ml

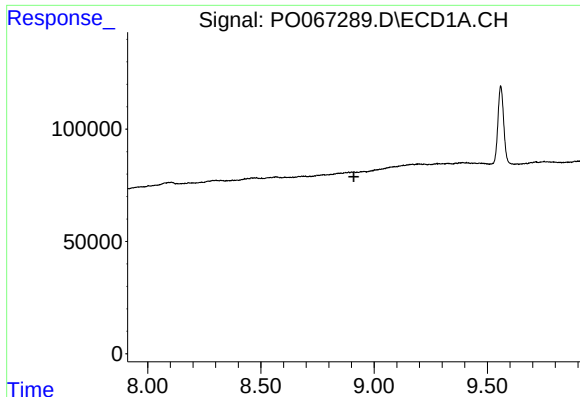

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 8.910 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

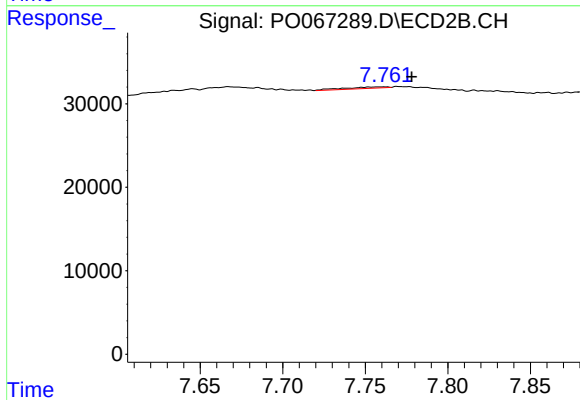


#40 AR-1262-5

R.T.: 7.761 min
Delta R.T.: -0.017 min
Response: 3270
Conc: 3.11 ng/ml

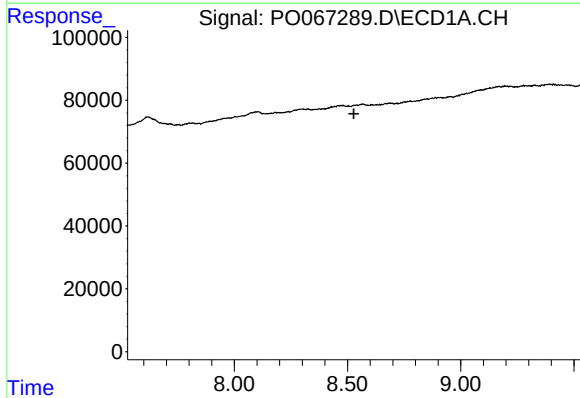


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 8.528 min
Response: 0
Conc: N.D.

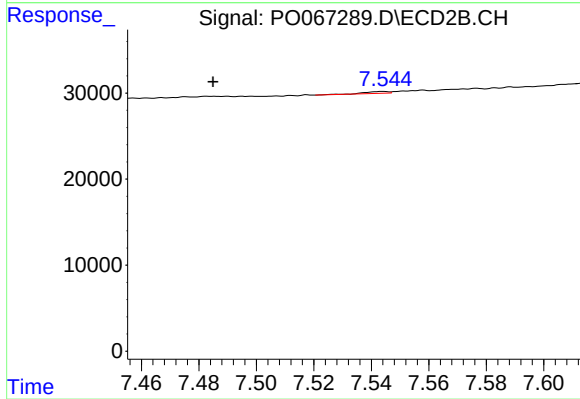

#43 AR-1268-3


R.T.: 7.544 min
Delta R.T.: 0.059 min
Response: 1325
Conc: 0.47 ng/ml

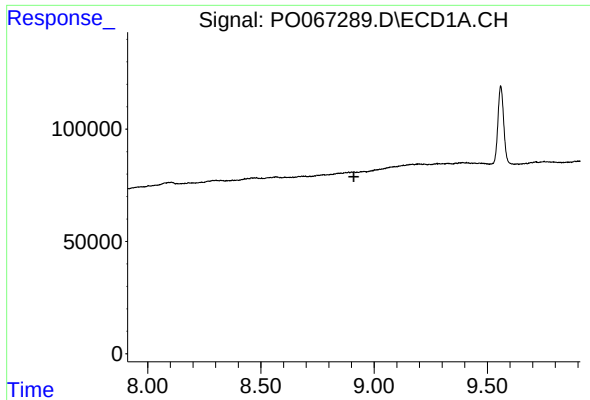

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 8.910 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

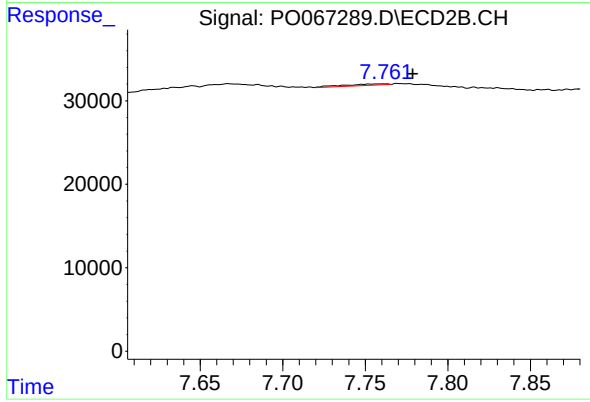

#44 AR-1268-4

R.T.: 7.761 min
Delta R.T.: -0.017 min
Response: 3270
Conc: 2.60 ng/ml