

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031620\
 Data File : P0067293.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Mar 2020 21:50
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 04:20:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 17 02:39:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.107	3.398	670219	314441	25.382	19.788
2) SA Decachlor...	9.560	8.268	723534	708283	20.572	20.437
Target Compounds						
45) L9 AR-1268-5	0.000	8.044	0	849	N.D.	0.086 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031620\
Data File : P0067293.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Mar 2020 21:50
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 04:20:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031620.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 17 02:39:09 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

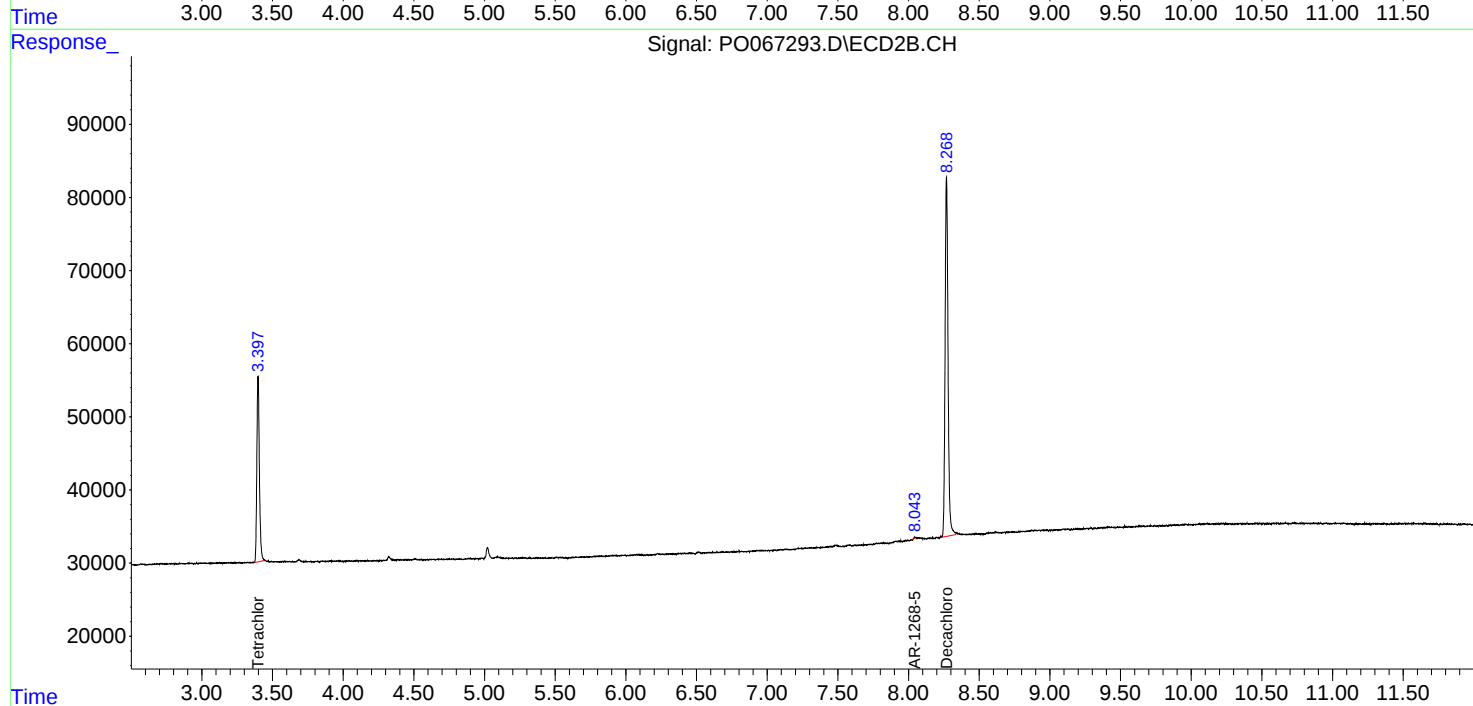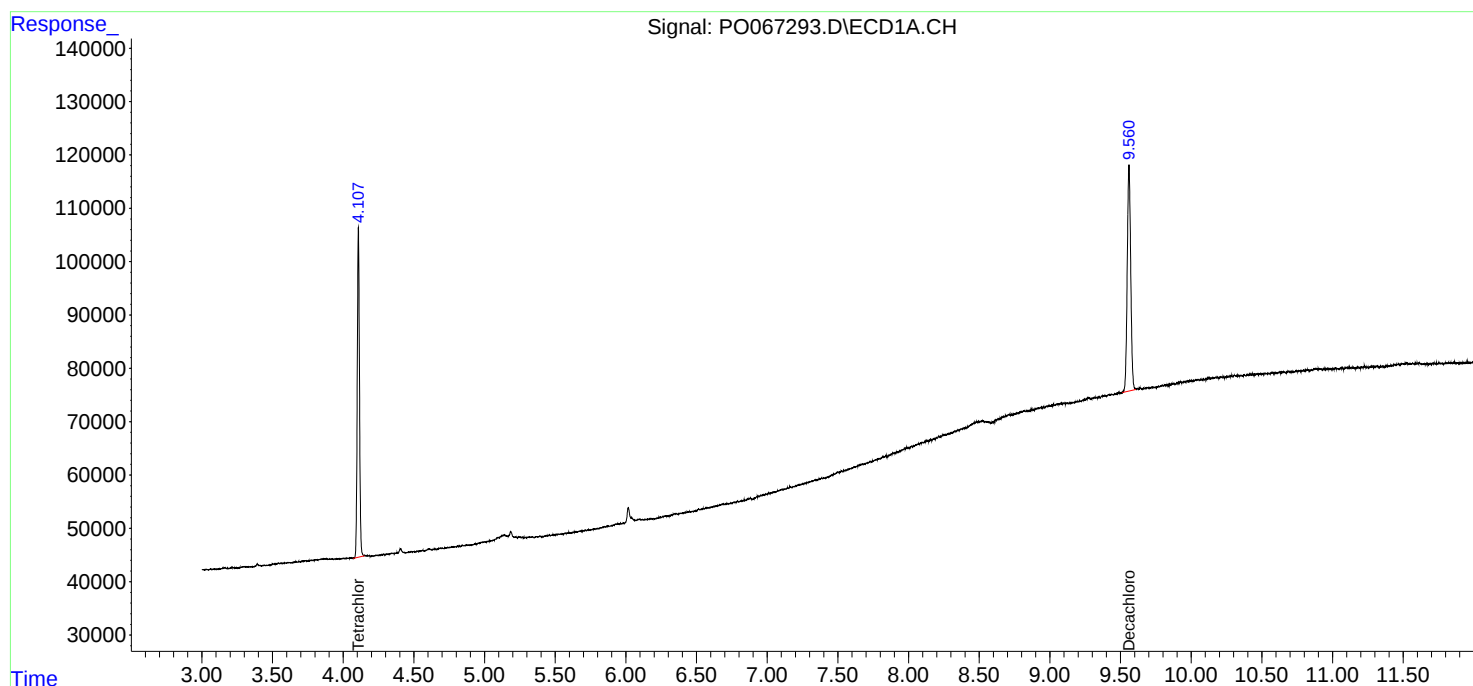


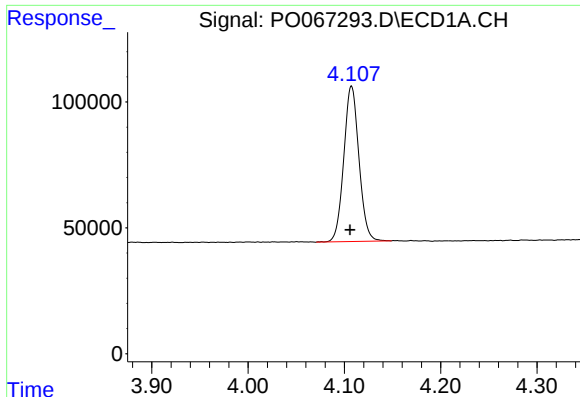

#1 Tetrachloro-m-xylene


R.T.: 4.107 min
Delta R.T.: 0.001 min
Response: 670219
Conc: 25.38 ng/ml

Instrument :
ECD_O
ClientSampleId :

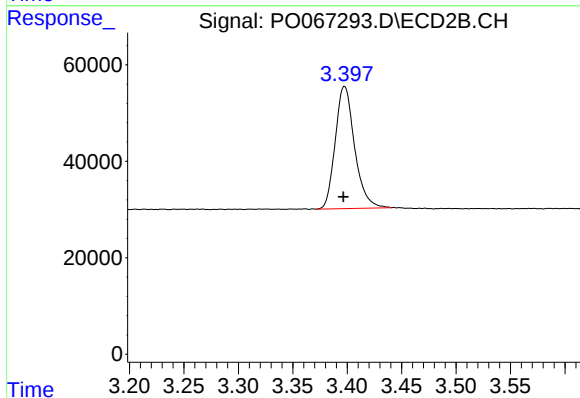


#1 Tetrachloro-m-xylene

R.T.: 3.398 min
Delta R.T.: 0.001 min
Response: 314441
Conc: 19.79 ng/ml

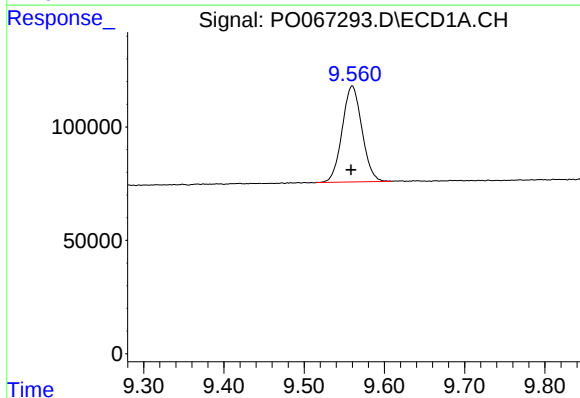


#2 Decachlorobiphenyl

R.T.: 9.560 min
Delta R.T.: 0.002 min
Response: 723534
Conc: 20.57 ng/ml

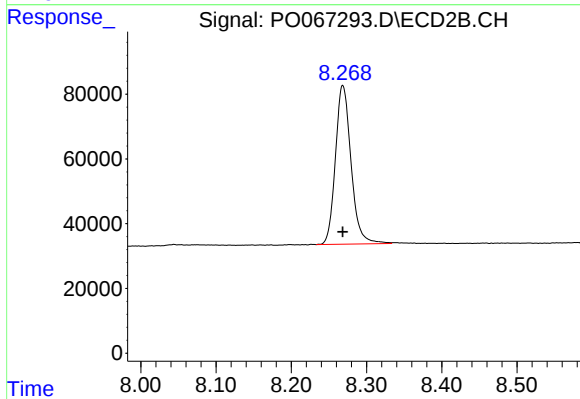

#2 Decachlorobiphenyl


R.T.: 8.268 min
Delta R.T.: 0.000 min
Response: 708283
Conc: 20.44 ng/ml

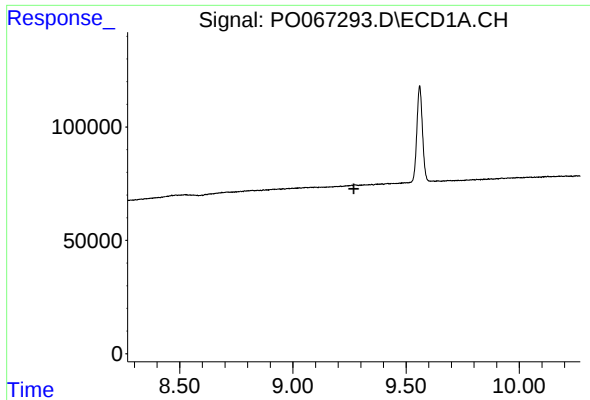

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.269 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

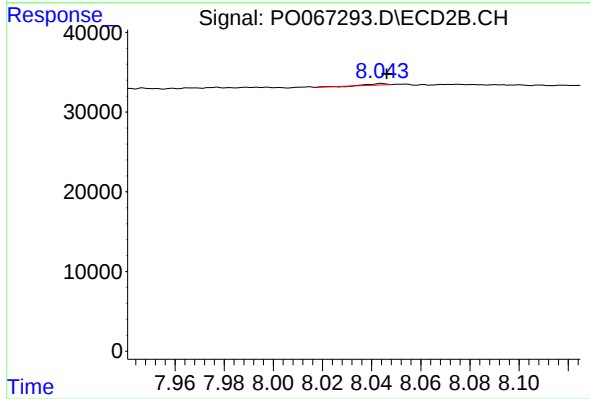

#45 AR-1268-5

R.T.: 8.044 min
Delta R.T.: -0.002 min
Response: 849
Conc: 0.09 ng/ml