

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031620\
 Data File : P0067299.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Mar 2020 23:48
 Operator : DD\AJ
 Sample : L1917-09
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 04:22:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 17 02:39:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.109	3.400	657736	298284	24.909	18.771
2) SA Decachlor...	9.560	8.268	518768	449552	14.750	12.971
Target Compounds						
7) L1 AR-1016-5	0.000	4.883	0	14105	N.D.	21.585 #
15) L3 AR-1232-5	0.000	4.883	0	14105	N.D.	68.131 #
20) L4 AR-1242-5	0.000	5.257	0	11058	N.D.	22.627 #
24) L5 AR-1248-4	0.000	4.883	0	14105	N.D.	21.482 #
25) L5 AR-1248-5	0.000	5.257	0	11058	N.D.	17.205 #
26) L6 AR-1254-1	0.000	5.257	0	11058	N.D.	10.134 #
32) L7 AR-1260-2	0.000	6.077	0	6471	N.D.	3.588 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031620\
Data File : P0067299.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Mar 2020 23:48
Operator : DD\AJ
Sample : L1917-09
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 04:22:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031620.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 17 02:39:09 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

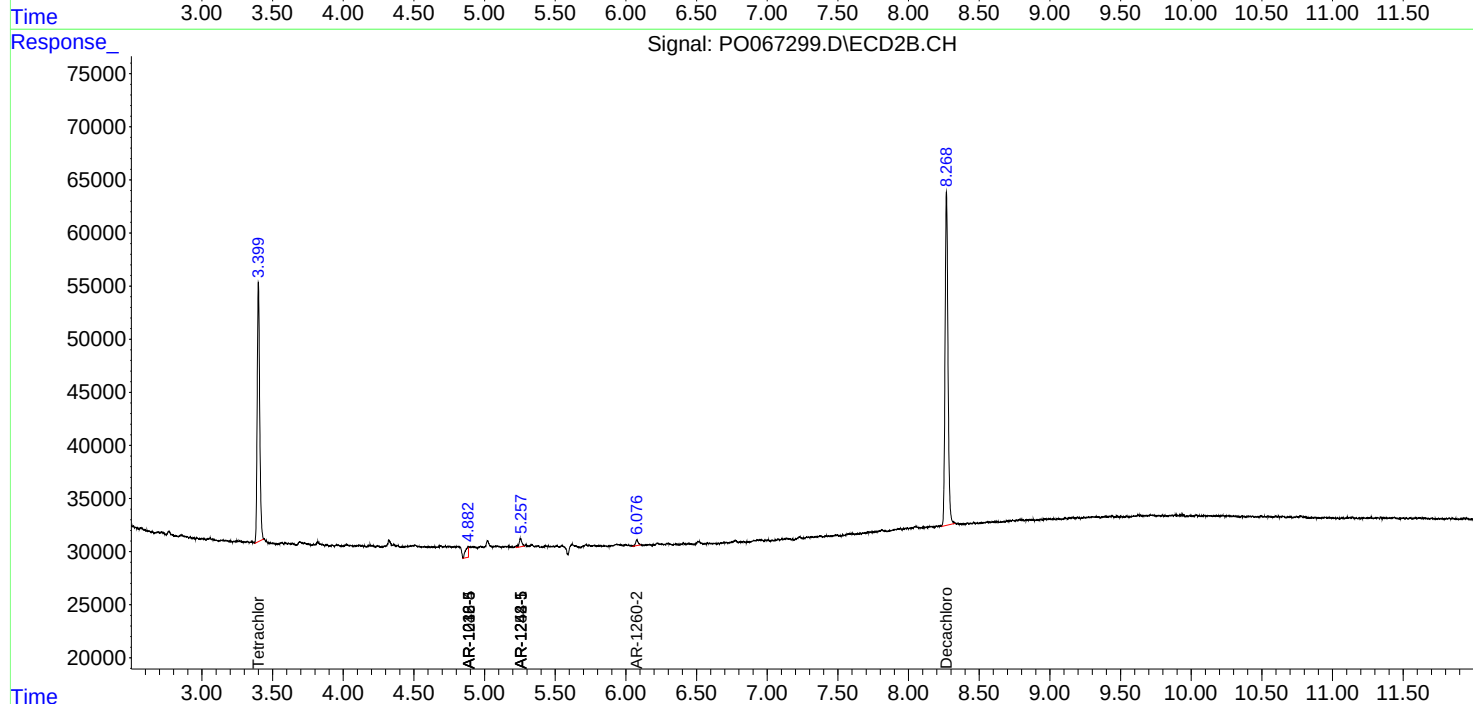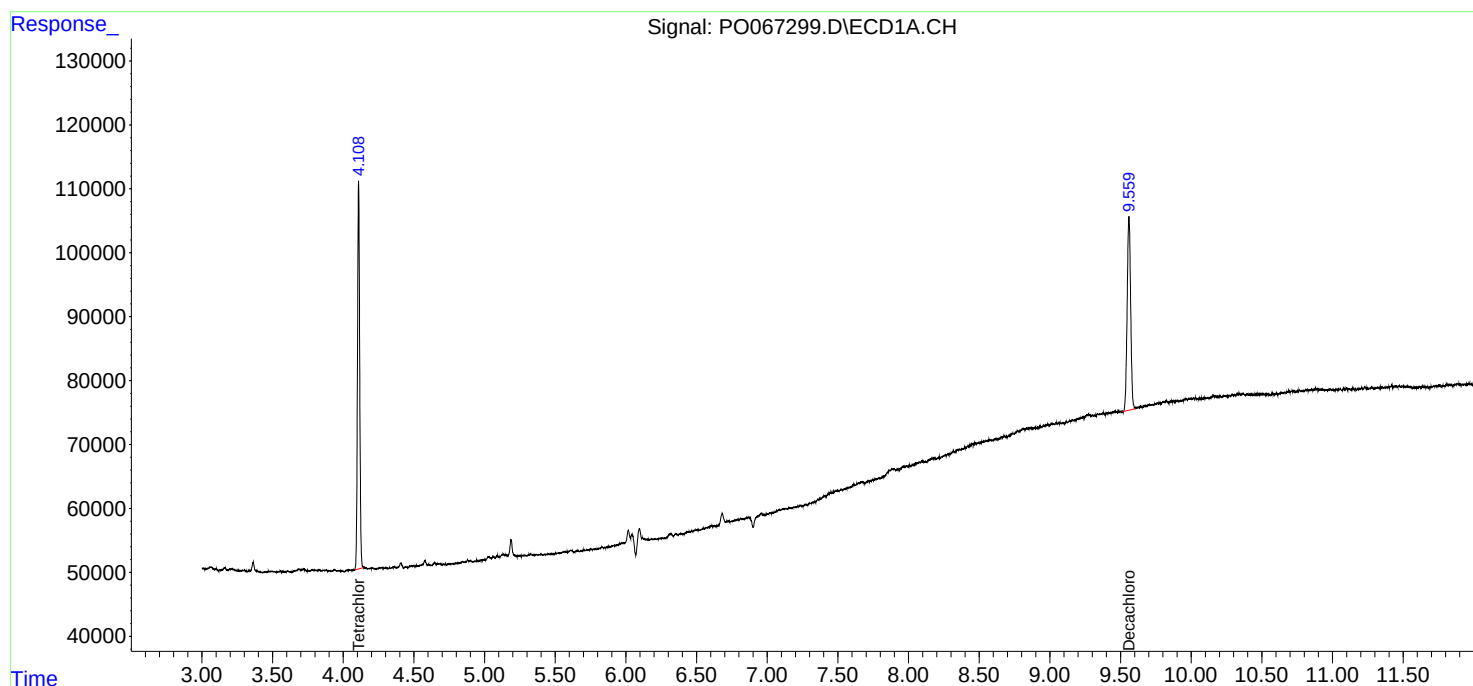


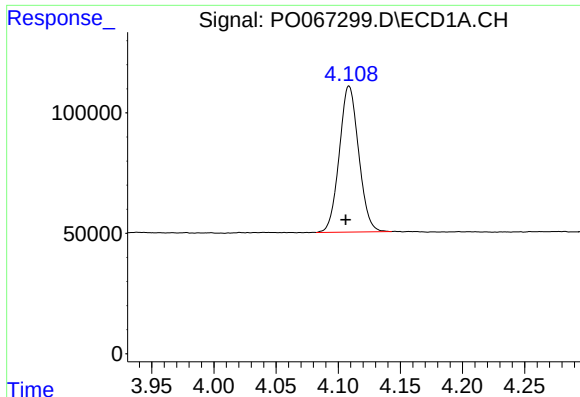

#1 Tetrachloro-m-xylene


R.T.: 4.109 min
Delta R.T.: 0.003 min
Response: 657736
Conc: 24.91 ng/ml

Instrument :
ECD_O
ClientSampleId :

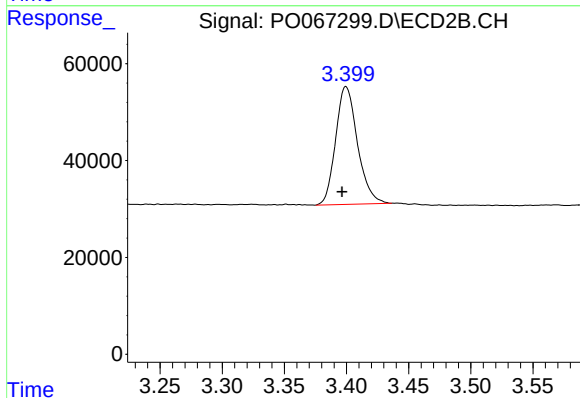


#1 Tetrachloro-m-xylene

R.T.: 3.400 min
Delta R.T.: 0.003 min
Response: 298284
Conc: 18.77 ng/ml

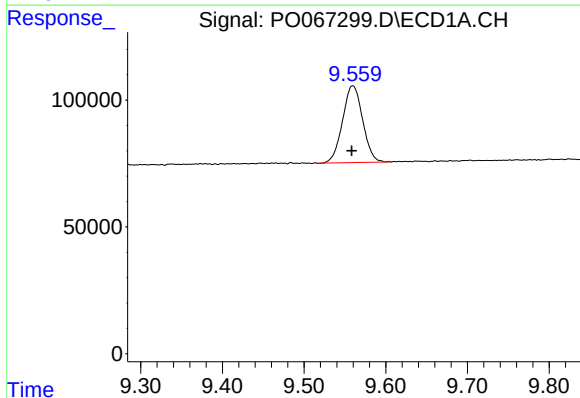


#2 Decachlorobiphenyl

R.T.: 9.560 min
Delta R.T.: 0.001 min
Response: 518768
Conc: 14.75 ng/ml

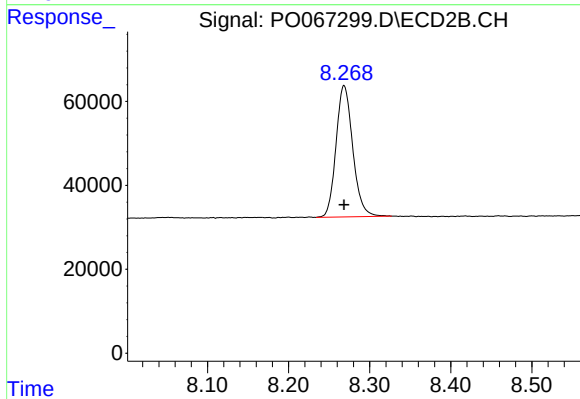

#2 Decachlorobiphenyl


R.T.: 8.268 min
Delta R.T.: 0.000 min
Response: 449552
Conc: 12.97 ng/ml

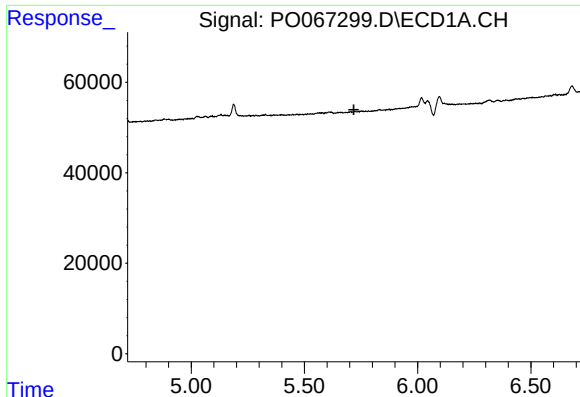

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 5.718 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

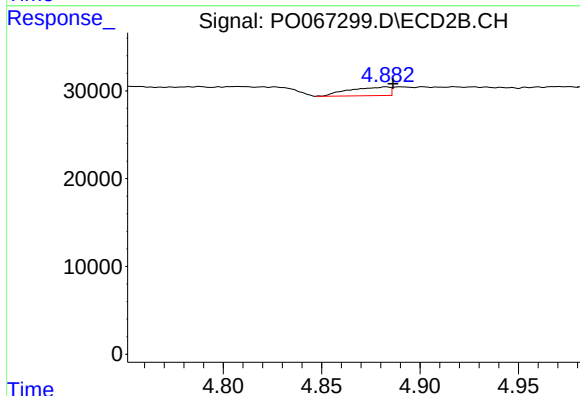


#7 AR-1016-5

R.T.: 4.883 min
Delta R.T.: -0.004 min
Response: 14105
Conc: 21.59 ng/ml

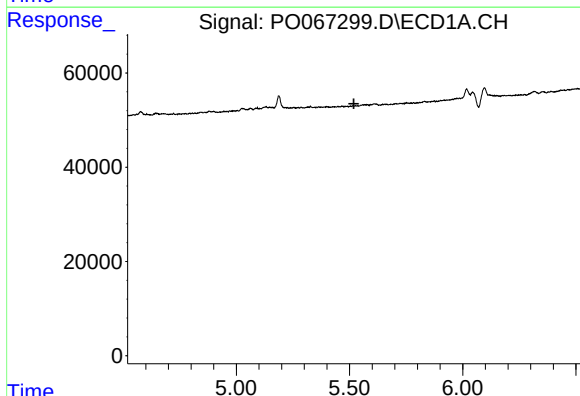


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T.: 5.519 min
Response: 0
Conc: N.D.

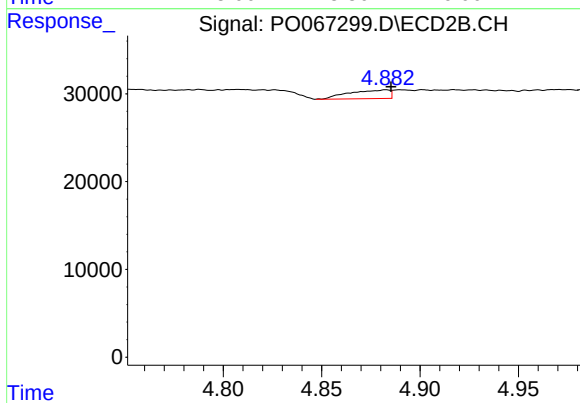

#15 AR-1232-5


R.T.: 4.883 min
Delta R.T.: -0.003 min
Response: 14105
Conc: 68.13 ng/ml

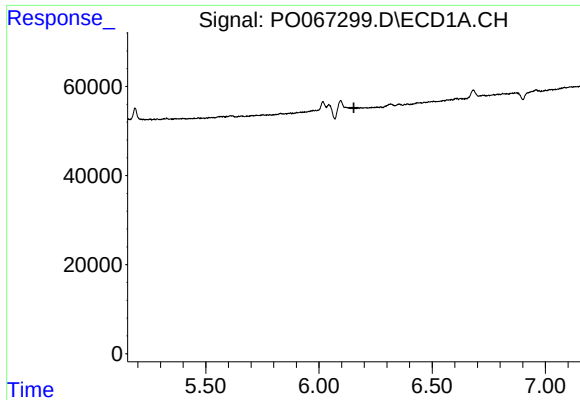

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 6.154 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

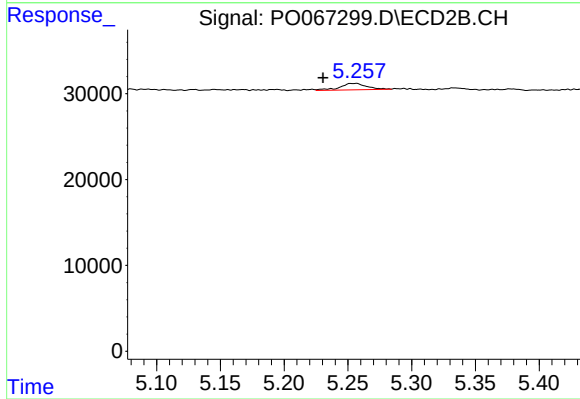


#20 AR-1242-5

R.T.: 5.257 min
Delta R.T.: 0.026 min
Response: 11058
Conc: 22.63 ng/ml

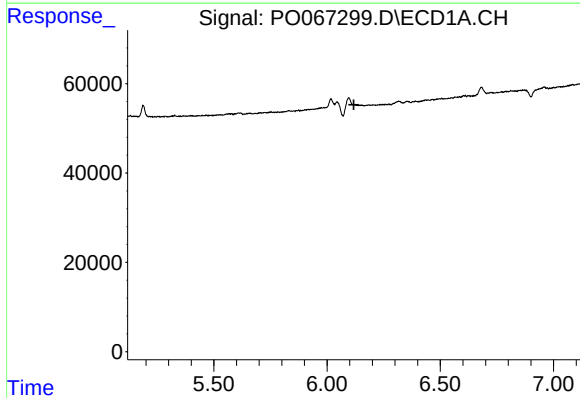


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T.: 6.118 min
Response: 0
Conc: N.D.

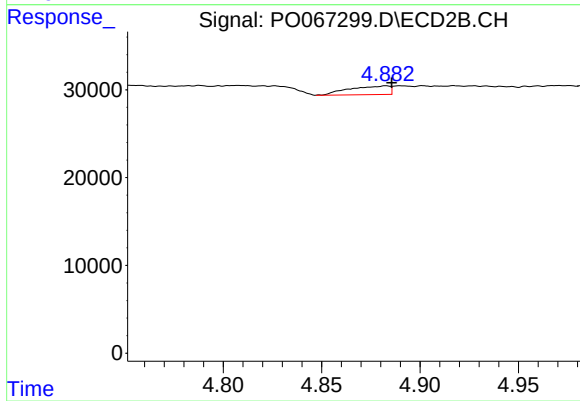

#24 AR-1248-4


R.T.: 4.883 min
Delta R.T.: -0.003 min
Response: 14105
Conc: 21.48 ng/ml

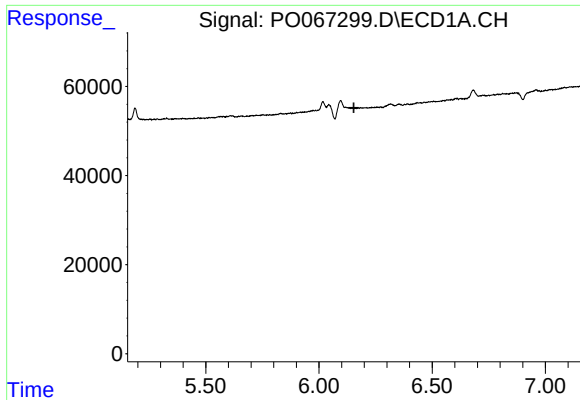

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.154 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

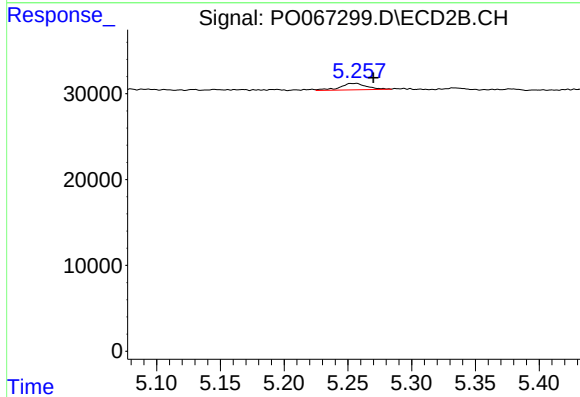


#25 AR-1248-5

R.T.: 5.257 min
Delta R.T.: -0.013 min
Response: 11058
Conc: 17.20 ng/ml

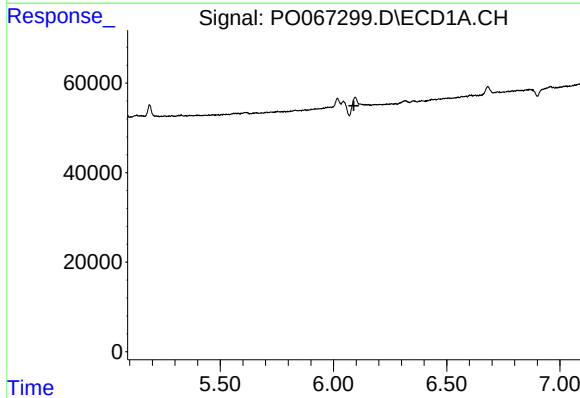


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 6.090 min
Response: 0
Conc: N.D.

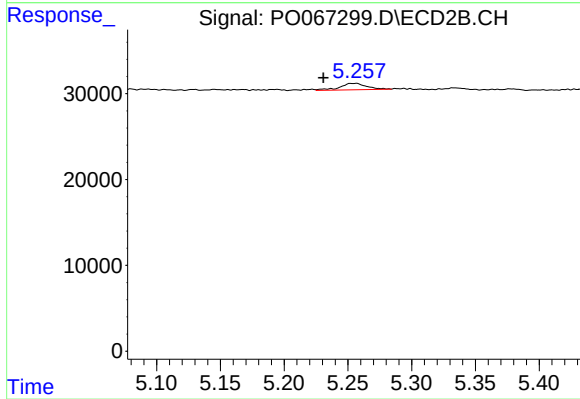

#26 AR-1254-1


R.T.: 5.257 min
Delta R.T.: 0.026 min
Response: 11058
Conc: 10.13 ng/ml

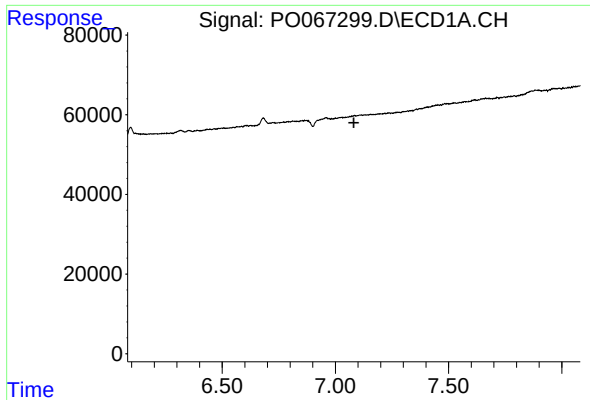

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 7.082 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

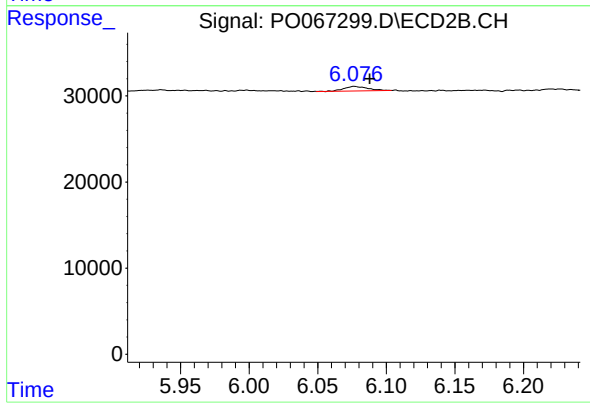

#32 AR-1260-2

R.T.: 6.077 min
Delta R.T.: -0.011 min
Response: 6471
Conc: 3.59 ng/ml