

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031620\
 Data File : P0067284.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Mar 2020 19:19
 Operator : DD\AJ
 Sample : L1934-05 5X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 03-13-E

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 04:17:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 17 02:39:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.108	3.397	124980	50680	4.733m	3.189 #
2) SA Decachlor...	9.561	8.271	117720	128533	3.347	3.709

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031620\
Data File : P0067284.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Mar 2020 19:19
Operator : DD\AJ
Sample : L1934-05 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
03-13-E

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 04:17:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031620.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 17 02:39:09 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

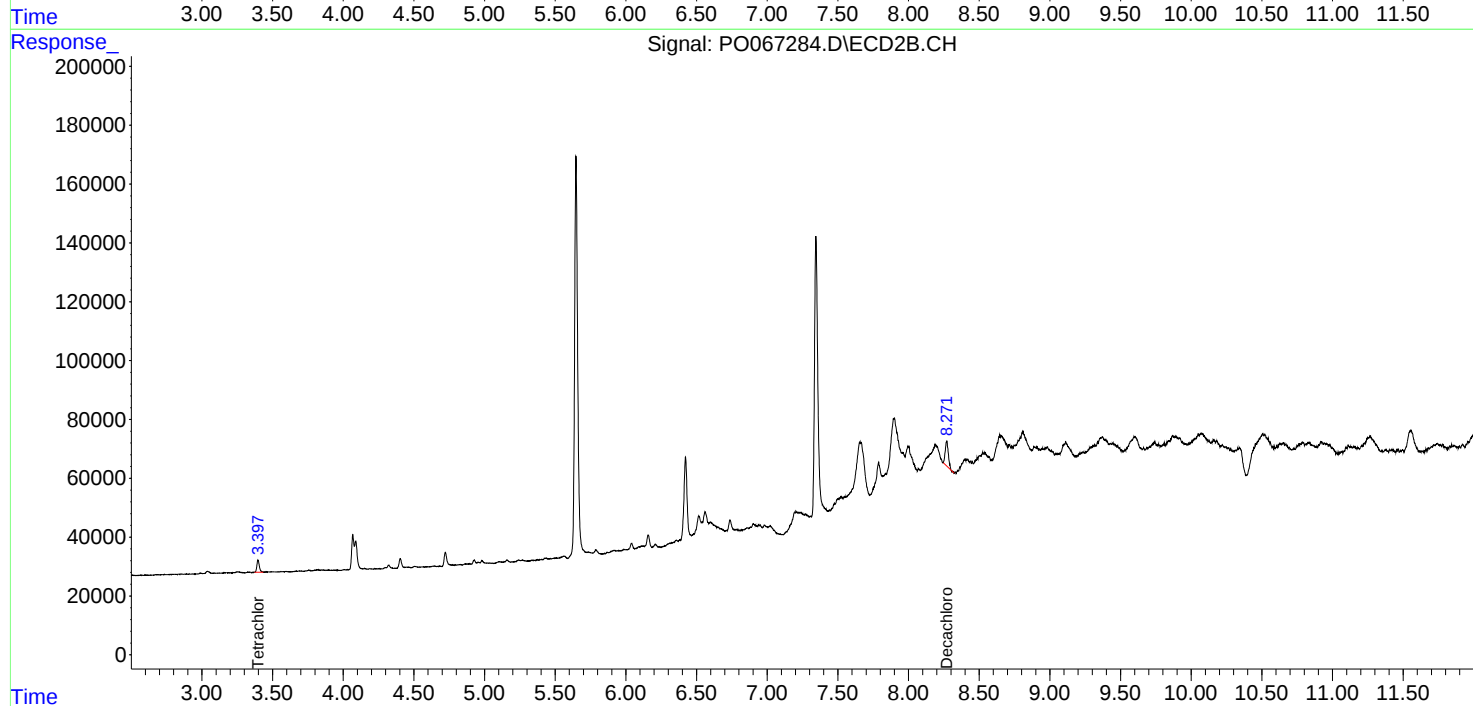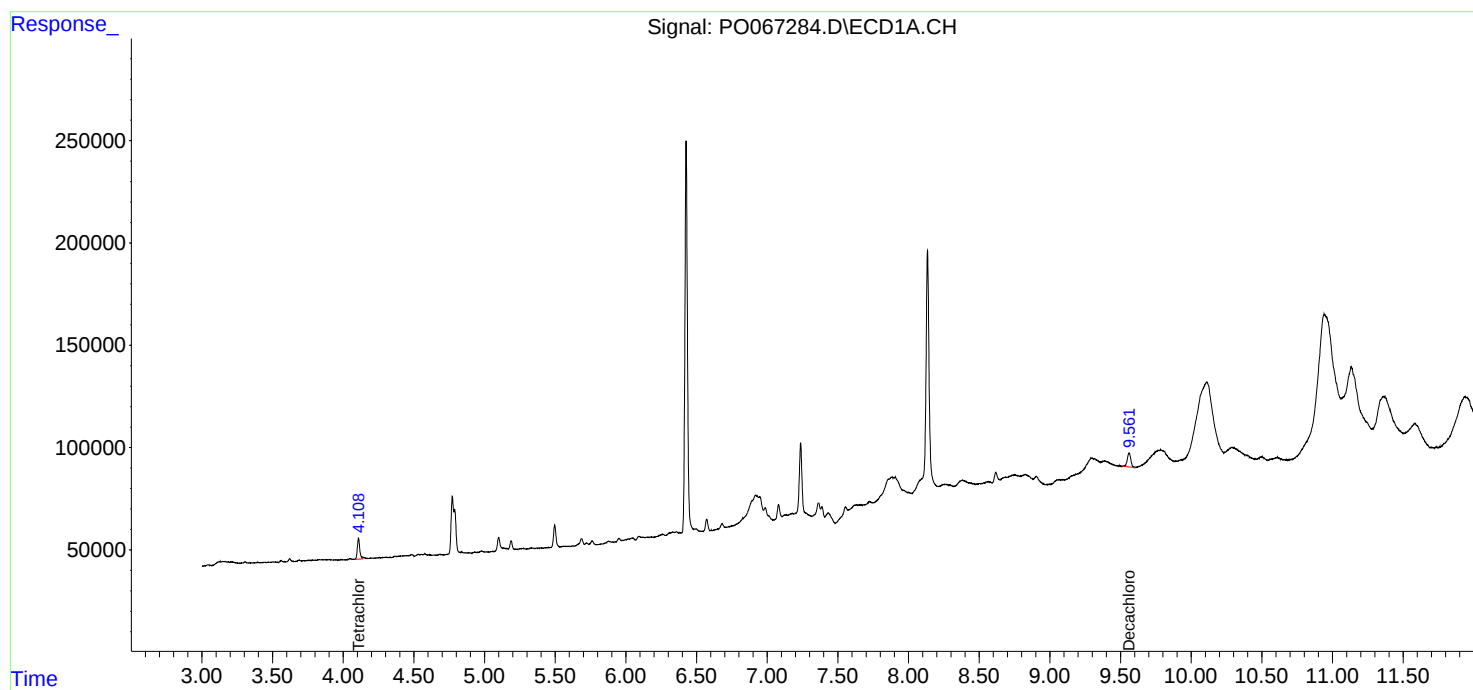


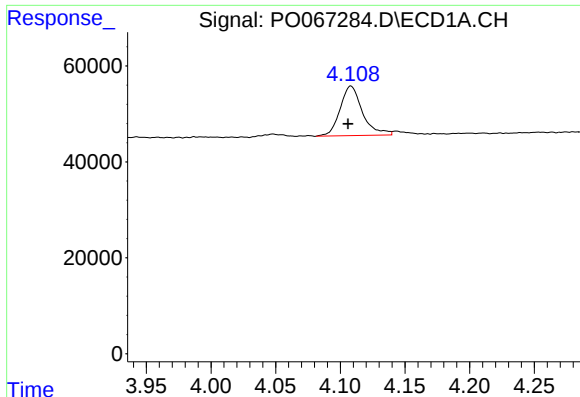

#1 Tetrachloro-m-xylene


R.T.: 4.108 min
Delta R.T.: 0.002 min
Response: 124980
Conc: 4.73 ng/ml m

Instrument :
ECD_O
ClientSampleId :
03-13-E

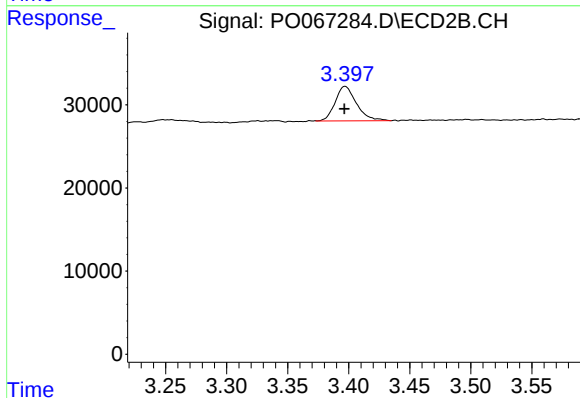


#1 Tetrachloro-m-xylene

R.T.: 3.397 min
Delta R.T.: 0.000 min
Response: 50680
Conc: 3.19 ng/ml

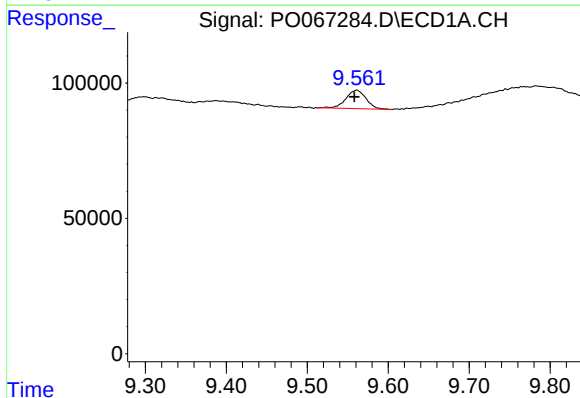

#2 Decachlorobiphenyl

R.T.: 9.561 min
Delta R.T.: 0.002 min
Response: 117720
Conc: 3.35 ng/ml

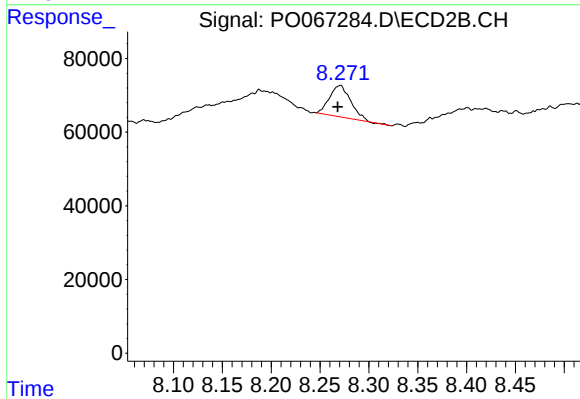

#2 Decachlorobiphenyl

R.T.: 8.271 min
Delta R.T.: 0.003 min
Response: 128533
Conc: 3.71 ng/ml