

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031620\
 Data File : P0067296.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Mar 2020 22:58
 Operator : DD\AJ
 Sample : L1917-06
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CBH-140

Manual Integrations
 APPROVED

Sohil
 3/17/2020 2:07:35 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 04:21:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 17 02:39:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.108	3.398	321180	121035	12.163	7.617m#
2) SA Decachlor...	9.560	8.268	121019	105563	3.441	3.046

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031620\
Data File : P0067296.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Mar 2020 22:58
Operator : DD\AJ
Sample : L1917-06
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CBH-140


Manual Integrations
APPROVED

Sohil
3/17/2020 2:07:35 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 04:21:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031620.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 17 02:39:09 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

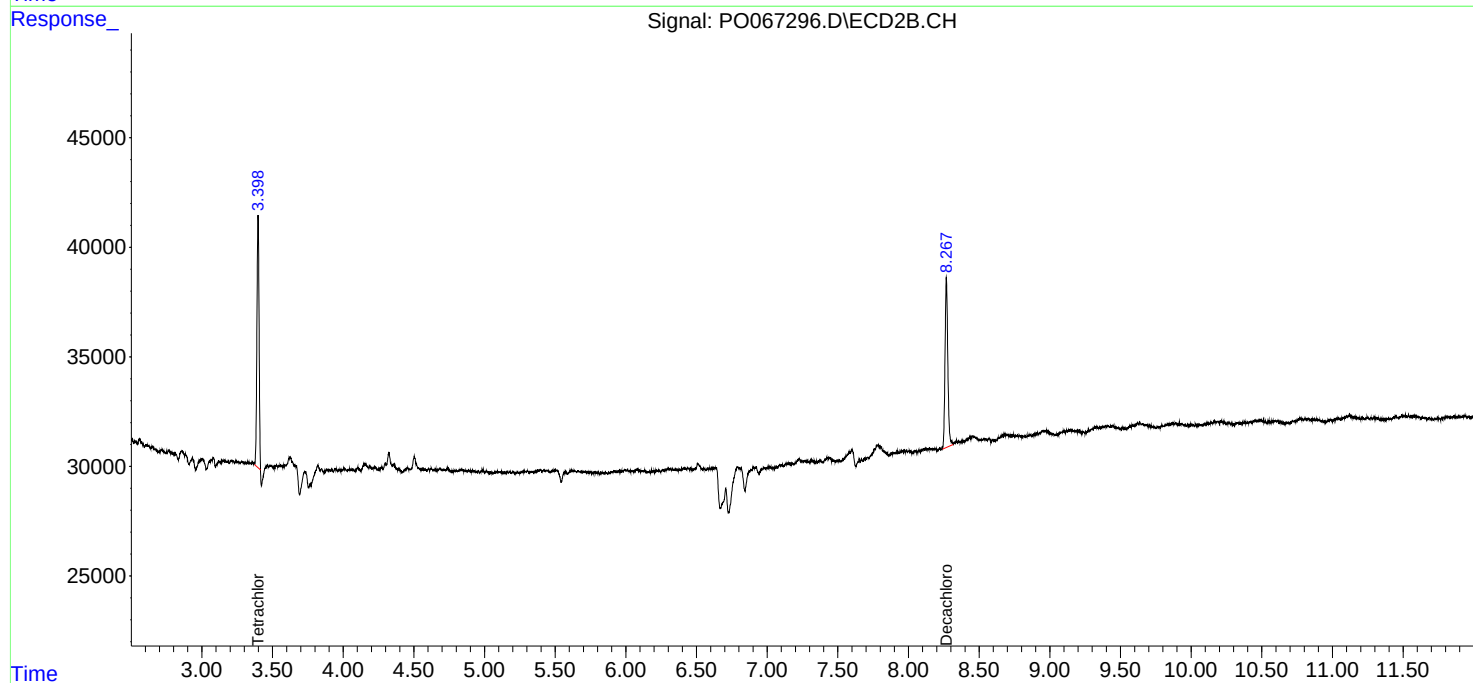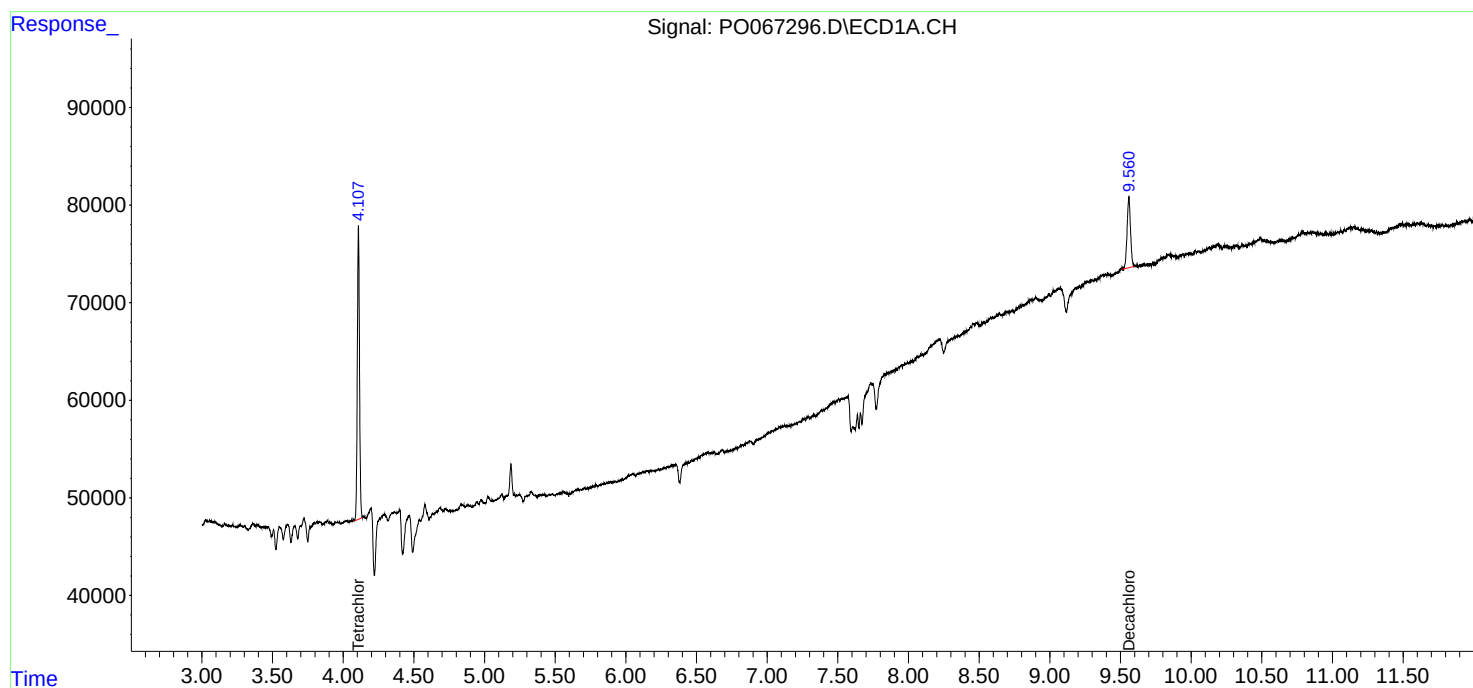

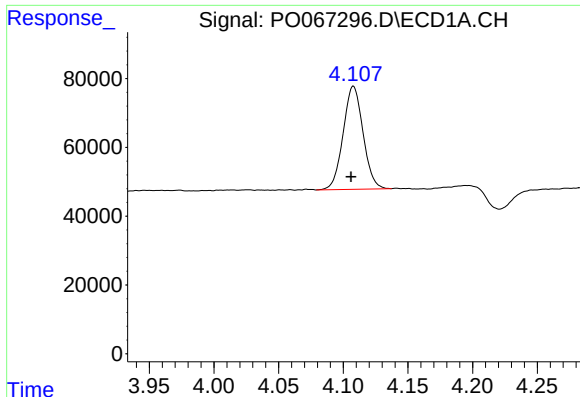


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.002 min
Response: 321180
Conc: 12.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
CBH-140


Manual Integrations
APPROVED

Sohil
3/17/2020 2:07:35 PM

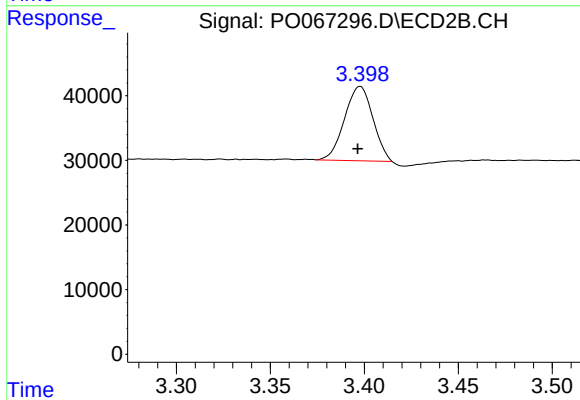


#1 Tetrachloro-m-xylene

R.T.: 3.398 min
Delta R.T.: 0.000 min
Response: 121035
Conc: 7.62 ng/ml m

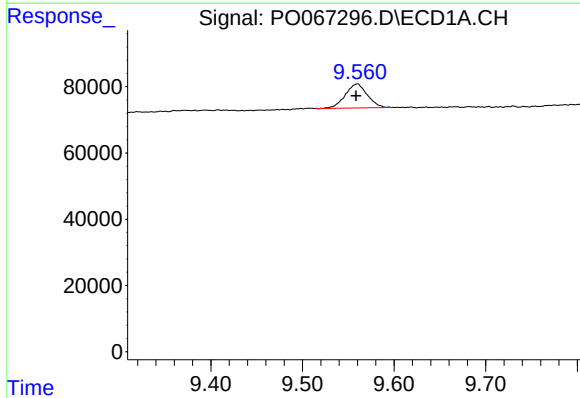

#2 Decachlorobiphenyl

R.T.: 9.560 min
Delta R.T.: 0.002 min
Response: 121019
Conc: 3.44 ng/ml

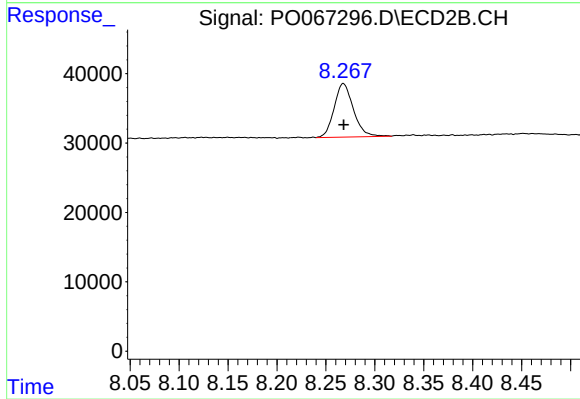

#2 Decachlorobiphenyl

R.T.: 8.268 min
Delta R.T.: 0.000 min
Response: 105563
Conc: 3.05 ng/ml