

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031720\
 Data File : P0067317.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Mar 2020 12:22
 Operator : DD\AJ
 Sample : L1913-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MK-031220-0-2-COMP-B4

Manual Integrations
 APPROVED

Sohil
 3/18/2020 3:03:44 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 16:06:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 17 02:39:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.106	3.397	760192	311344	28.789m	19.593 #
2) SA Decachlor...	9.560	8.271	656926	493076	18.678	14.227

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031720\
Data File : P0067317.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Mar 2020 12:22
Operator : DD\AJ
Sample : L1913-14
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MK-031220-0-2-COMP-B4


Manual Integrations
APPROVED

Sohil
3/18/2020 3:03:44 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 16:06:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031620.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 17 02:39:09 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

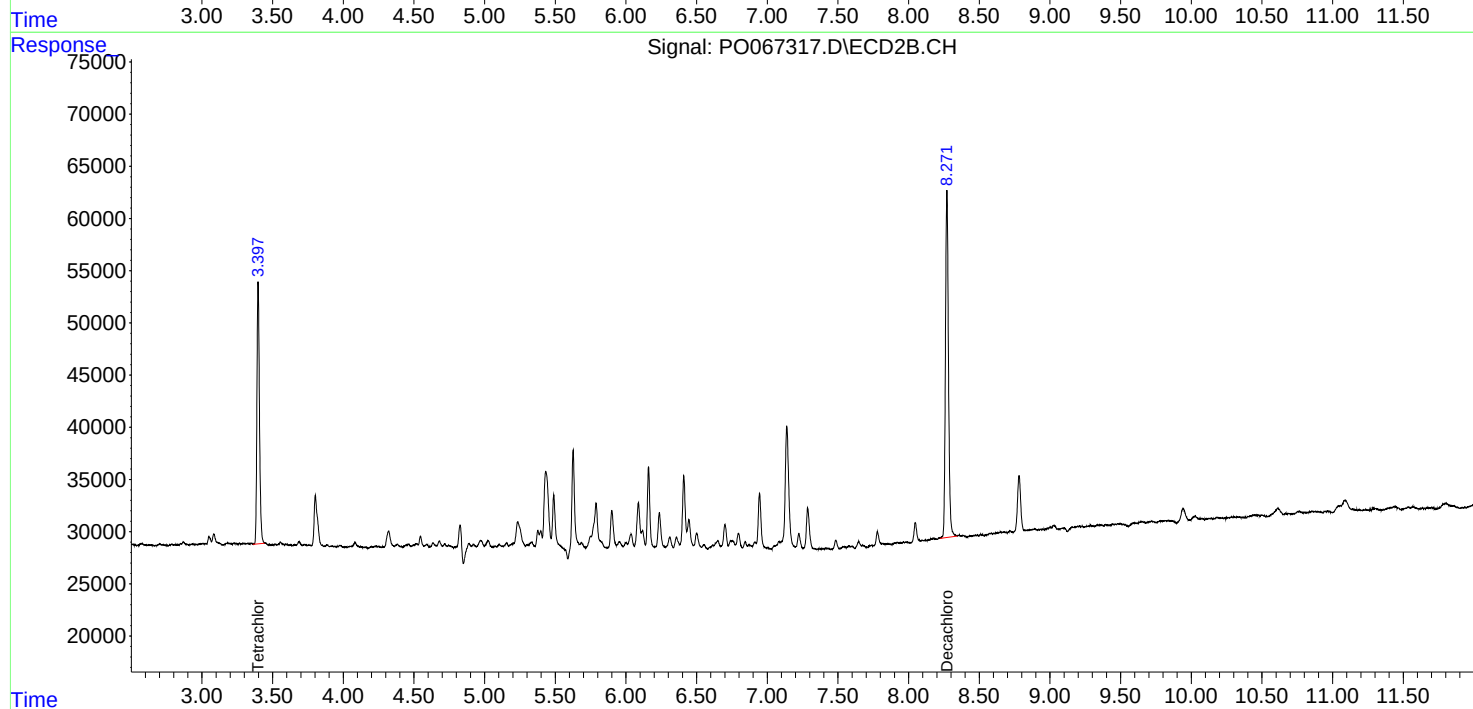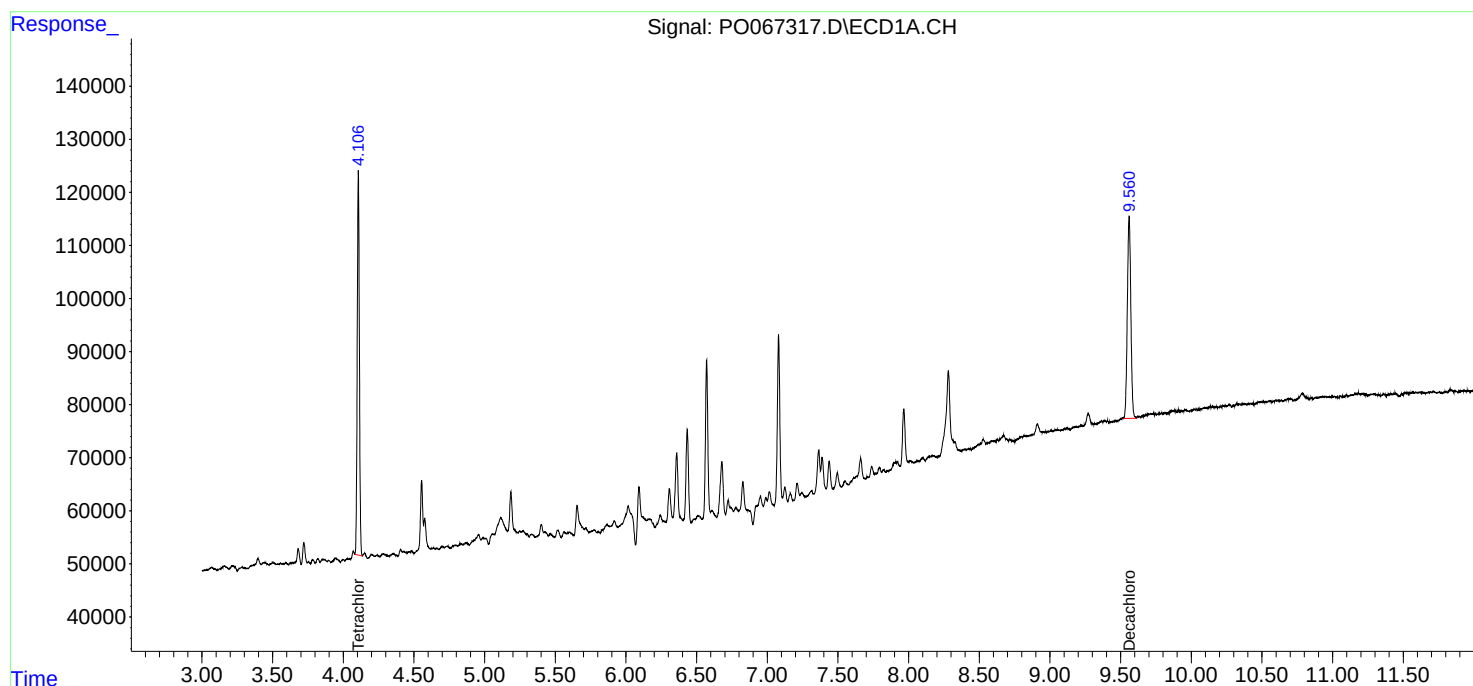

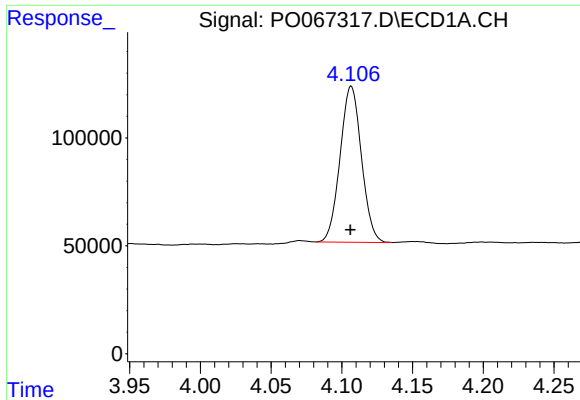


#1 Tetrachloro-m-xylene

R.T.: 4.106 min
Delta R.T.: 0.000 min
Response: 760192
Conc: 28.79 ng/ml m

Instrument :
ECD_O
ClientSampleId :
MK-031220-0-2-COMP-B4


Manual Integrations
APPROVED

Sohil
3/18/2020 3:03:44 PM

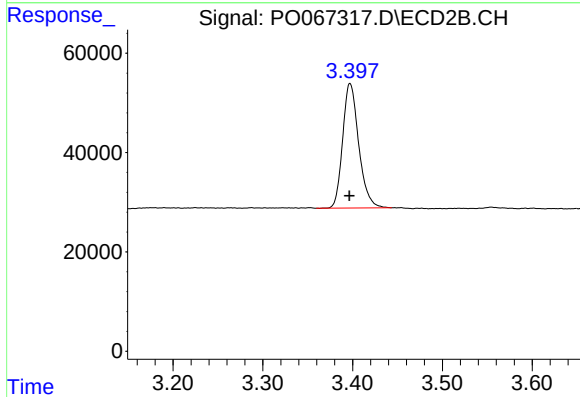


#1 Tetrachloro-m-xylene

R.T.: 3.397 min
Delta R.T.: 0.000 min
Response: 311344
Conc: 19.59 ng/ml

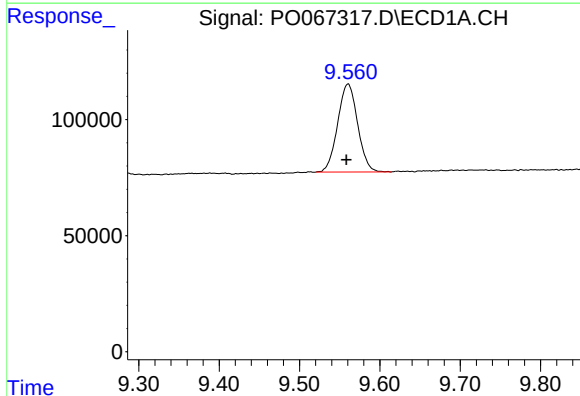

#2 Decachlorobiphenyl

R.T.: 9.560 min
Delta R.T.: 0.002 min
Response: 656926
Conc: 18.68 ng/ml

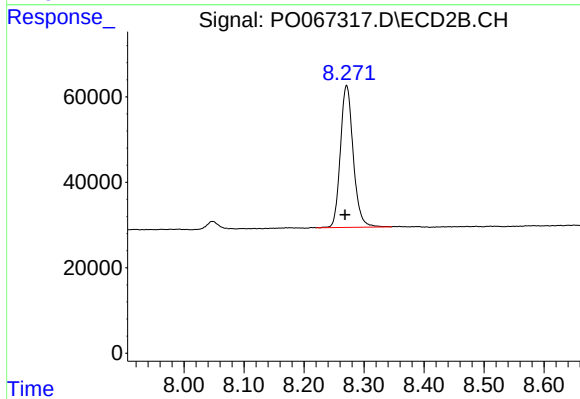

#2 Decachlorobiphenyl

R.T.: 8.271 min
Delta R.T.: 0.003 min
Response: 493076
Conc: 14.23 ng/ml