

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031919\
 Data File : P0054462.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Mar 2019 19:56
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 07:15:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 20 07:14:02 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.341	3.653	58657652	8772516	19.342	20.444
2) SA Decachlor...	9.980	8.655	12112853	7566134	19.413	20.740

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031919\
Data File : P0054462.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Mar 2019 19:56
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 07:15:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 20 07:14:02 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

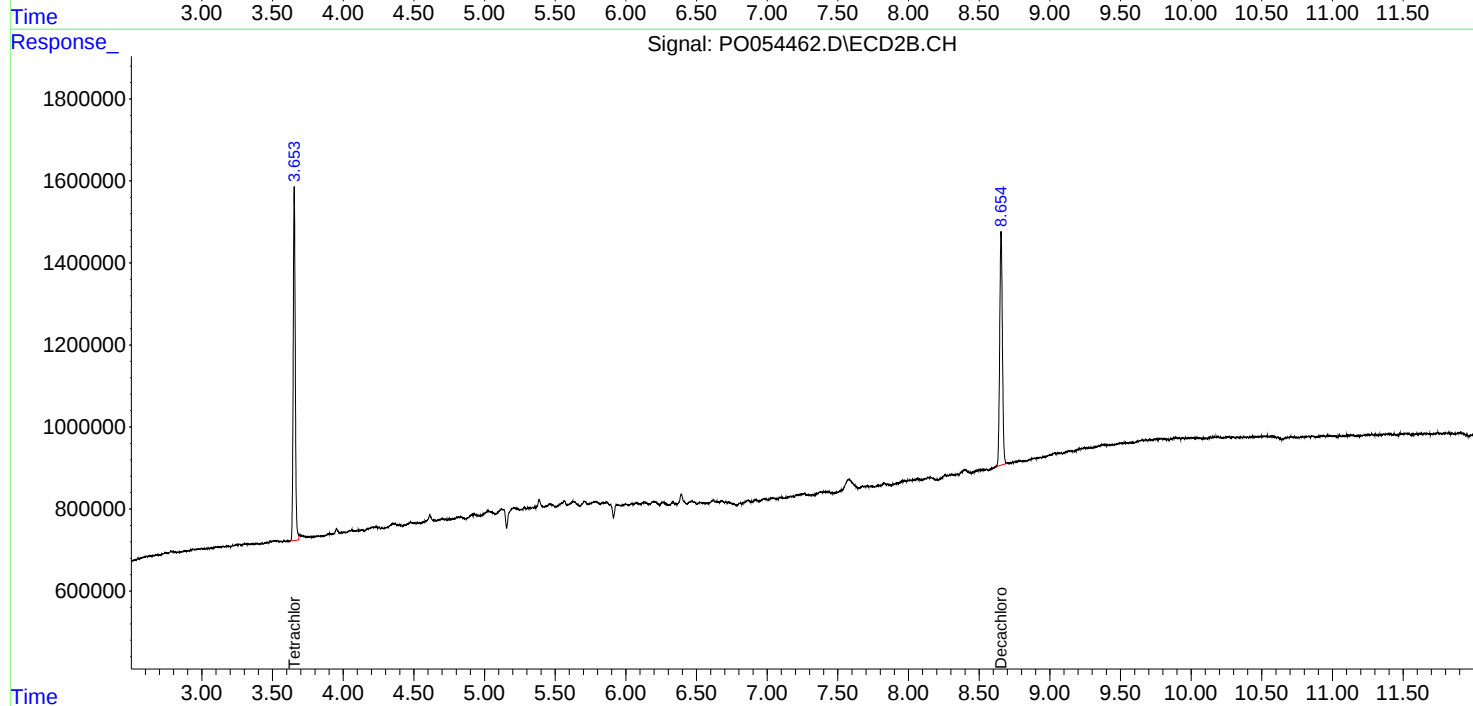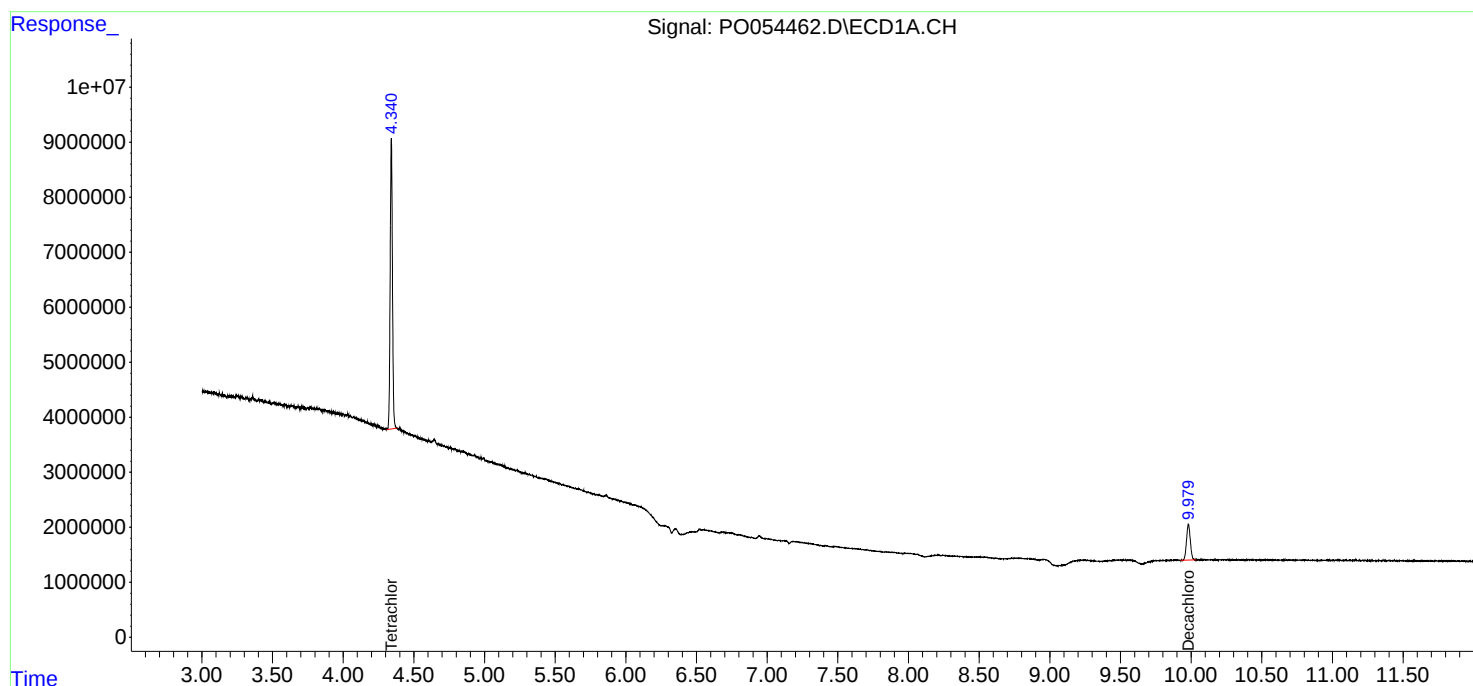


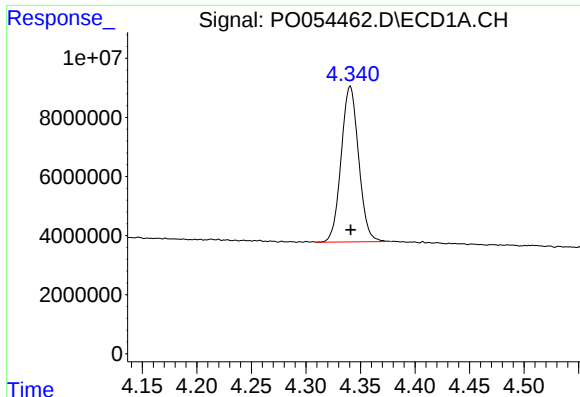

#1 Tetrachloro-m-xylene


R.T.: 4.341 min
Delta R.T.: 0.000 min
Response: 58657652
Conc: 19.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

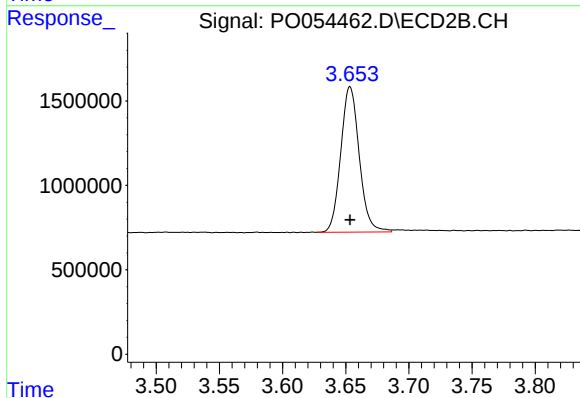


#1 Tetrachloro-m-xylene

R.T.: 3.653 min
Delta R.T.: 0.000 min
Response: 8772516
Conc: 20.44 ng/ml

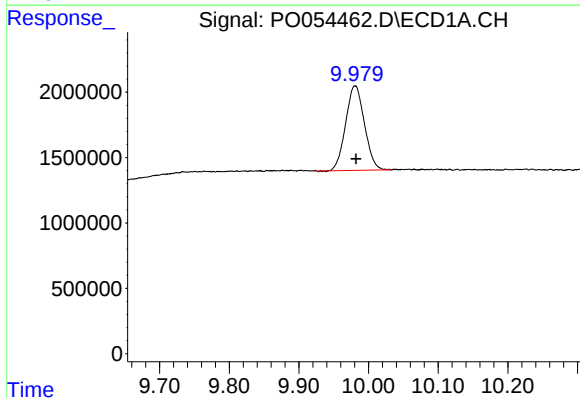

#2 Decachlorobiphenyl

R.T.: 9.980 min
Delta R.T.: -0.002 min
Response: 12112853
Conc: 19.41 ng/ml

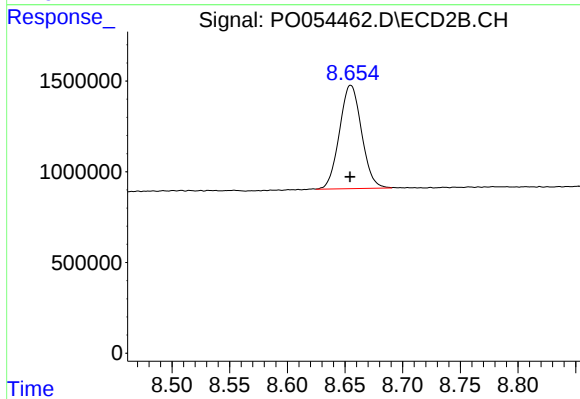

#2 Decachlorobiphenyl

R.T.: 8.655 min
Delta R.T.: 0.000 min
Response: 7566134
Conc: 20.74 ng/ml