

Data Path : P:\HPCHEM1\ECD 0\Data\P0032018\
 Data File : P0043194.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Mar 2018 16:01
 Operator : SM/UA
 Sample : J1953-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 031418-TIDO-F-D-S

Manual Integrations
 APPROVED

ugo
 3/22/2018 2:24:17 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 21 04:45:21 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0022118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 26 14:24:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.080	3.333	2730349	3972771	11.022m	10.751
2) SA Decachlor...	9.441	8.106	2759851	3594109	10.920	9.320

Target Compounds

 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\P0032018\
Data File : P0043194.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Mar 2018 16:01
Operator : SM/UA
Sample : J1953-02
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
031418-TIDO-F-D-S


Manual Integrations
APPROVED

ugo
3/22/2018 2:24:17 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 21 04:45:21 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0022118.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 26 14:24:10 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

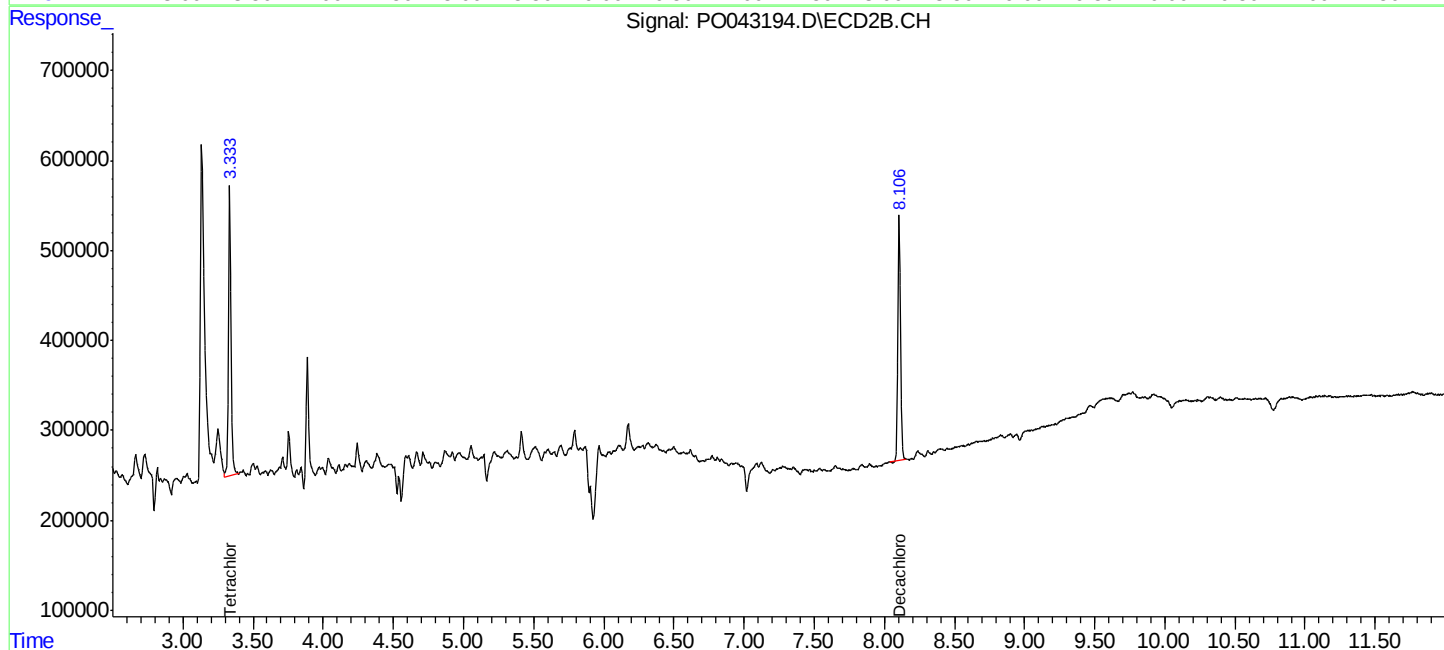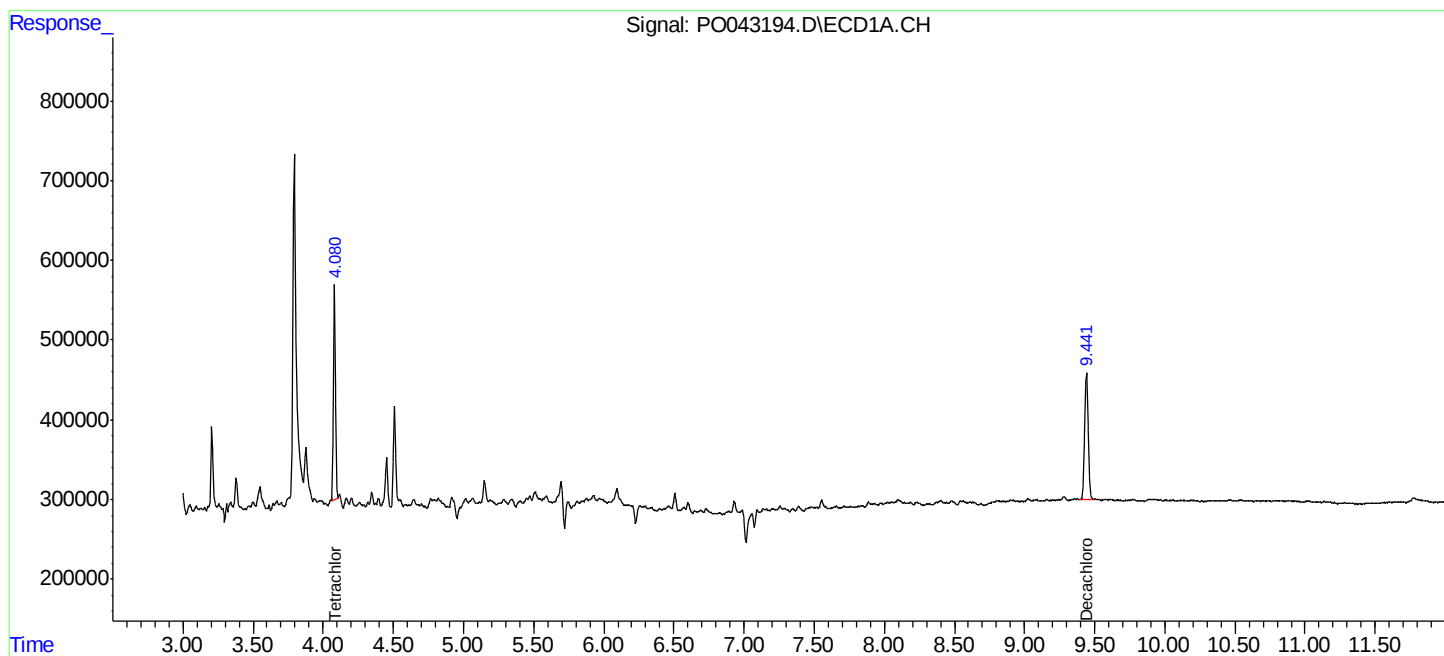

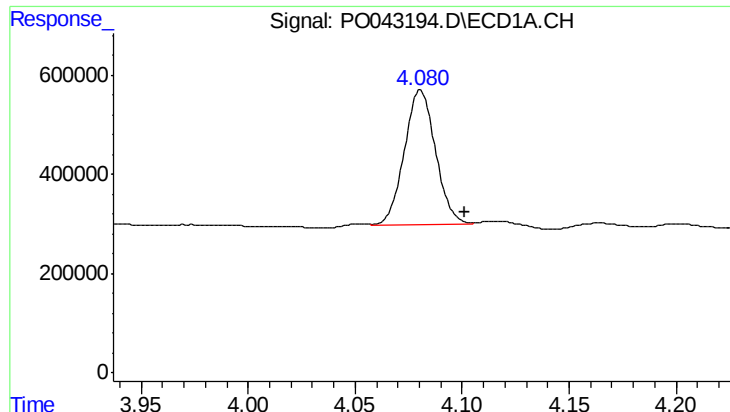


#1 Tetrachloro-m-xylene

R.T.: 4.080 min
Delta R.T.: -0.021 min
Response: 2730349
Conc: 11.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
031418-TIDO-F-D-S


Manual Integrations
APPROVED

ugo
3/22/2018 2:24:17 PM

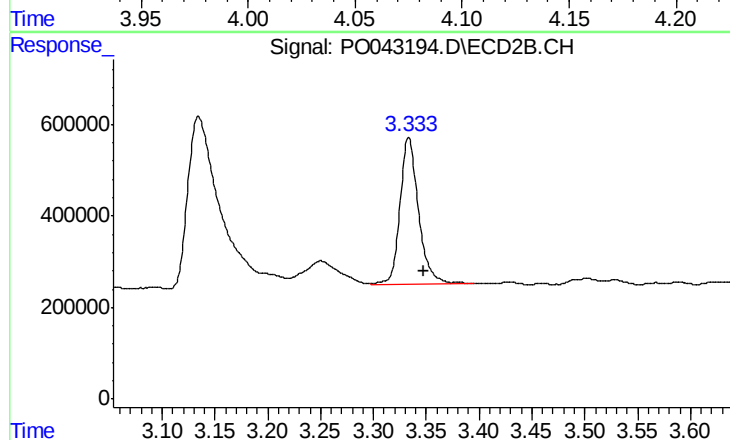


#1 Tetrachloro-m-xylene

R.T.: 3.333 min
Delta R.T.: -0.015 min
Response: 3972771
Conc: 10.75 ng/ml

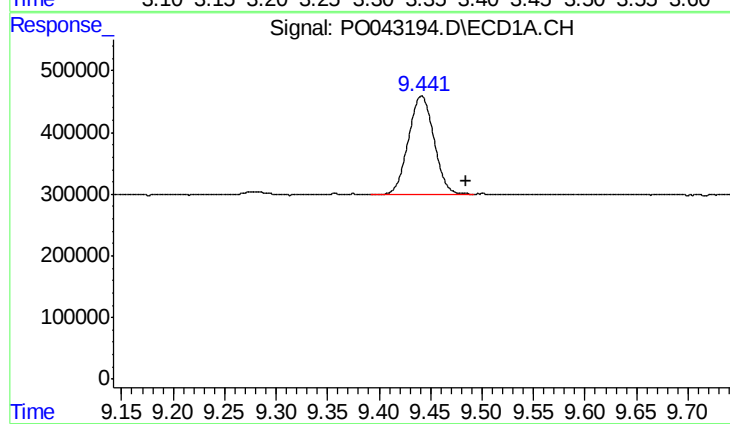

#2 Decachlorobiphenyl

R.T.: 9.441 min
Delta R.T.: -0.043 min
Response: 2759851
Conc: 10.92 ng/ml

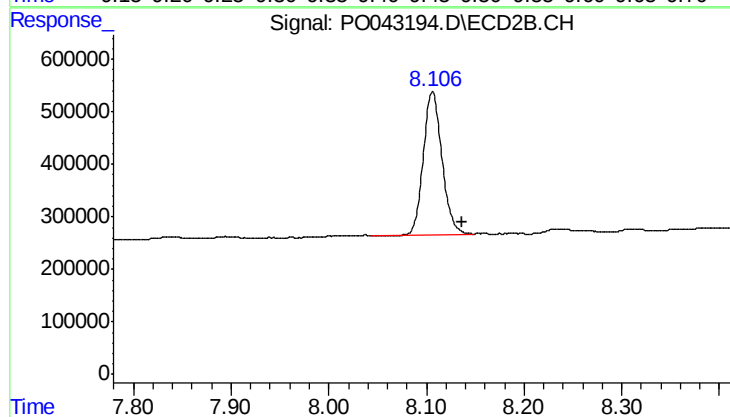

#2 Decachlorobiphenyl

R.T.: 8.106 min
Delta R.T.: -0.030 min
Response: 3594109
Conc: 9.32 ng/ml