

Data Path : P:\HPCHEM1\ECD 0\Data\P0032018\
 Data File : P0043214.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Mar 2018 21:01
 Operator : SM/UA
 Sample : J1954-10
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 031518-TIDO-F-U-S

Manual Integrations
 APPROVED

ugo
 3/22/2018 2:25:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 21 05:32:33 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0022118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 26 14:24:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.080	3.333	3461687	4808754	13.974m	13.013
2) SA Decachlor...	9.440	8.105	3605865	5358530	14.268	13.896m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\PO032018\
Data File : PO043214.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Mar 2018 21:01
Operator : SM/UA
Sample : J1954-10
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
031518-TIDO-F-U-S


Manual Integrations
APPROVED

ugo
3/22/2018 2:25:27 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 21 05:32:33 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\PO022118.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 26 14:24:10 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

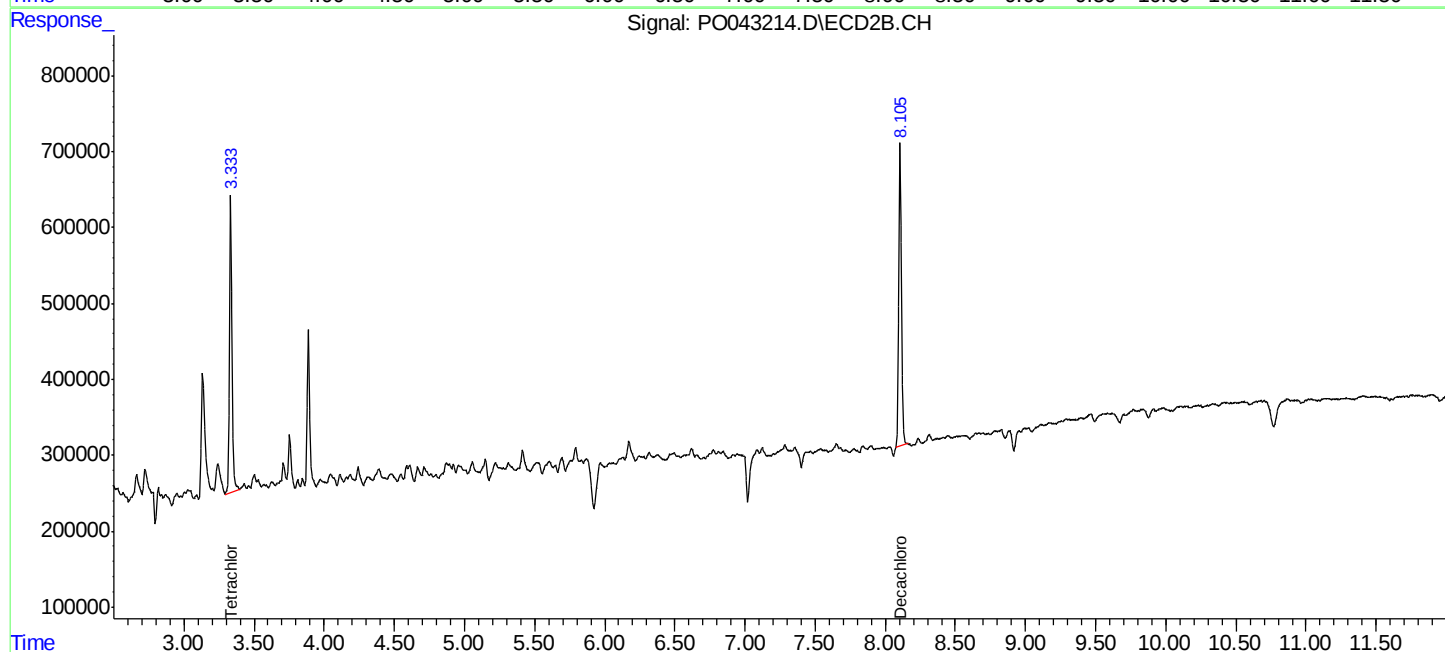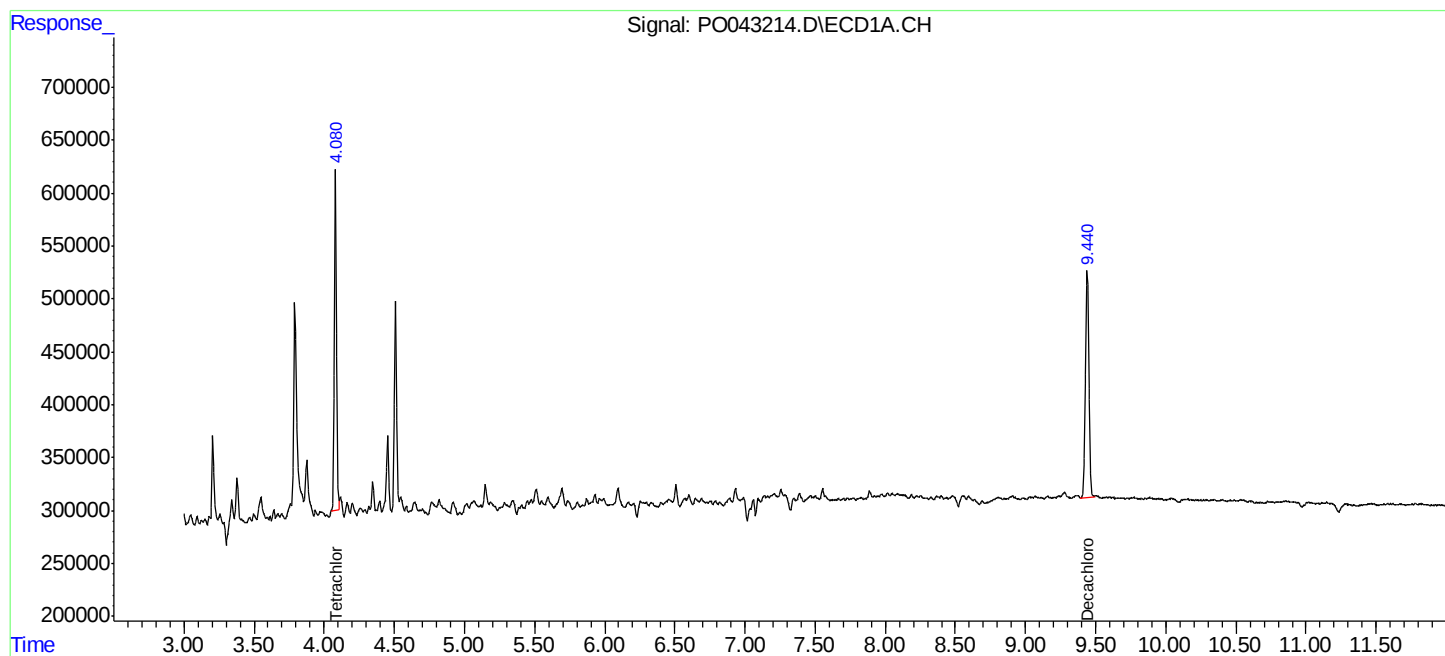

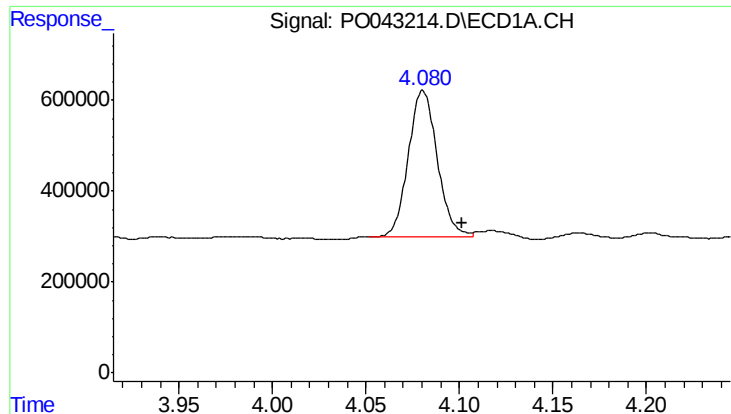


#1 Tetrachloro-m-xylene

R.T.: 4.080 min
Delta R.T.: -0.021 min
Response: 3461687
Conc: 13.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
031518-TIDO-F-U-S


Manual Integrations
APPROVED

ugo
3/22/2018 2:25:27 PM

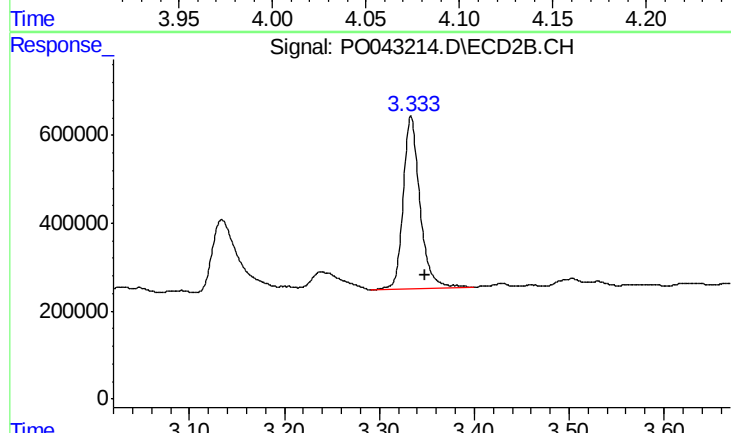


#1 Tetrachloro-m-xylene

R.T.: 3.333 min
Delta R.T.: -0.014 min
Response: 4808754
Conc: 13.01 ng/ml

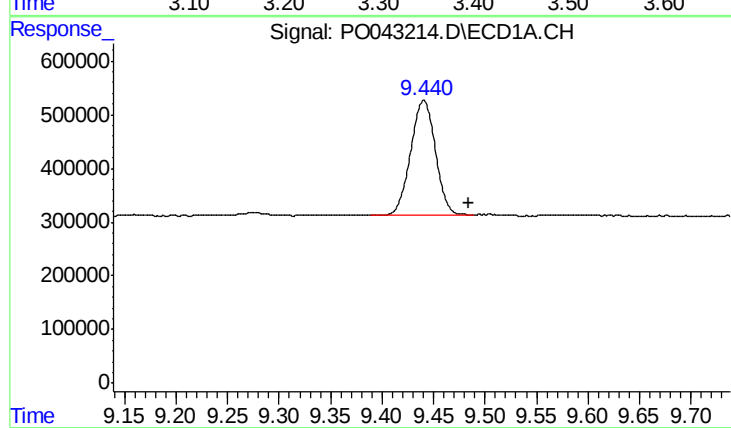

#2 Decachlorobiphenyl

R.T.: 9.440 min
Delta R.T.: -0.044 min
Response: 3605865
Conc: 14.27 ng/ml

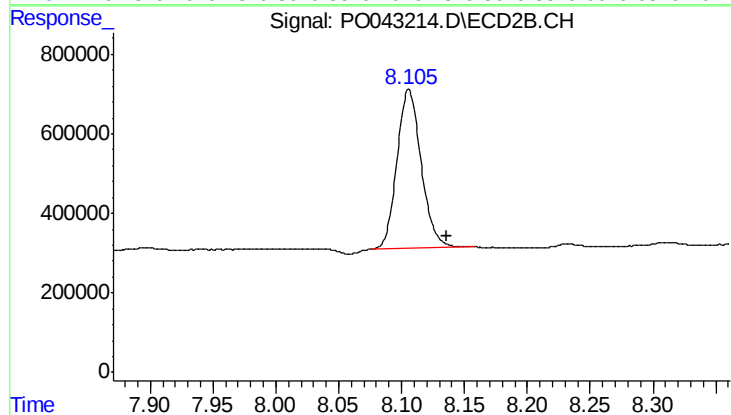

#2 Decachlorobiphenyl

R.T.: 8.105 min
Delta R.T.: -0.031 min
Response: 5358530
Conc: 13.90 ng/ml m