

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032020\
 Data File : P0067362.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Mar 2020 15:51
 Operator : DD\AJ
 Sample : L1762-18
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 17:07:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 19 16:36:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.942	3.952	552920	911387	26.015	26.071
2)	SA Decachlor...	10.928	9.249	647451	854254	22.533	21.901
Target Compounds							
5)	L1 AR-1016-3	0.000	5.415	0	121027	N.D.	108.444 #
6)	L1 AR-1016-4	0.000	5.455	0	84148	N.D.	90.476 #
13)	L3 AR-1232-3	0.000	5.415	0	121027	N.D.	309.718 #
14)	L3 AR-1232-4	0.000	5.540	0	70560	N.D.	197.542 #
18)	L4 AR-1242-3	0.000	5.415	0	121027	N.D.	143.448 #
19)	L4 AR-1242-4	0.000	5.540	0	70560	N.D.	83.450 #
22)	L5 AR-1248-2	0.000	5.455	0	84148	N.D.	81.559 #
23)	L5 AR-1248-3	0.000	5.540	0	70560	N.D.	67.041 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032020\
Data File : P0067362.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Mar 2020 15:51
Operator : DD\AJ
Sample : L1762-18
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 17:07:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031920.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 19 16:36:53 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

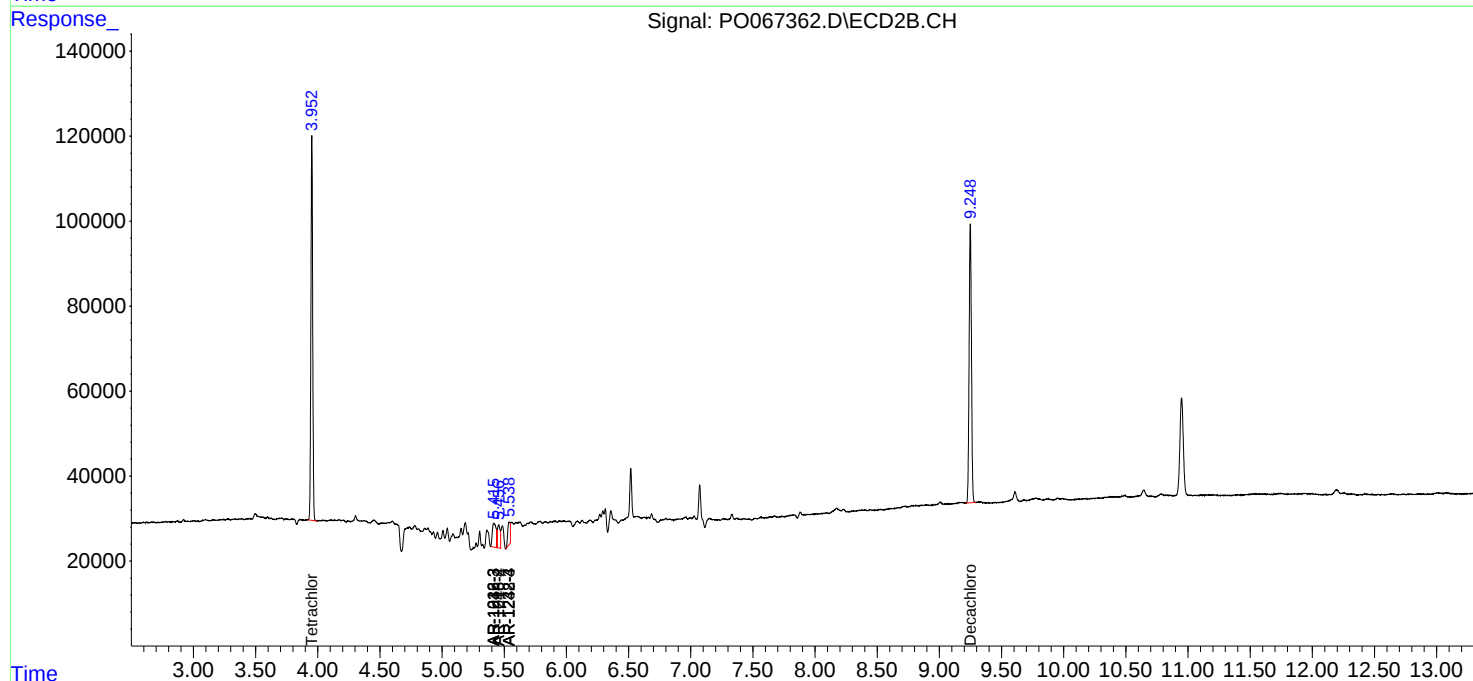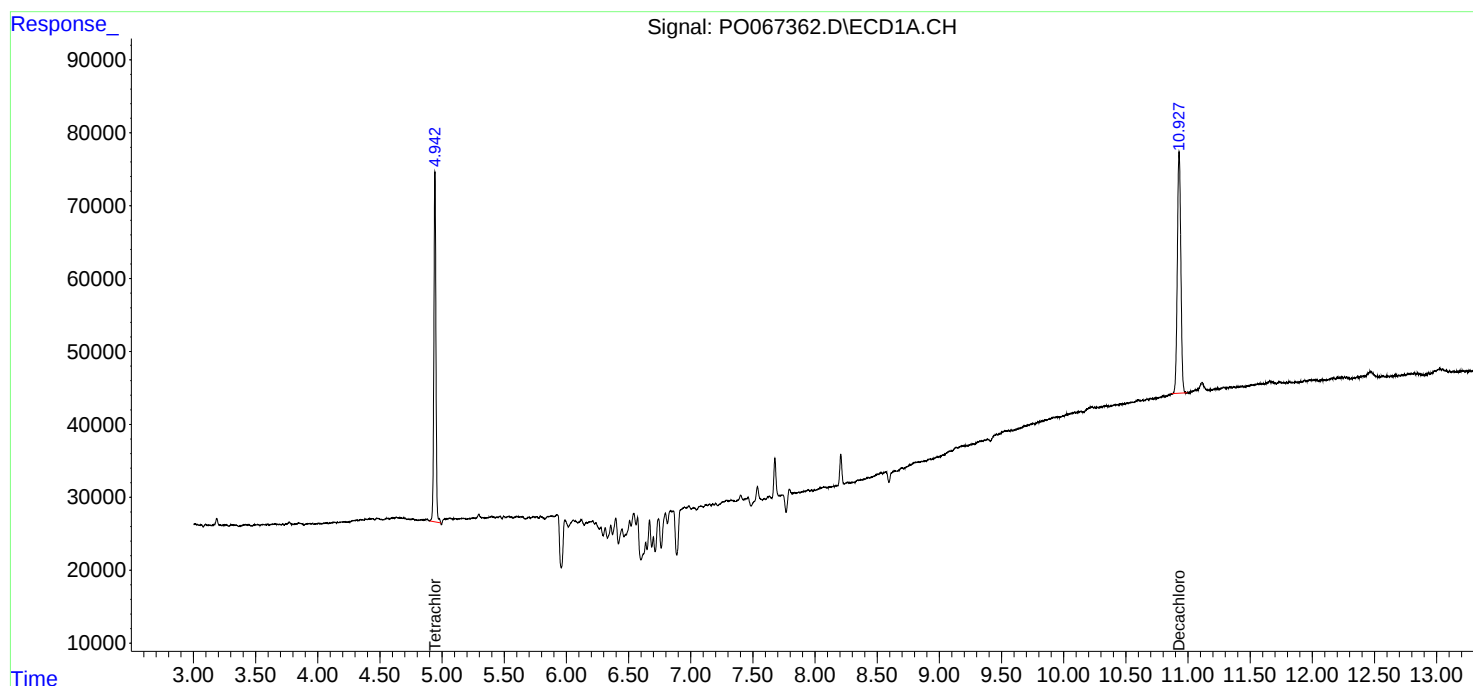


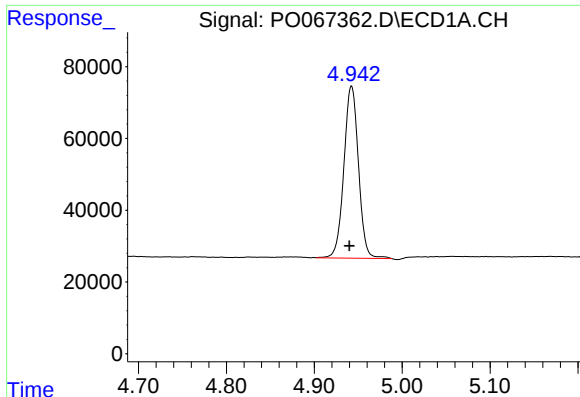

#1 Tetrachloro-m-xylene


R.T.: 4.942 min
Delta R.T.: 0.002 min
Response: 552920
Conc: 26.02 ng/ml

Instrument :
ECD_O
ClientSampleId :

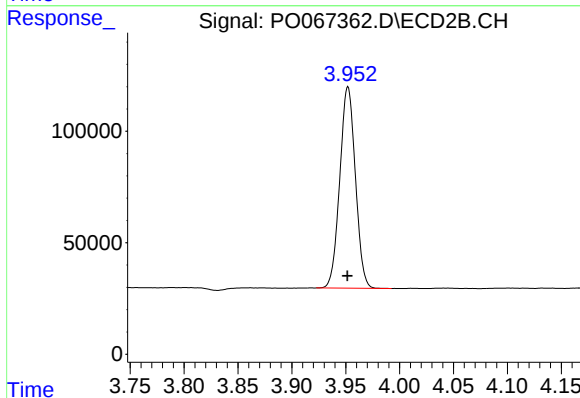


#1 Tetrachloro-m-xylene

R.T.: 3.952 min
Delta R.T.: 0.000 min
Response: 911387
Conc: 26.07 ng/ml

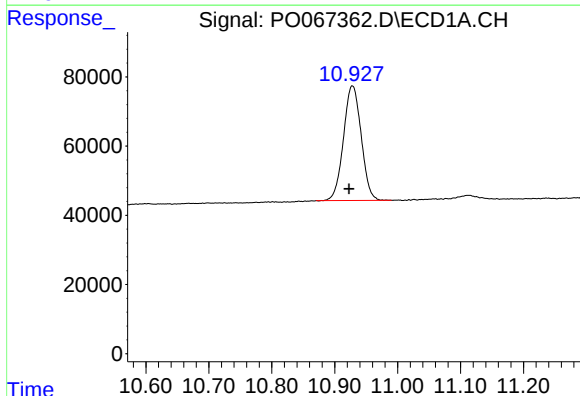


#2 Decachlorobiphenyl

R.T.: 10.928 min
Delta R.T.: 0.005 min
Response: 647451
Conc: 22.53 ng/ml

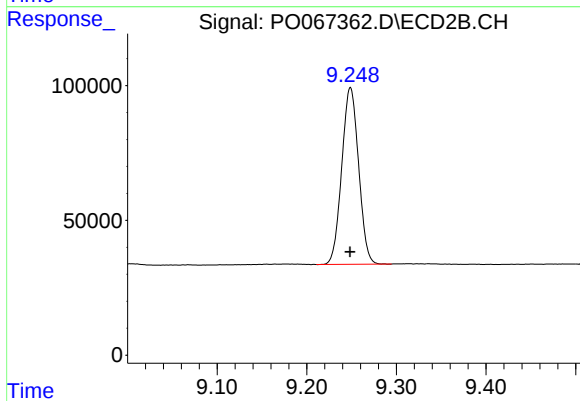

#2 Decachlorobiphenyl


R.T.: 9.249 min
Delta R.T.: 0.000 min
Response: 854254
Conc: 21.90 ng/ml

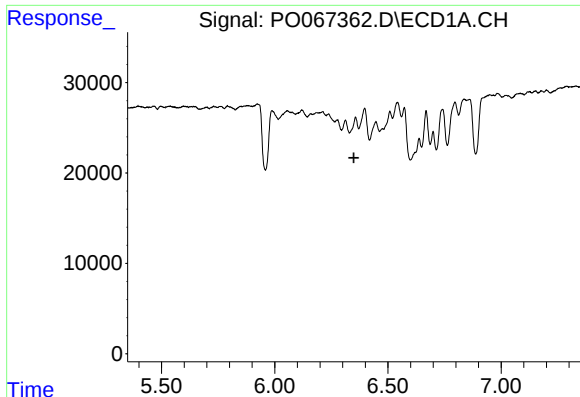

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 6.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

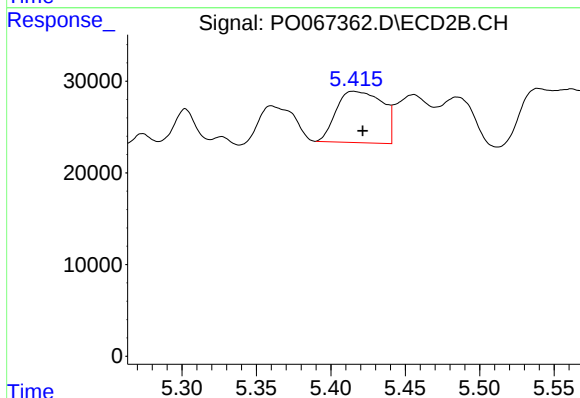


#5 AR-1016-3

R.T.: 5.415 min
Delta R.T.: -0.006 min
Response: 121027
Conc: 108.44 ng/ml

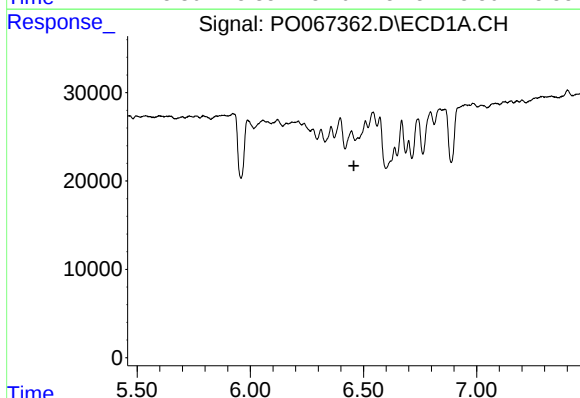


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

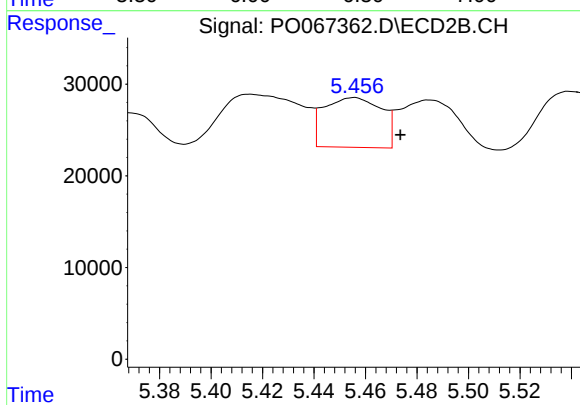

#6 AR-1016-4


R.T.: 5.455 min
Delta R.T.: -0.018 min
Response: 84148
Conc: 90.48 ng/ml

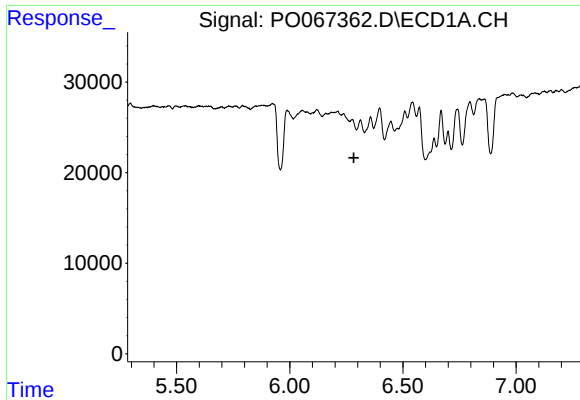

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T.: 6.283 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

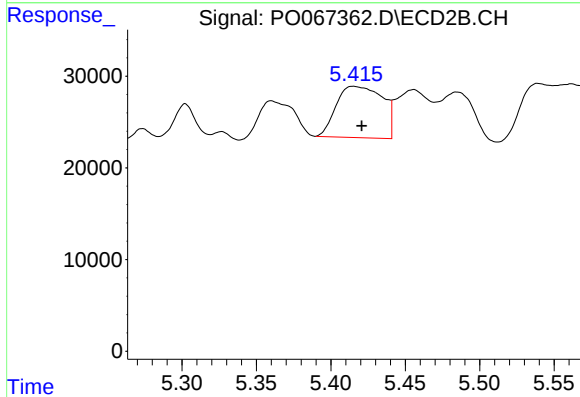


#13 AR-1232-3

R.T.: 5.415 min
Delta R.T.: -0.006 min
Response: 121027
Conc: 309.72 ng/ml

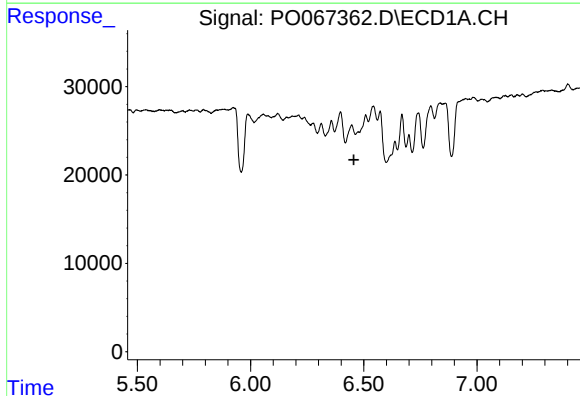


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T.: 6.456 min
Response: 0
Conc: N.D.

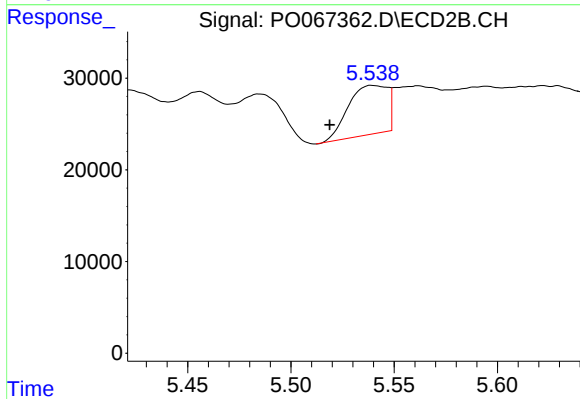

#14 AR-1232-4


R.T.: 5.540 min
Delta R.T.: 0.021 min
Response: 70560
Conc: 197.54 ng/ml

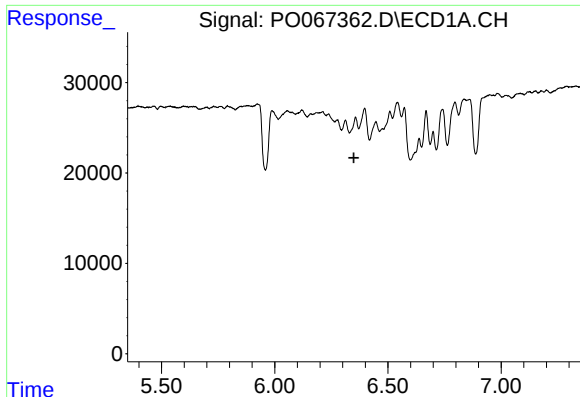

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T.: 6.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

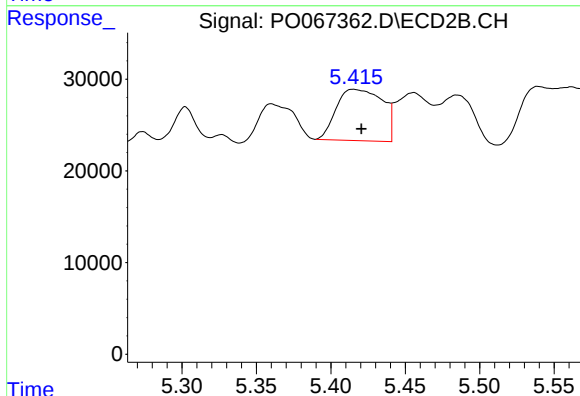


#18 AR-1242-3

R.T.: 5.415 min
Delta R.T.: -0.005 min
Response: 121027
Conc: 143.45 ng/ml

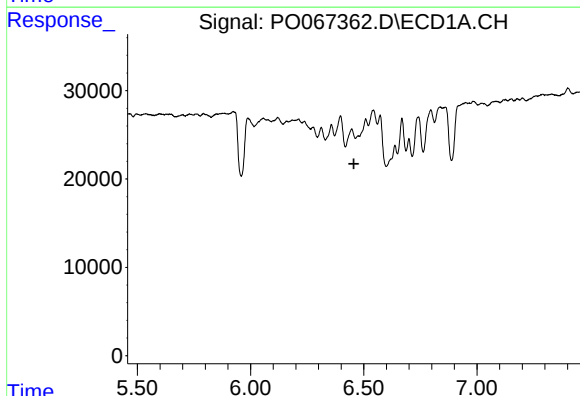


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T.: 6.456 min
Response: 0
Conc: N.D.

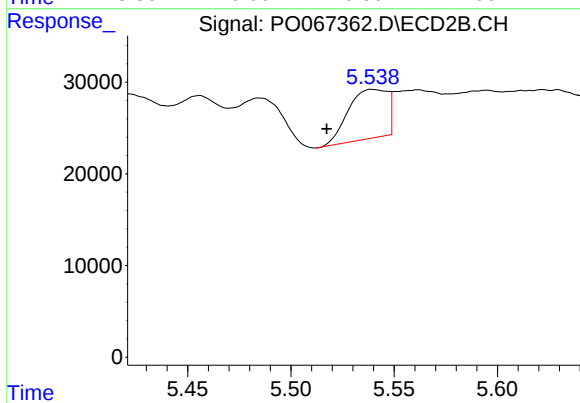

#19 AR-1242-4


R.T.: 5.540 min
Delta R.T.: 0.022 min
Response: 70560
Conc: 83.45 ng/ml

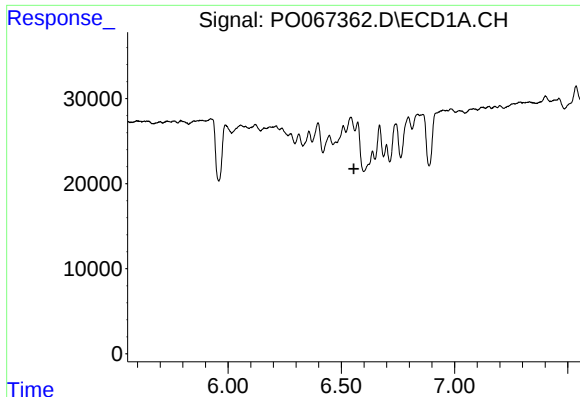

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T.: 6.555 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

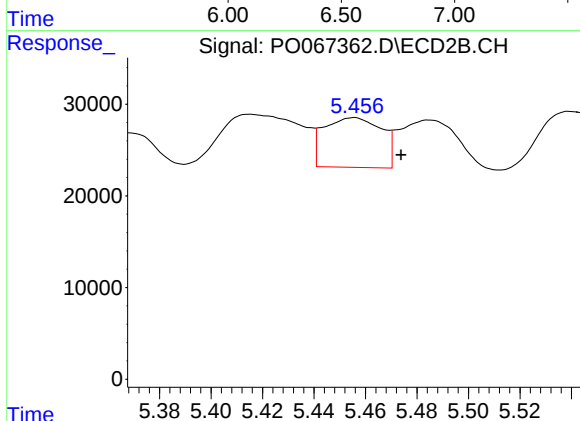


#22 AR-1248-2

R.T.: 5.455 min
Delta R.T.: -0.018 min
Response: 84148
Conc: 81.56 ng/ml

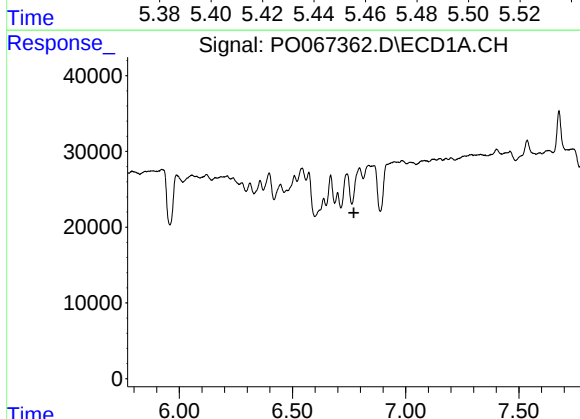

#23 AR-1248-3

R.T.: 0.000 min
Exp R.T.: 6.772 min
Response: 0
Conc: N.D.

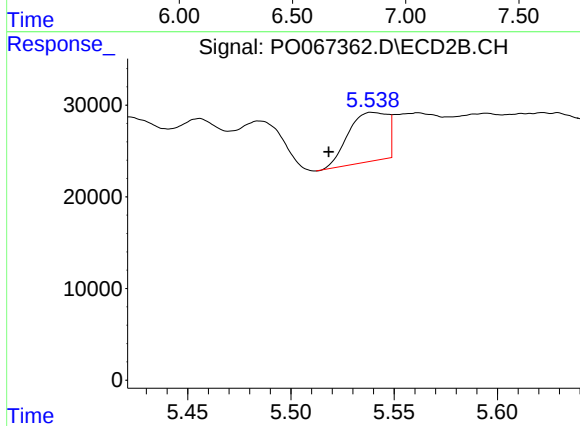

#23 AR-1248-3

R.T.: 5.540 min
Delta R.T.: 0.021 min
Response: 70560
Conc: 67.04 ng/ml