

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032020\
 Data File : P0067360.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Mar 2020 15:16
 Operator : DD\AJ
 Sample : L1749-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BU-02-031920

Manual Integrations
 APPROVED

Sohil
 3/24/2020 2:49:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 16:08:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 19 16:36:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.941	3.952	483972	812937	22.771m	23.254
2) SA Decachlor...	10.926	9.248	554445	781055	19.296	20.024

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032020\
Data File : P0067360.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Mar 2020 15:16
Operator : DD\AJ
Sample : L1749-01
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BU-02-031920


Manual Integrations
APPROVED

Sohil
3/24/2020 2:49:50 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 16:08:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031920.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 19 16:36:53 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

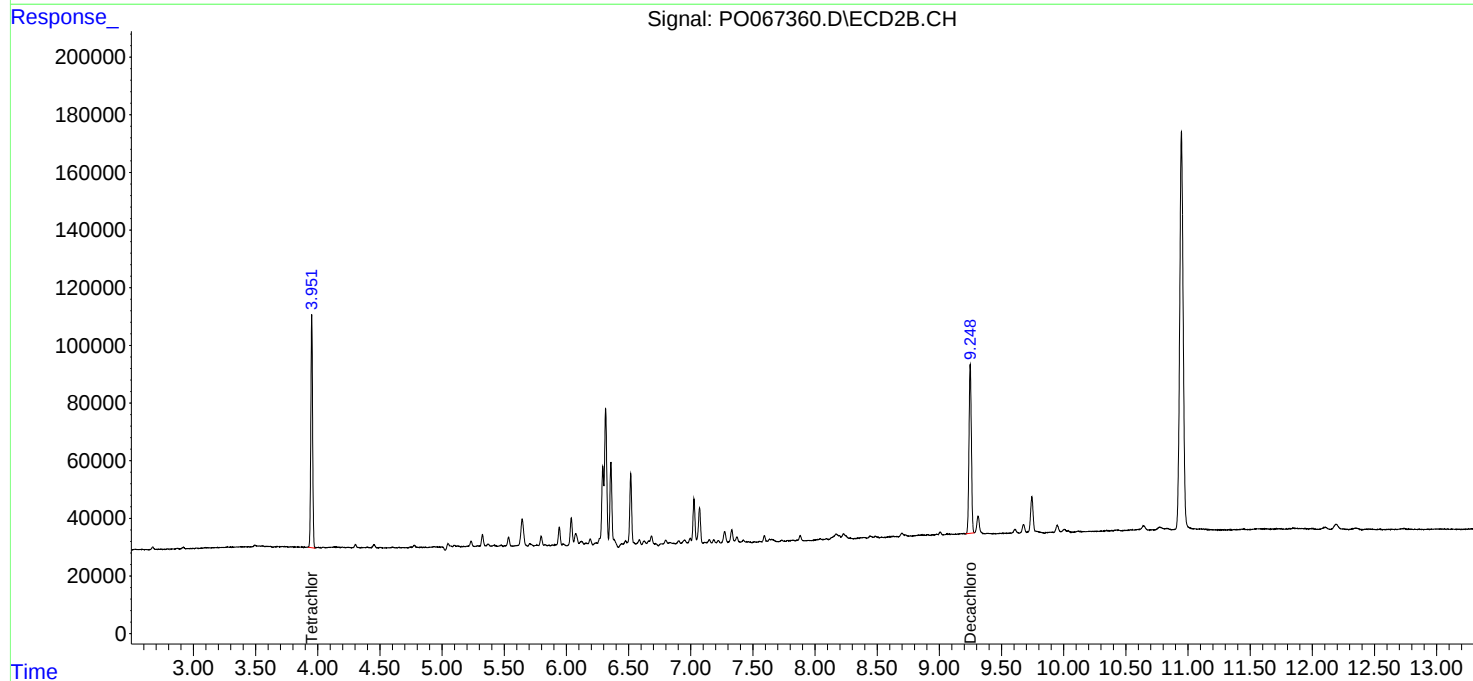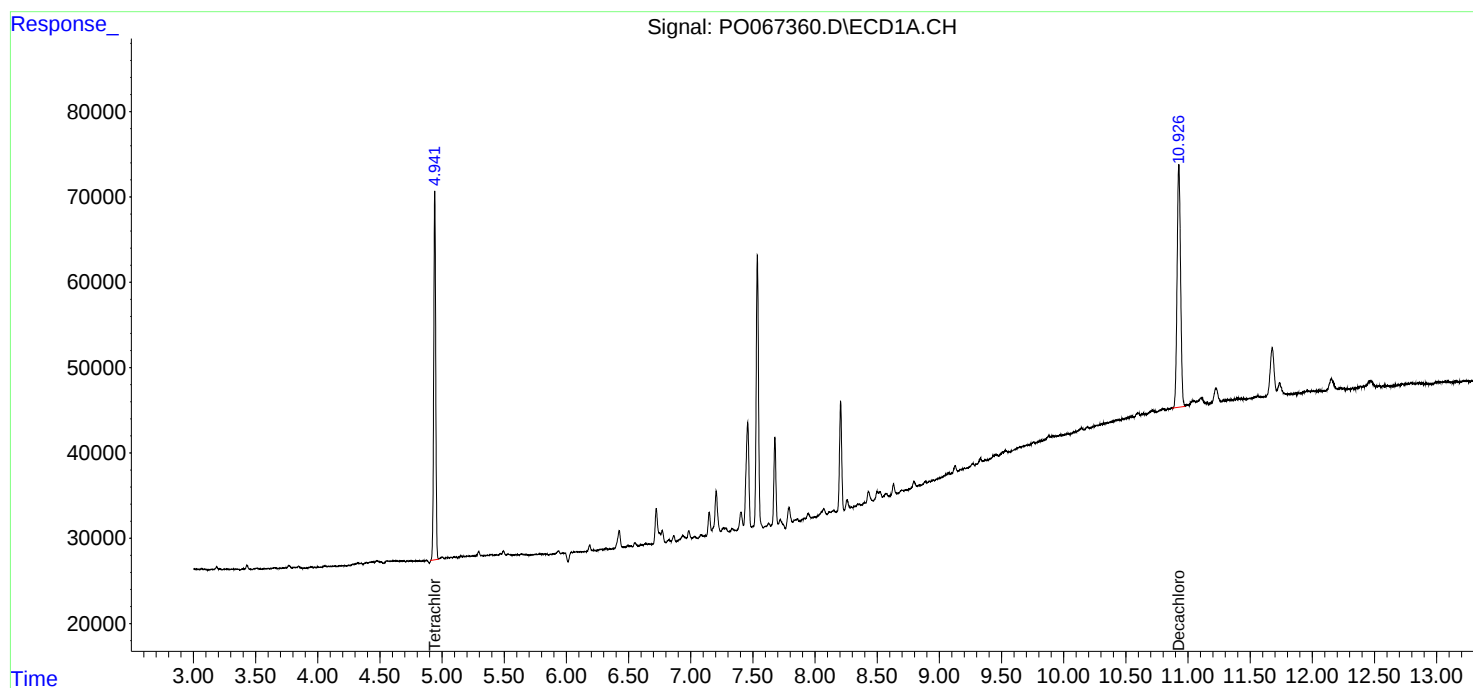

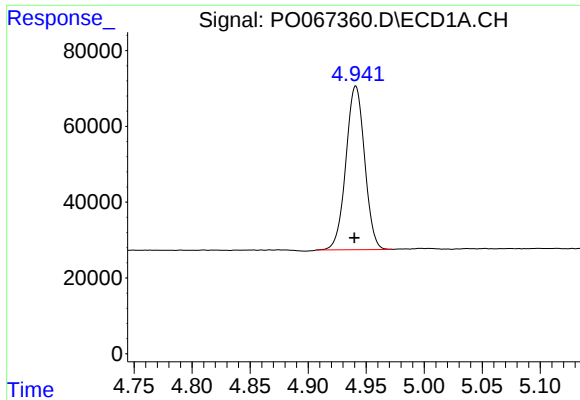


#1 Tetrachloro-m-xylene

R.T.: 4.941 min
Delta R.T.: 0.000 min
Response: 483972
Conc: 22.77 ng/ml m

Instrument :
ECD_O
ClientSampleId :
BU-02-031920


Manual Integrations
APPROVED

Sohil
3/24/2020 2:49:50 PM

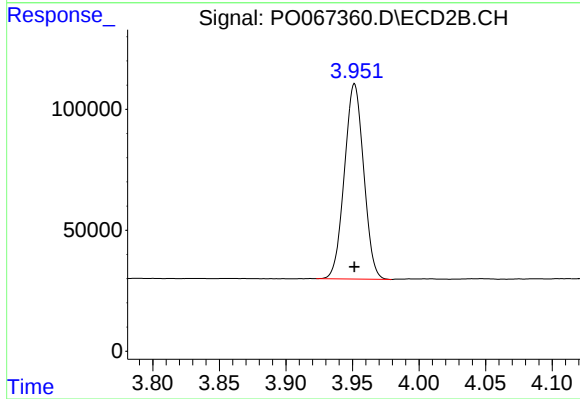


#1 Tetrachloro-m-xylene

R.T.: 3.952 min
Delta R.T.: 0.000 min
Response: 812937
Conc: 23.25 ng/ml

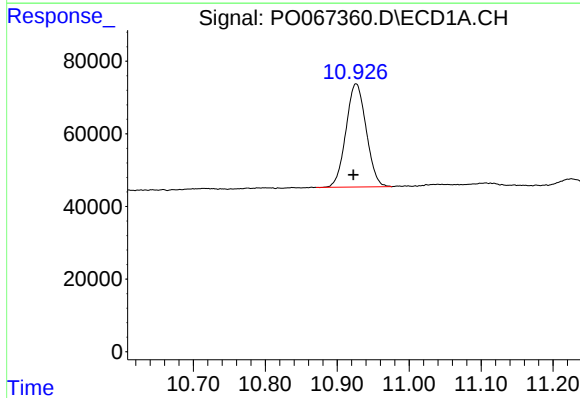

#2 Decachlorobiphenyl

R.T.: 10.926 min
Delta R.T.: 0.004 min
Response: 554445
Conc: 19.30 ng/ml

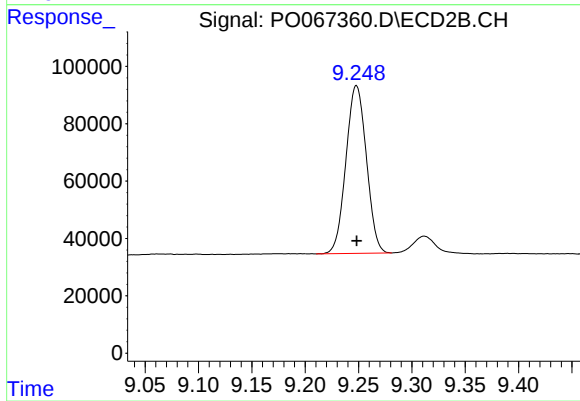

#2 Decachlorobiphenyl

R.T.: 9.248 min
Delta R.T.: 0.000 min
Response: 781055
Conc: 20.02 ng/ml