

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032020\
 Data File : P0067362.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Mar 2020 15:51
 Operator : DD\AJ
 Sample : L1762-18
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TR-05-031920

Manual Integrations
 APPROVED

Sohil
 3/24/2020 2:49:52 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 17:07:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 19 16:36:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.942	3.952	545494	911387	25.666m	26.071
2) SA Decachlor...	10.928	9.249	647451	854254	22.533	21.901

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032020\
Data File : P0067362.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Mar 2020 15:51
Operator : DD\AJ
Sample : L1762-18
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TR-05-031920


Manual Integrations
APPROVED

Sohil
3/24/2020 2:49:52 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 17:07:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031920.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 19 16:36:53 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

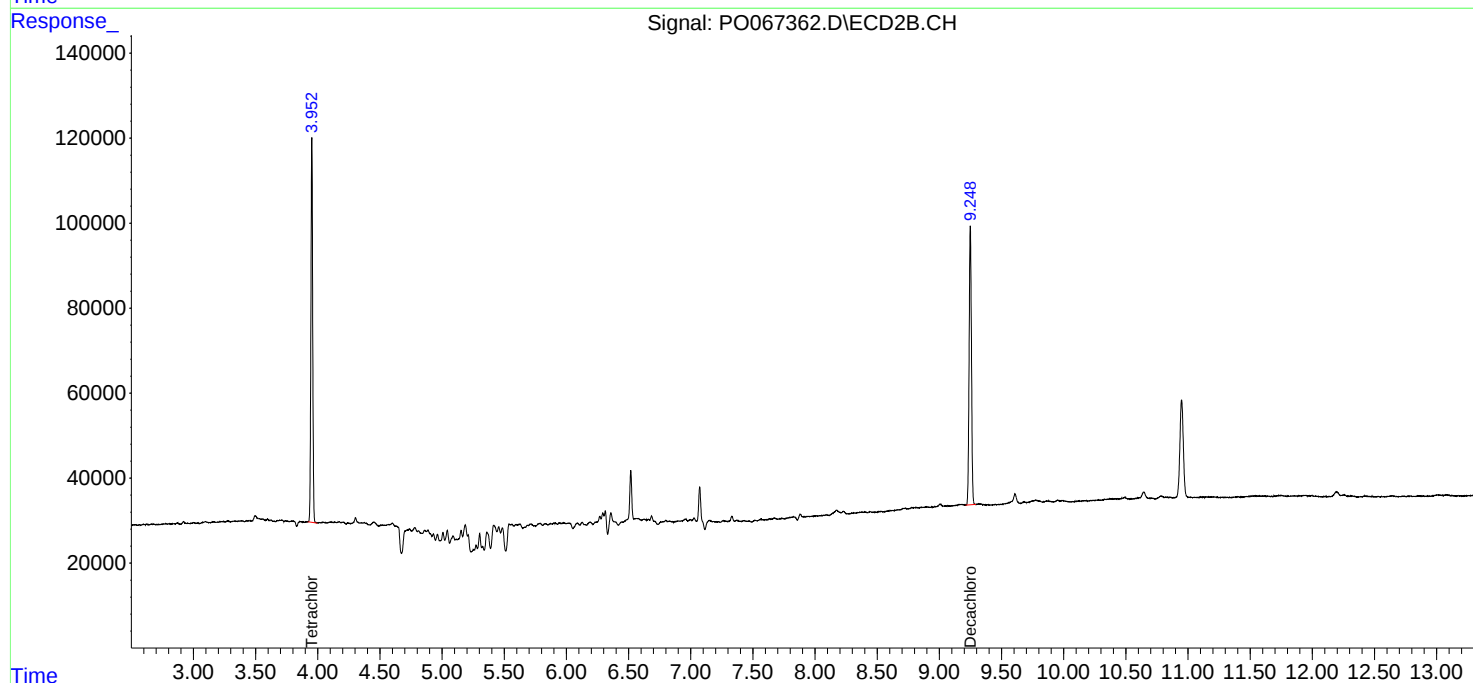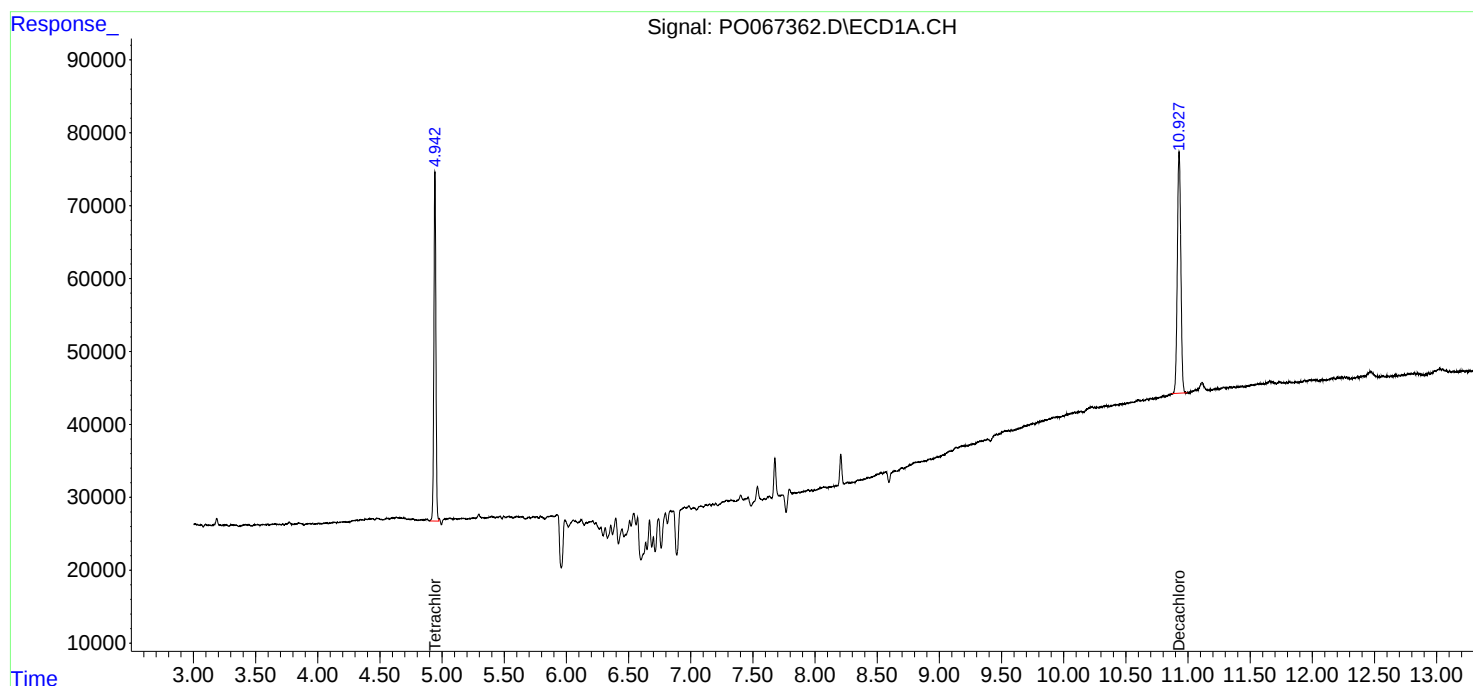

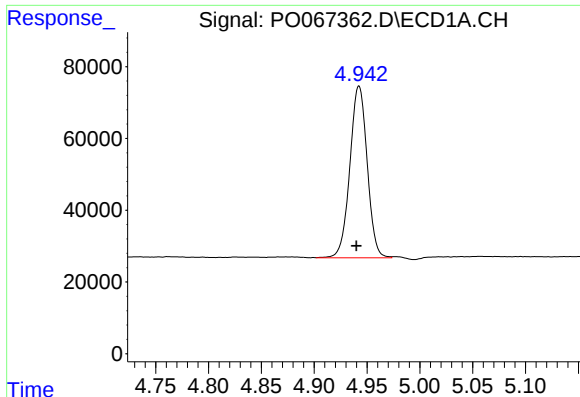


#1 Tetrachloro-m-xylene

R.T.: 4.942 min
Delta R.T.: 0.002 min
Response: 545494
Conc: 25.67 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TR-05-031920


Manual Integrations
APPROVED

Sohil
3/24/2020 2:49:52 PM

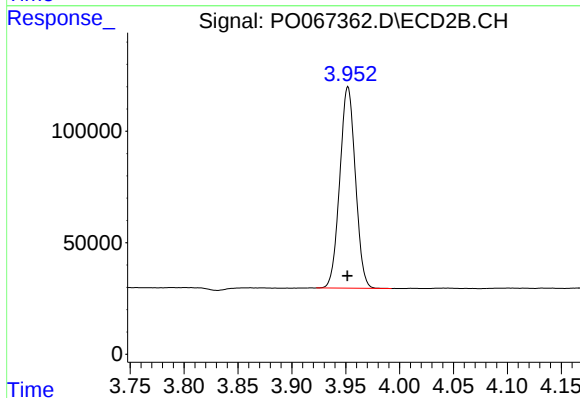


#1 Tetrachloro-m-xylene

R.T.: 3.952 min
Delta R.T.: 0.000 min
Response: 911387
Conc: 26.07 ng/ml

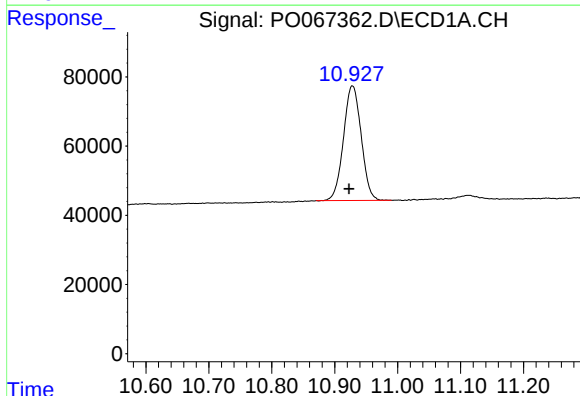

#2 Decachlorobiphenyl

R.T.: 10.928 min
Delta R.T.: 0.005 min
Response: 647451
Conc: 22.53 ng/ml

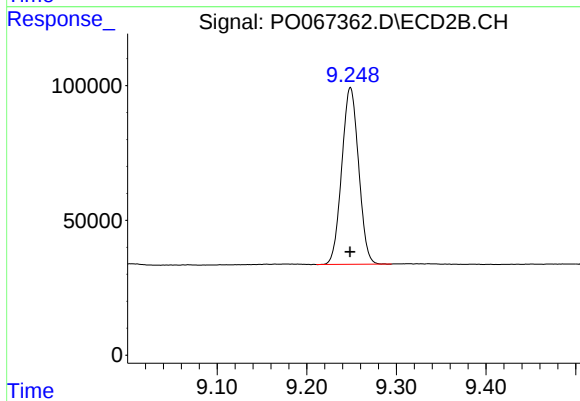

#2 Decachlorobiphenyl

R.T.: 9.249 min
Delta R.T.: 0.000 min
Response: 854254
Conc: 21.90 ng/ml