

Data Path : P:\HPCHEM1\ECD 0\Data\P0032218\
 Data File : P0043223.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Mar 2018 10:22
 Operator : SM/UA
 Sample : J1981-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TILCON-MT-HOPE-1

Manual Integrations
 APPROVED

UGO
 3/23/2018 9:21:49 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 10:36:25 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0022118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 26 14:24:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.081	3.334	3784199	5241145	15.276	14.183
2) SA Decachlor...	9.443	8.107	3901437	6004350	15.437m	15.571

Target Compounds

 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\P0032218\
Data File : P0043223.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Mar 2018 10:22
Operator : SM/UA
Sample : J1981-01
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TILCON-MT-HOPE-1


Manual Integrations
APPROVED

UGO
3/23/2018 9:21:49 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 10:36:25 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0022118.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 26 14:24:10 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

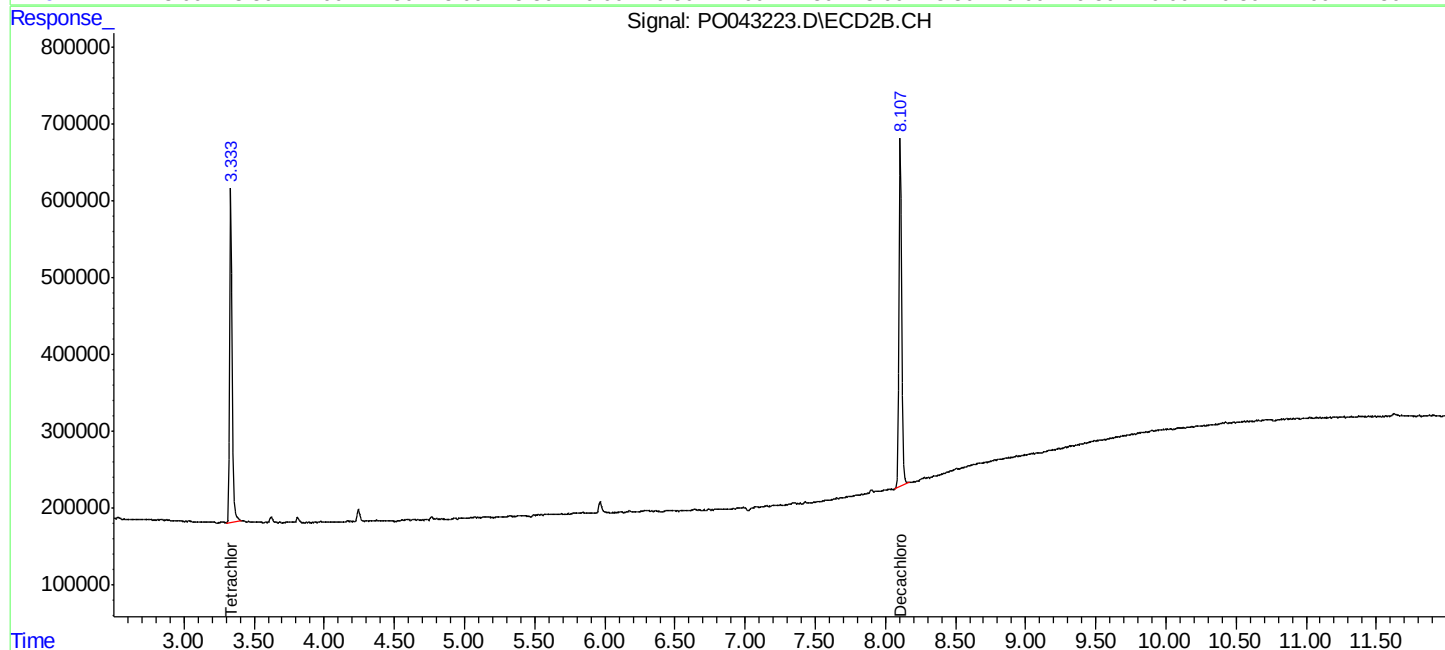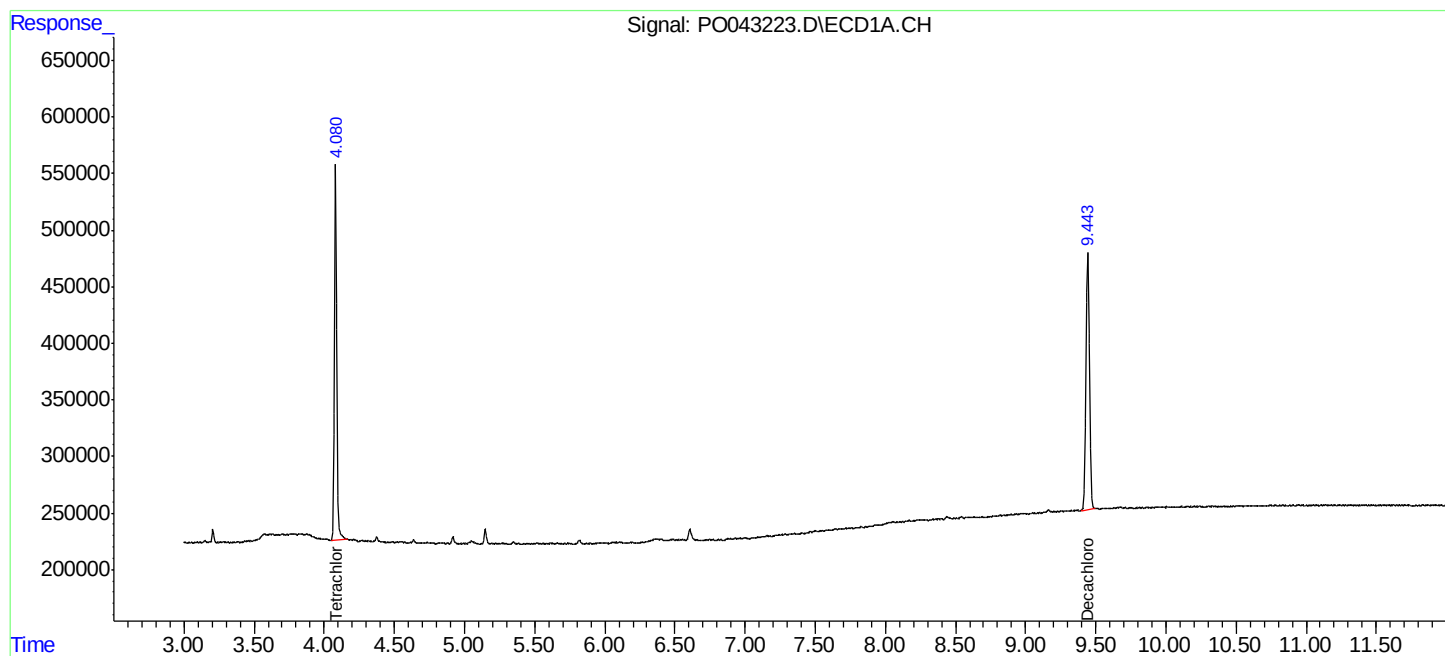

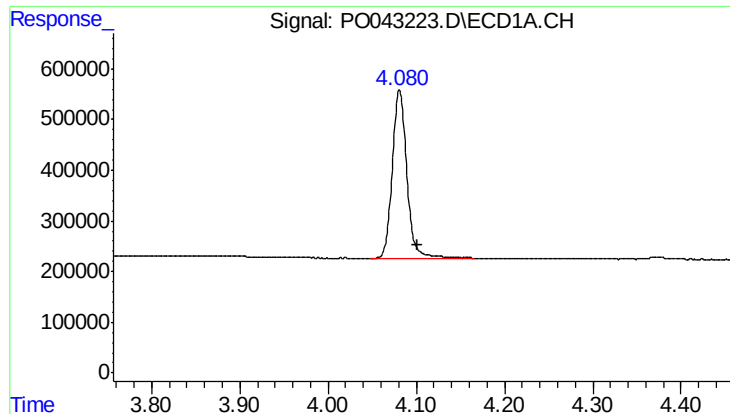


#1 Tetrachloro-m-xylene

R.T.: 4.081 min
Delta R.T.: -0.020 min
Response: 3784199
Conc: 15.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
TILCON-MT-HOPE-1


Manual Integrations
APPROVED

UGO
3/23/2018 9:21:49 AM

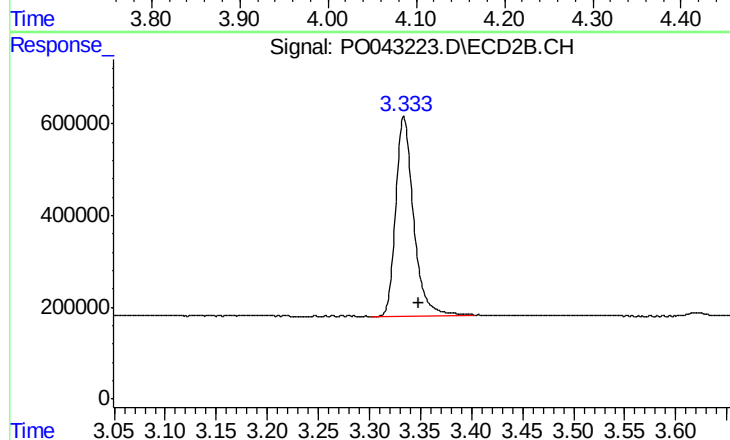


#1 Tetrachloro-m-xylene

R.T.: 3.334 min
Delta R.T.: -0.014 min
Response: 5241145
Conc: 14.18 ng/ml

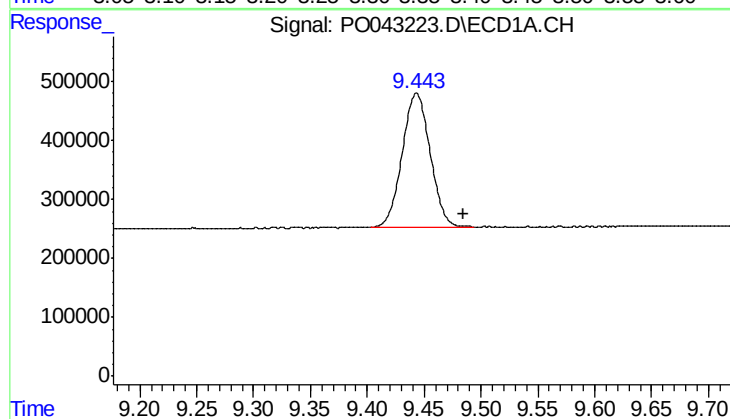

#2 Decachlorobiphenyl

R.T.: 9.443 min
Delta R.T.: -0.041 min
Response: 3901437
Conc: 15.44 ng/ml m

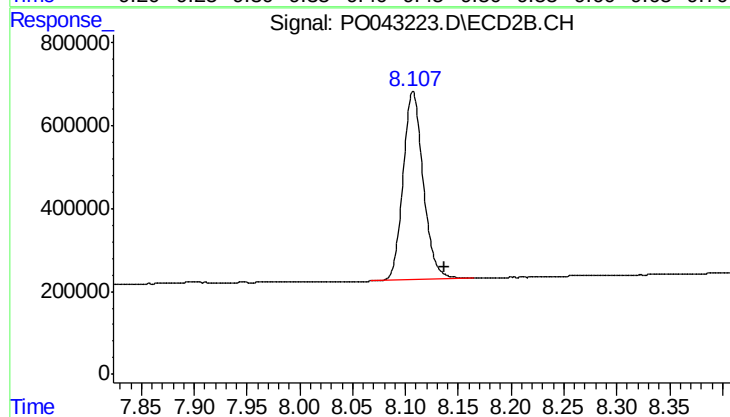

#2 Decachlorobiphenyl

R.T.: 8.107 min
Delta R.T.: -0.029 min
Response: 6004350
Conc: 15.57 ng/ml