

Data Path : P:\HPCHEM1\ECD 0\Data\P0032218\
 Data File : P0043242.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Mar 2018 16:12
 Operator : SM/UA
 Sample : J1972-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S-2 COMP

Manual Integrations
 APPROVED

UGO
 3/23/2018 9:20:49 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 01:30:24 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0022118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 26 14:24:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.081	3.335	4183427	5820792	16.888m	15.752m
2) SA Decachlor...	9.441	8.106	2207453	2813221	8.734	7.295m

Target Compounds

 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\P0032218\
Data File : P0043242.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Mar 2018 16:12
Operator : SM/UA
Sample : J1972-04
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
S-2 COMP


Manual Integrations
APPROVED

UGO
3/23/2018 9:20:49 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 01:30:24 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0022118.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 26 14:24:10 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

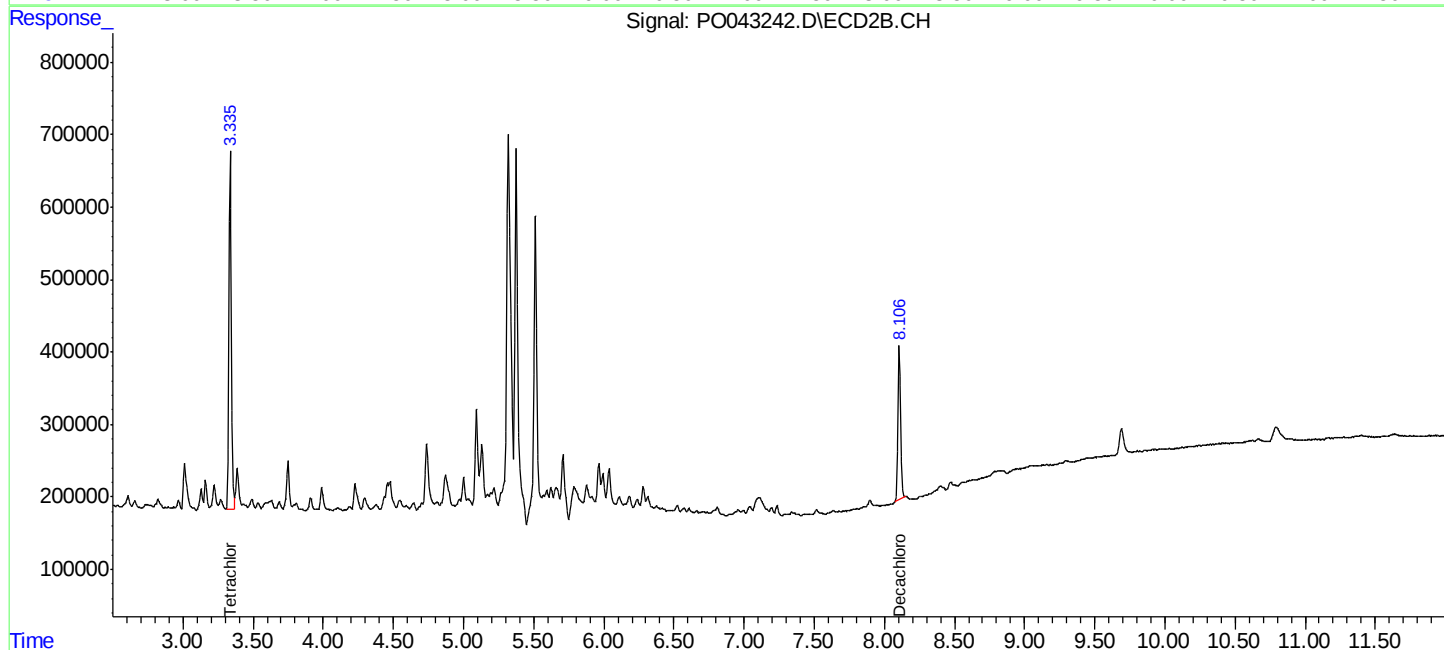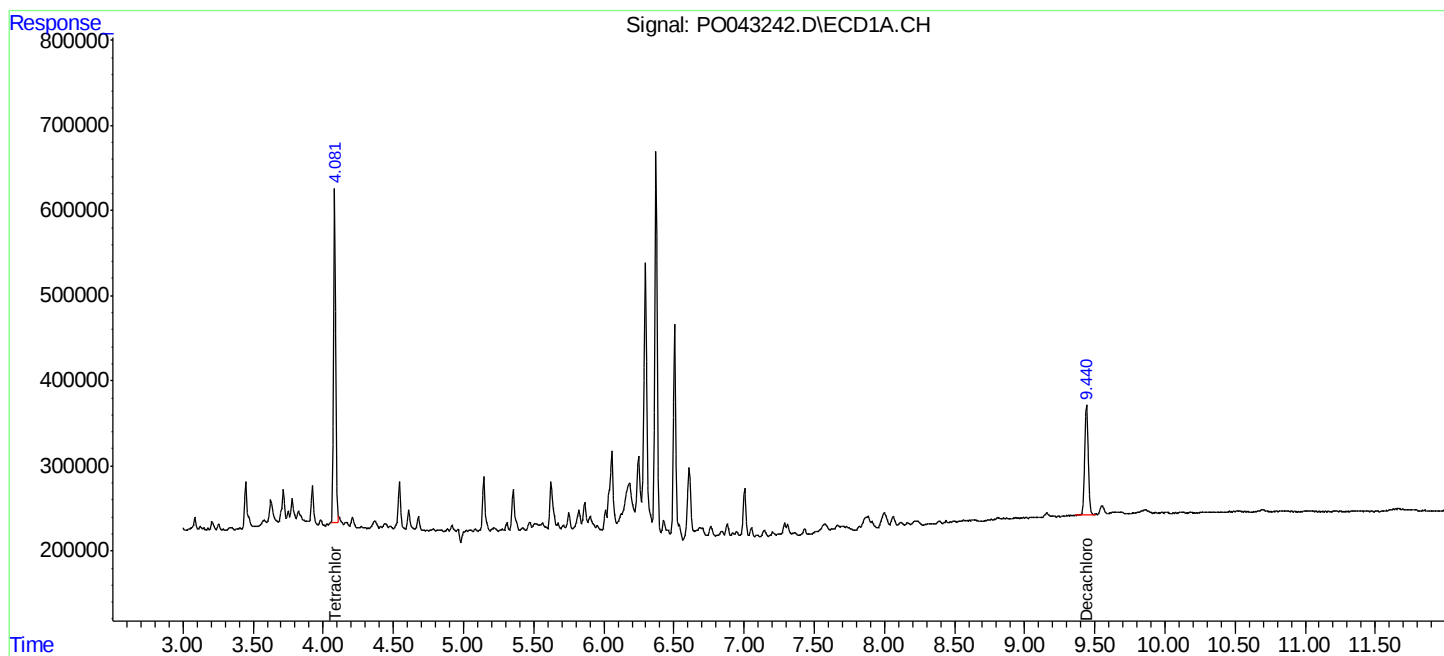

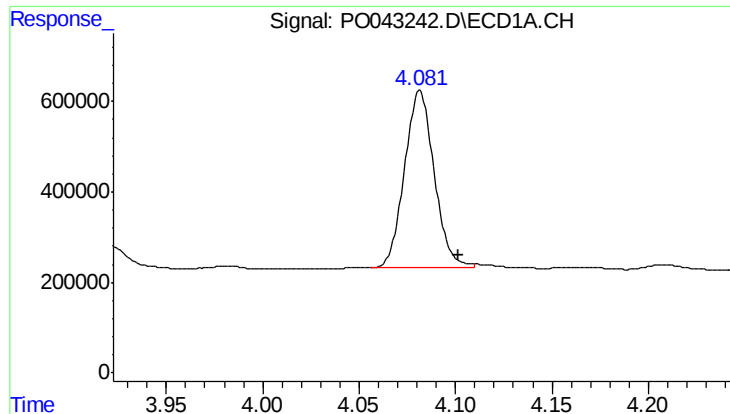


#1 Tetrachloro-m-xylene

R.T.: 4.081 min
Delta R.T.: -0.020 min
Response: 4183427
Conc: 16.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
S-2 COMP


Manual Integrations
APPROVED

UGO
3/23/2018 9:20:49 AM

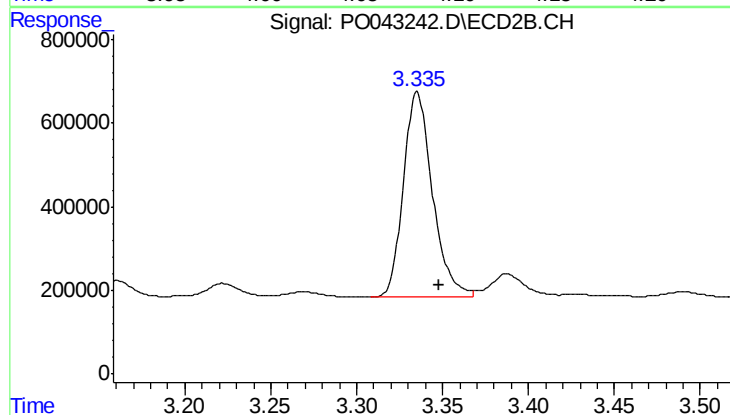


#1 Tetrachloro-m-xylene

R.T.: 3.335 min
Delta R.T.: -0.013 min
Response: 5820792
Conc: 15.75 ng/ml m

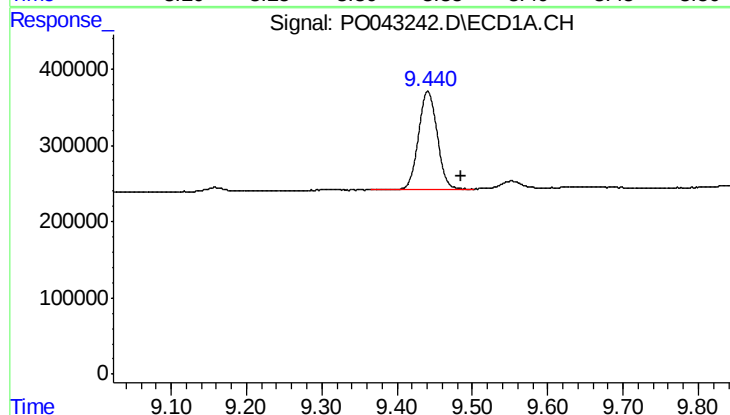

#2 Decachlorobiphenyl

R.T.: 9.441 min
Delta R.T.: -0.043 min
Response: 2207453
Conc: 8.73 ng/ml

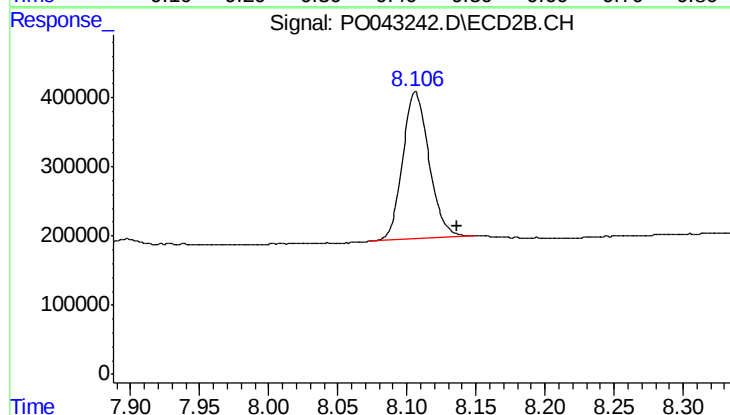

#2 Decachlorobiphenyl

R.T.: 8.106 min
Delta R.T.: -0.031 min
Response: 2813221
Conc: 7.30 ng/ml m