

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032320\
 Data File : P0067404.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Mar 2020 17:58
 Operator : DD\AJ
 Sample : L2009-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TRACKS-66-67

Manual Integrations
 APPROVED

Sohil
 3/24/2020 2:55:20 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 18:15:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 19 16:36:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.940	3.951	538626	877293	25.343	25.095
2) SA Decachlor...	10.925	9.244	558725	729287	19.445	18.697m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032320\
Data File : P0067404.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Mar 2020 17:58
Operator : DD\AJ
Sample : L2009-01
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TRACKS-66-67


Manual Integrations
APPROVED

Sohil
3/24/2020 2:55:20 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 18:15:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031920.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 19 16:36:53 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

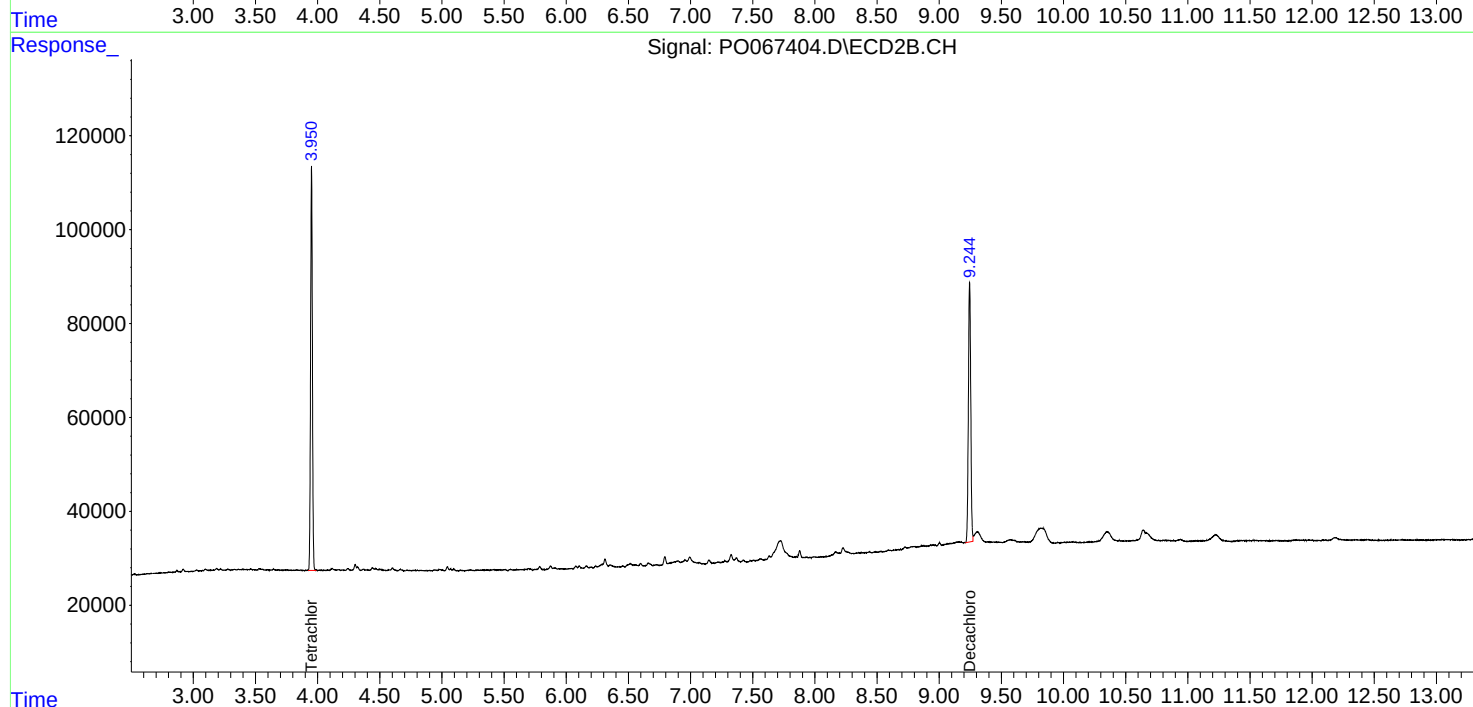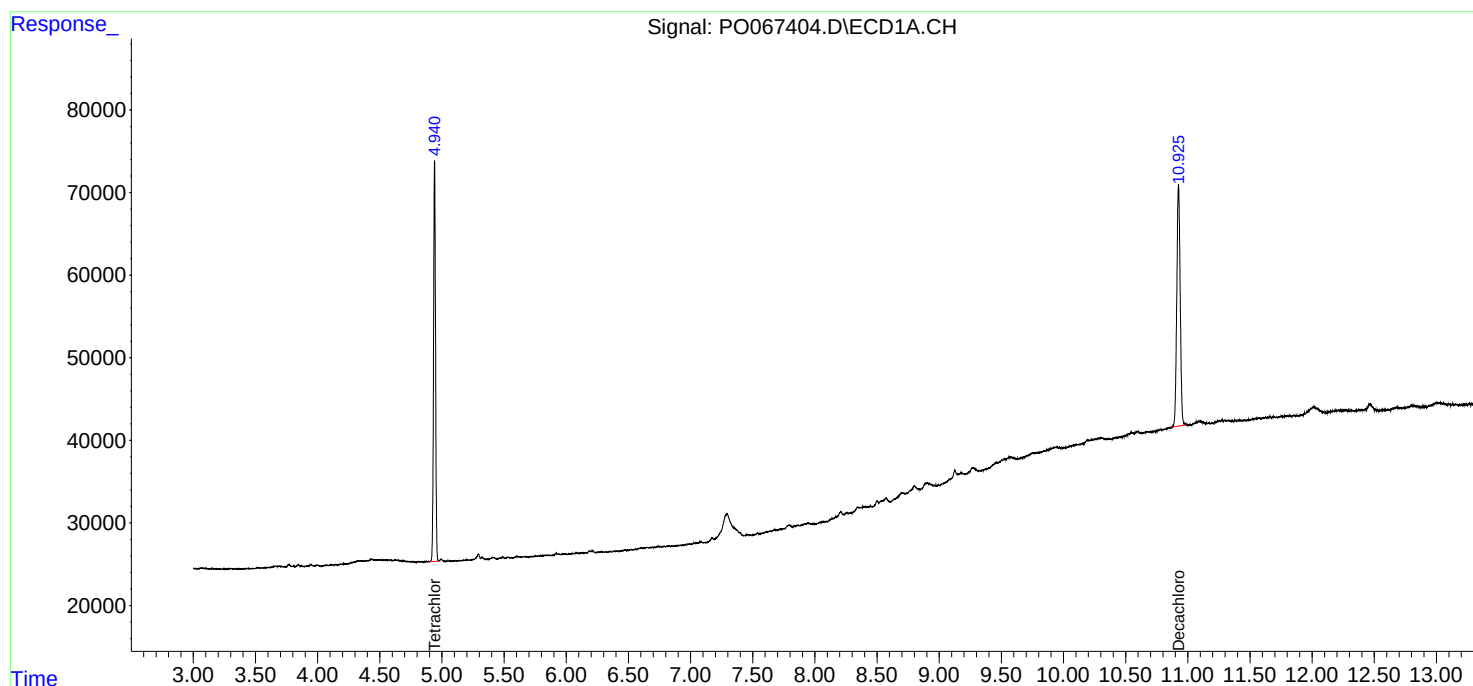

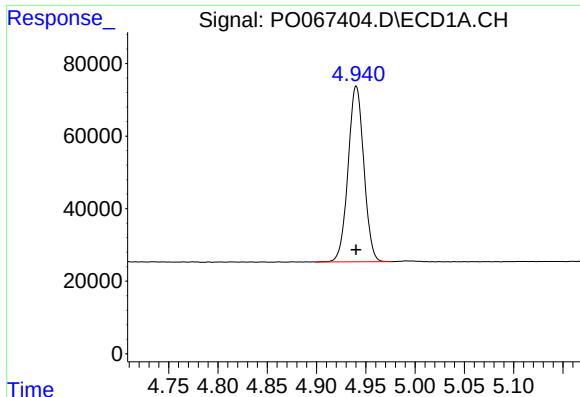


#1 Tetrachloro-m-xylene

R.T.: 4.940 min
Delta R.T.: 0.000 min
Response: 538626
Conc: 25.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
TRACKS-66-67


Manual Integrations
APPROVED

Sohil
3/24/2020 2:55:20 PM

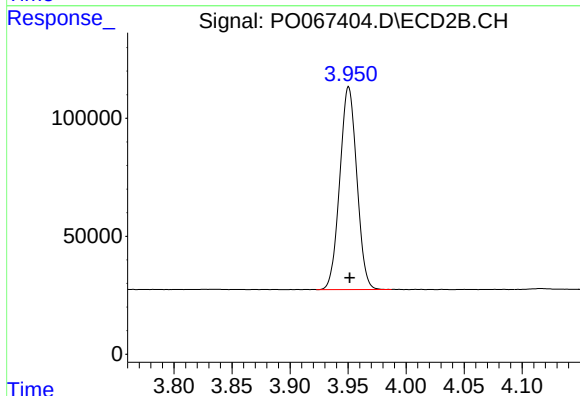


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 877293
Conc: 25.10 ng/ml

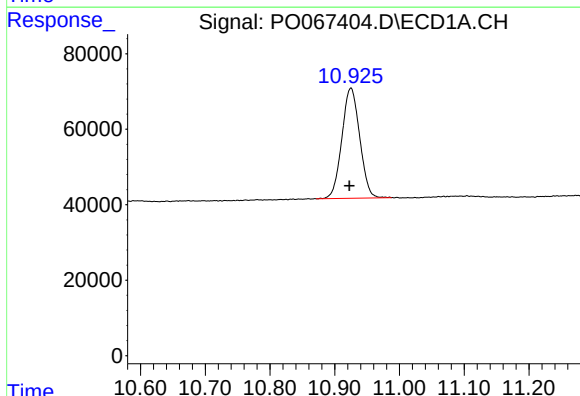

#2 Decachlorobiphenyl

R.T.: 10.925 min
Delta R.T.: 0.002 min
Response: 558725
Conc: 19.45 ng/ml

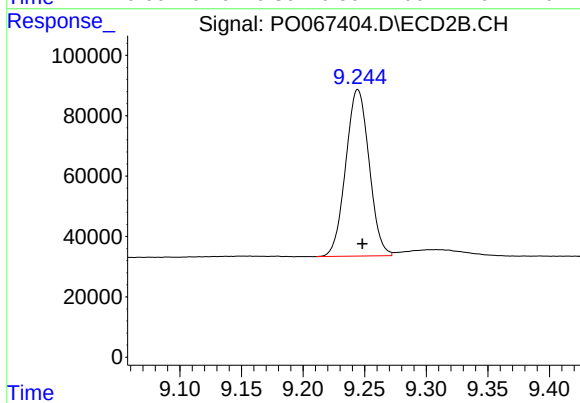

#2 Decachlorobiphenyl

R.T.: 9.244 min
Delta R.T.: -0.004 min
Response: 729287
Conc: 18.70 ng/ml m