

Data Path : P:\HPCHEM1\ECD_0\Data\P0032418\
Data File : P0043289.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Mar 2018 17:09
Operator : SM/UA
Sample : J1972-04RE
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
S-2 COMPRE

Manual Integrations
APPROVED

UGO
3/23/2018 7:30:38 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 17:32:21 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0032318.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 23 05:22:35 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.089	3.337	4429954	6538184	20.906m	22.338
2) SA Decachlor...	9.451	8.110	1497023	1488723	6.164m	4.163 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\P0032418\
Data File : P0043289.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Mar 2018 17:09
Operator : SM/UA
Sample : J1972-04RE
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
S-2 COMPRE


Manual Integrations
APPROVED

UGO
3/23/2018 7:30:38 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 17:32:21 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0032318.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 23 05:22:35 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

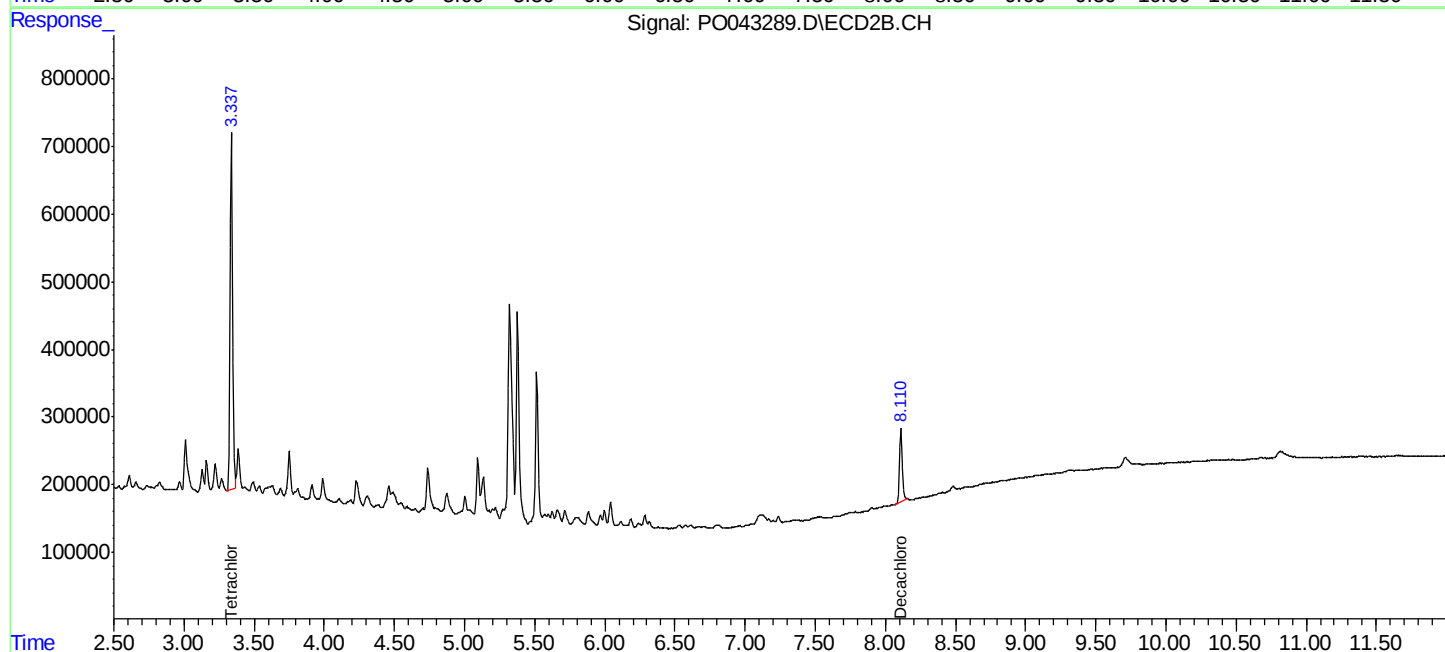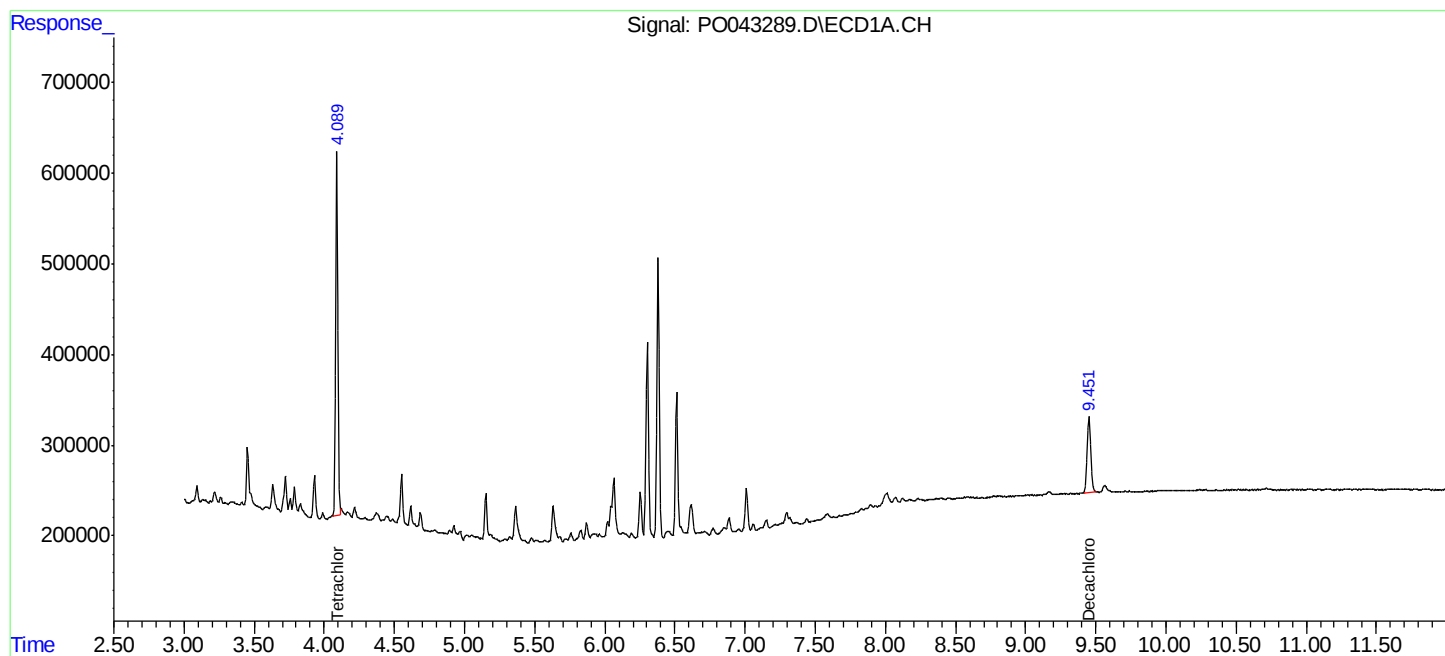

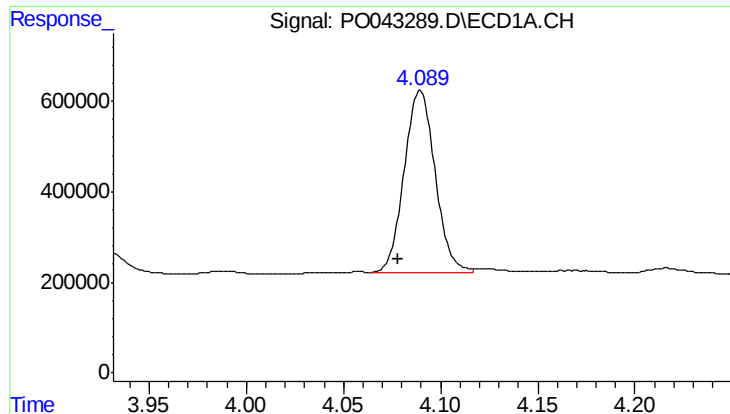


#1 Tetrachloro-m-xylene

R.T.: 4.089 min
Delta R.T.: 0.011 min
Response: 4429954
Conc: 20.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
S-2 COMPRE


Manual Integrations
APPROVED

UGO
3/23/2018 7:30:38 PM

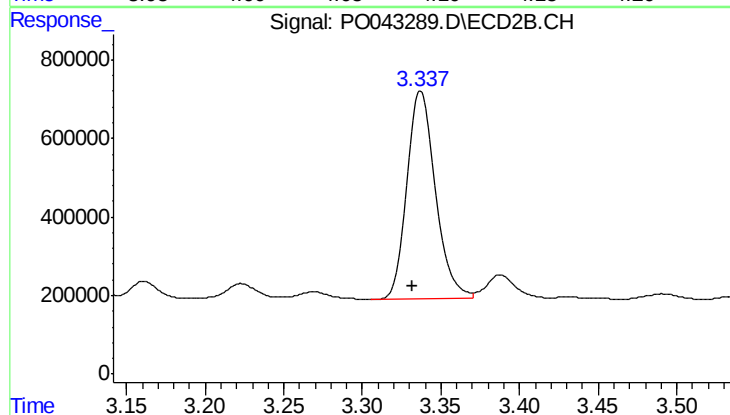


#1 Tetrachloro-m-xylene

R.T.: 3.337 min
Delta R.T.: 0.005 min
Response: 6538184
Conc: 22.34 ng/ml

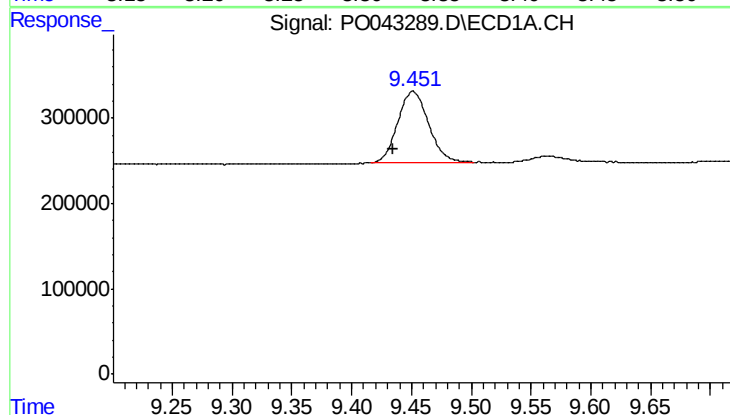

#2 Decachlorobiphenyl

R.T.: 9.451 min
Delta R.T.: 0.016 min
Response: 1497023
Conc: 6.16 ng/ml m

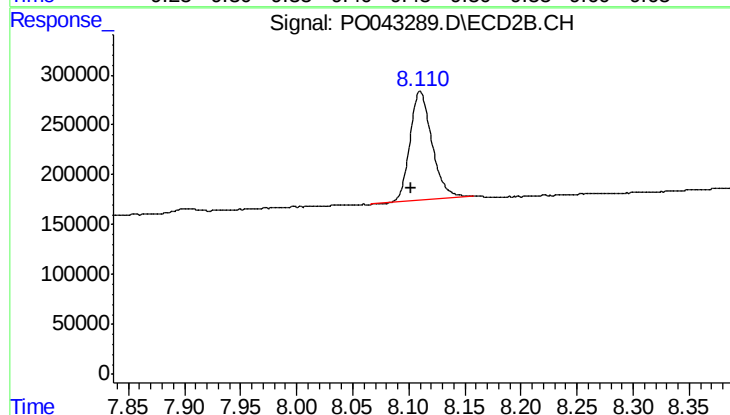

#2 Decachlorobiphenyl

R.T.: 8.110 min
Delta R.T.: 0.008 min
Response: 1488723
Conc: 4.16 ng/ml