

Data Path : P:\HPCHEM1\ECD_0\Data\P0032418\
Data File : P0043291.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Mar 2018 17:39
Operator : SM/UA
Sample : J1972-08RE
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
S-4 COMPRE

Manual Integrations
APPROVED

UGO
3/23/2018 7:30:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 17:57:47 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0032318.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 23 05:22:35 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.084	3.338	4199267	6316523	19.818m	21.580
2)	SA Decachlor...	9.444	8.108	1300490	1330499	5.355	3.720 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\P0032418\
Data File : P0043291.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Mar 2018 17:39
Operator : SM/UA
Sample : J1972-08RE
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
S-4 COMPRE


Manual Integrations
APPROVED

UGO
3/23/2018 7:30:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 17:57:47 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0032318.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 23 05:22:35 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

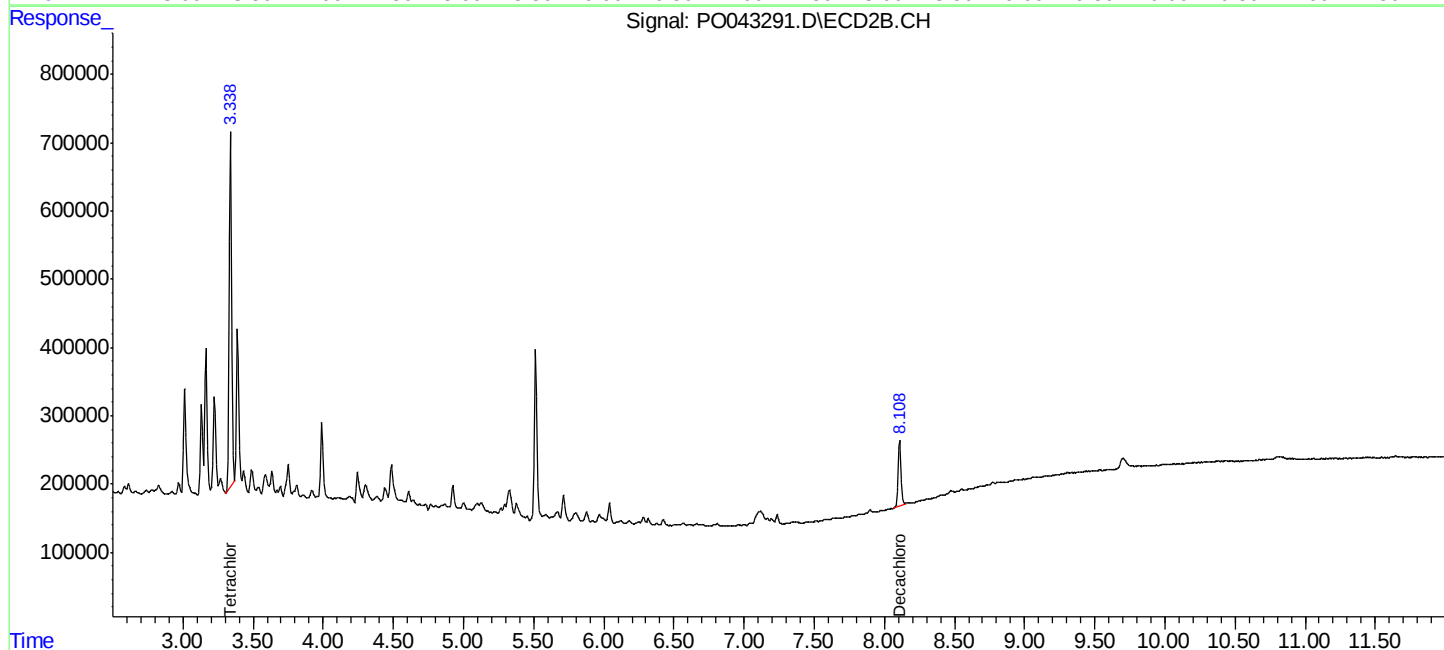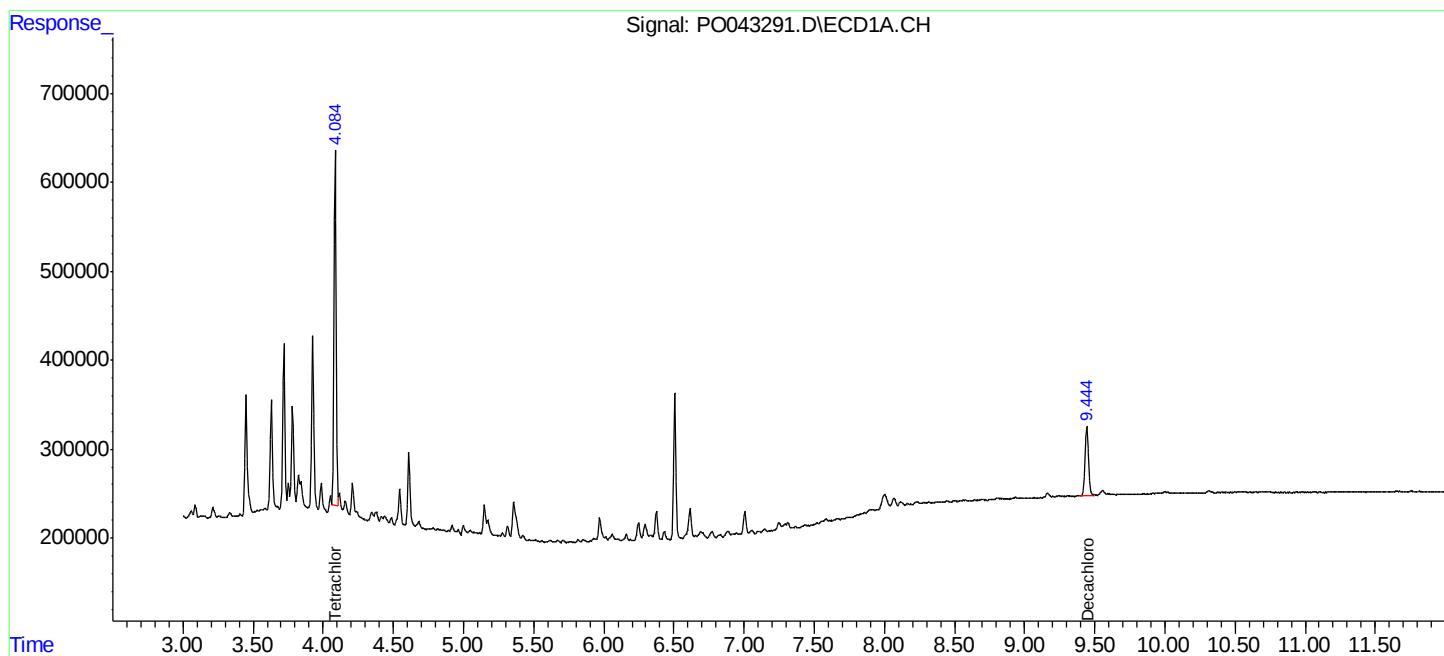

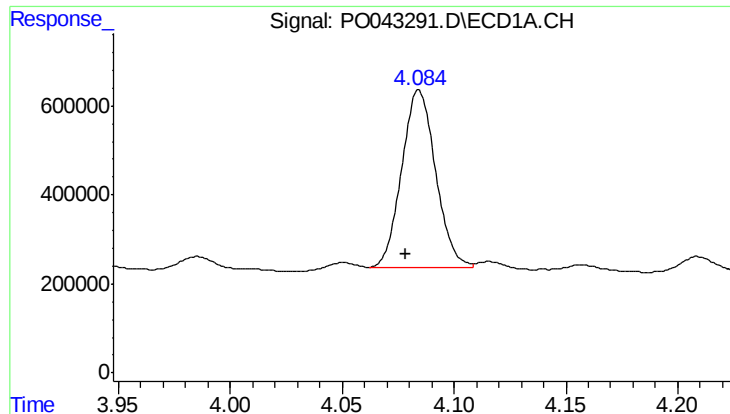


#1 Tetrachloro-m-xylene

R.T.: 4.084 min
Delta R.T.: 0.006 min
Response: 4199267
Conc: 19.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
S-4 COMPRE


Manual Integrations
APPROVED

UGO
3/23/2018 7:30:43 PM

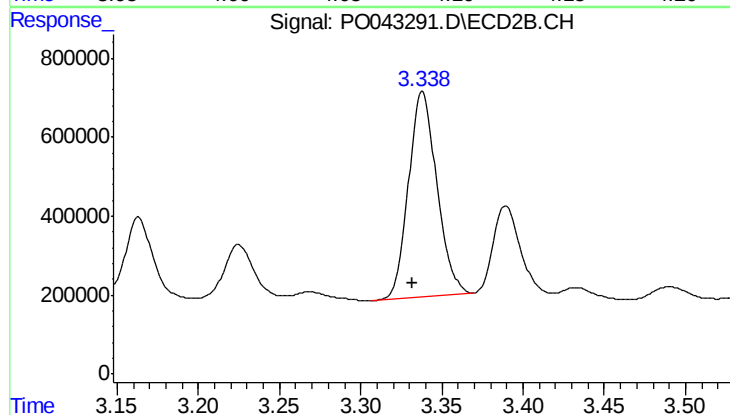


#1 Tetrachloro-m-xylene

R.T.: 3.338 min
Delta R.T.: 0.006 min
Response: 6316523
Conc: 21.58 ng/ml

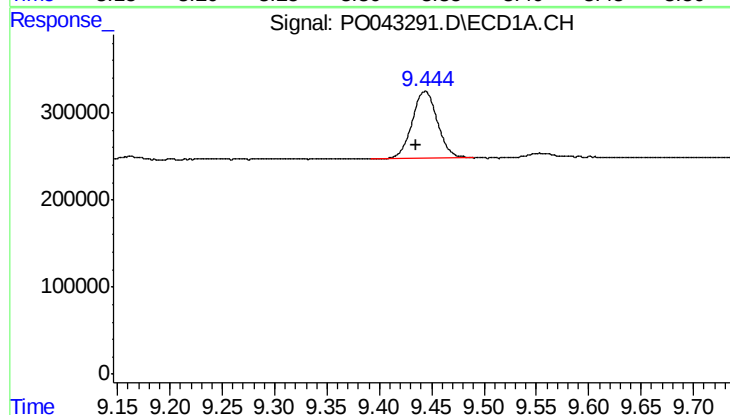

#2 Decachlorobiphenyl

R.T.: 9.444 min
Delta R.T.: 0.009 min
Response: 1300490
Conc: 5.35 ng/ml

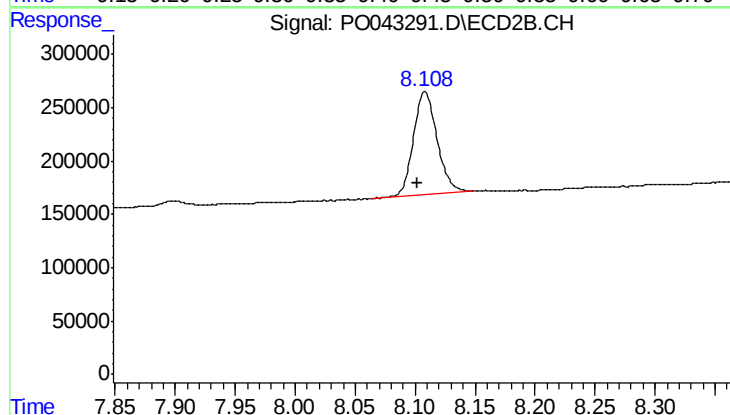

#2 Decachlorobiphenyl

R.T.: 8.108 min
Delta R.T.: 0.006 min
Response: 1330499
Conc: 3.72 ng/ml