

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032419\
 Data File : P0054547.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Mar 2019 15:33
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 05:31:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 05:05:57 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.308	3.626	659669	624867	18.881	18.857
2) SA Decachlor...	9.930	8.612	912141	641705	19.398	19.301
Target Compounds						
9) L2 AR-1221-2	0.000	3.925	0	9903	N.D.	31.498 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032419\
Data File : P0054547.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Mar 2019 15:33
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 05:31:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032319.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 05:05:57 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

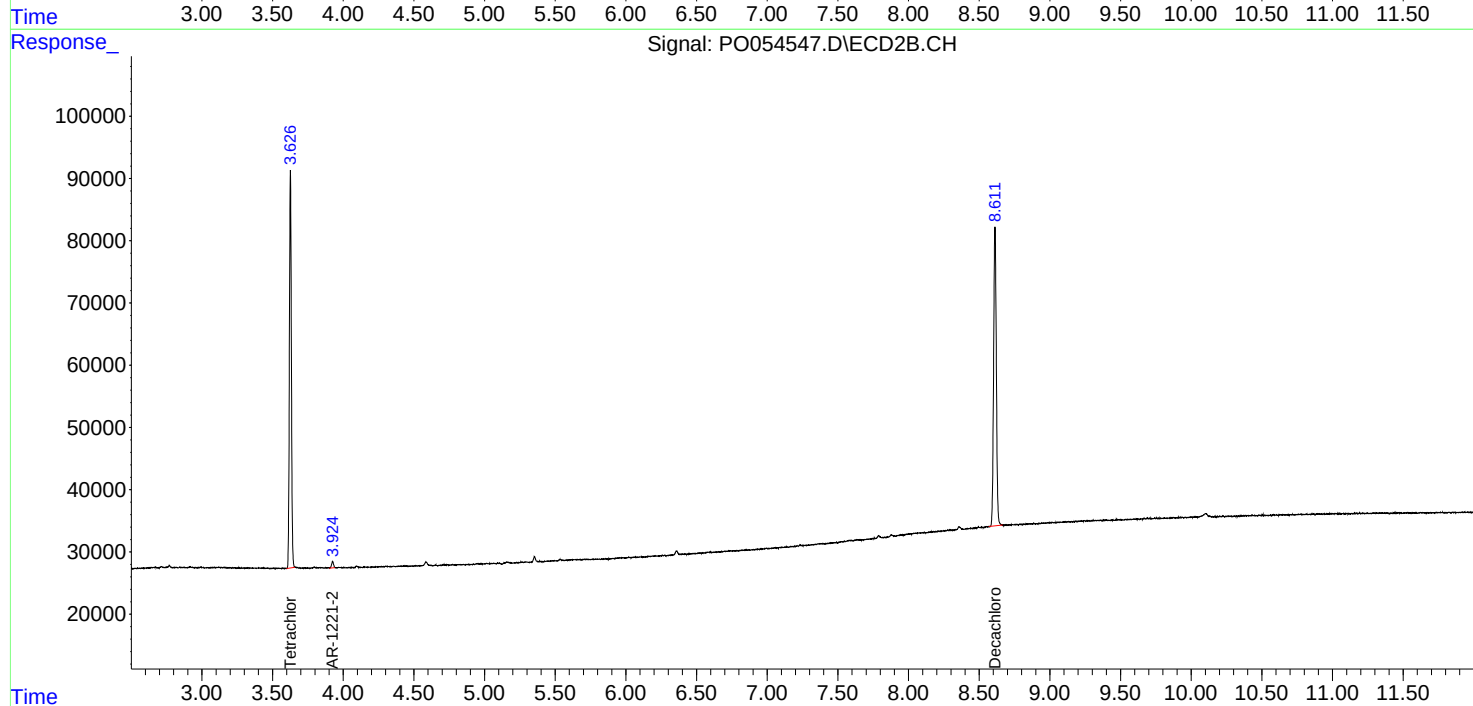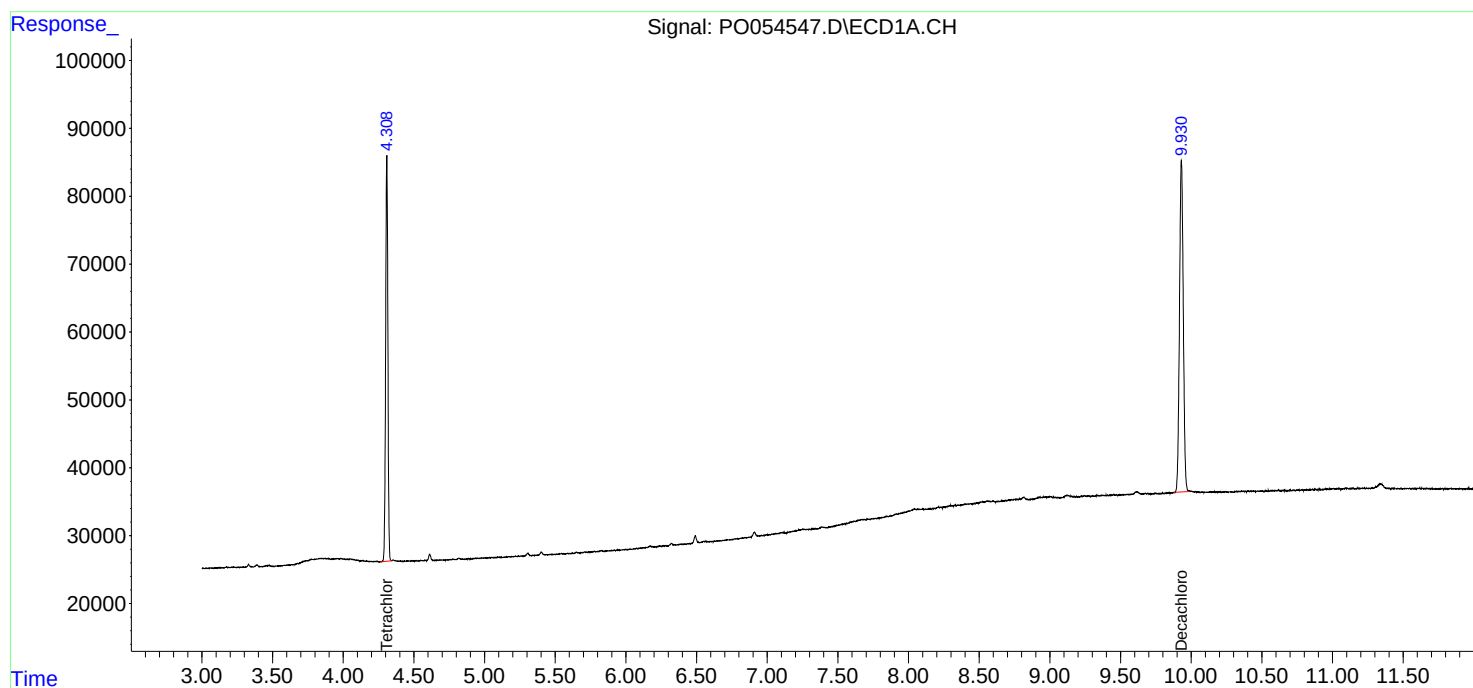


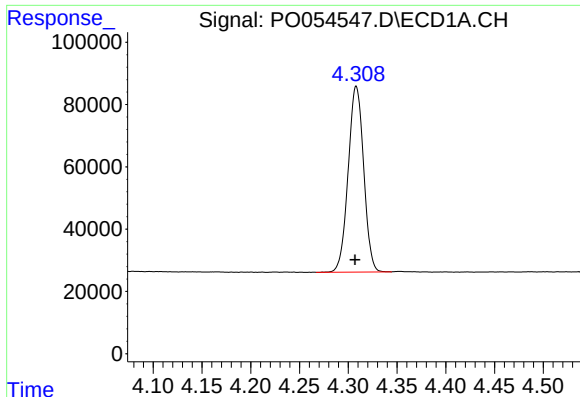

#1 Tetrachloro-m-xylene


R.T.: 4.308 min
Delta R.T.: 0.001 min
Response: 659669
Conc: 18.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

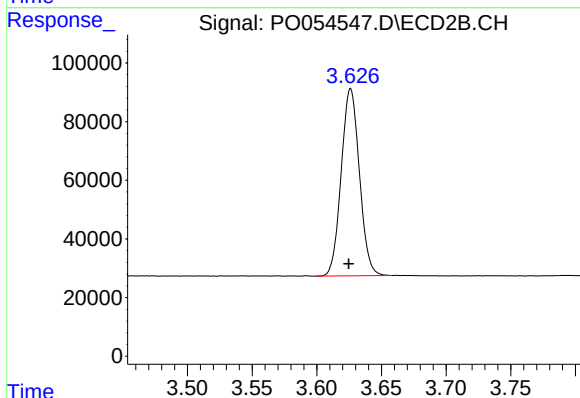


#1 Tetrachloro-m-xylene

R.T.: 3.626 min
Delta R.T.: 0.002 min
Response: 624867
Conc: 18.86 ng/ml

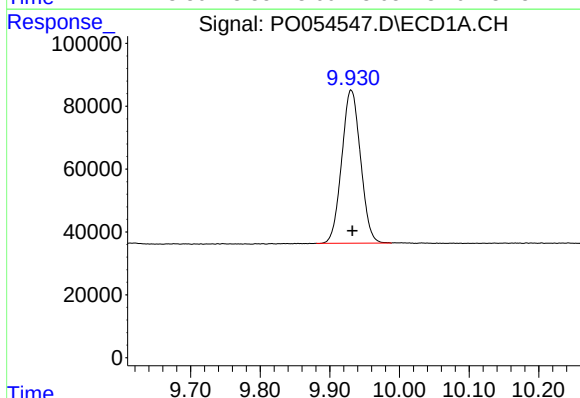


#2 Decachlorobiphenyl

R.T.: 9.930 min
Delta R.T.: -0.002 min
Response: 912141
Conc: 19.40 ng/ml

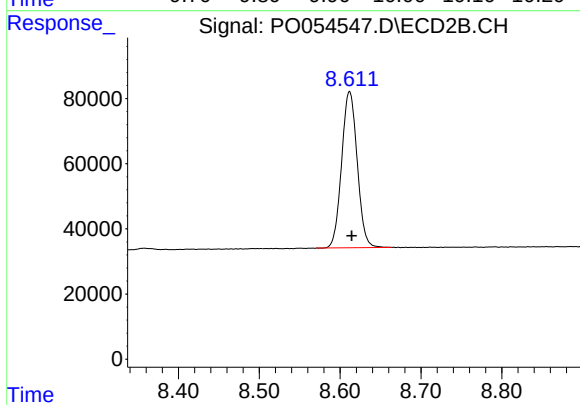

#2 Decachlorobiphenyl


R.T.: 8.612 min
Delta R.T.: -0.003 min
Response: 641705
Conc: 19.30 ng/ml

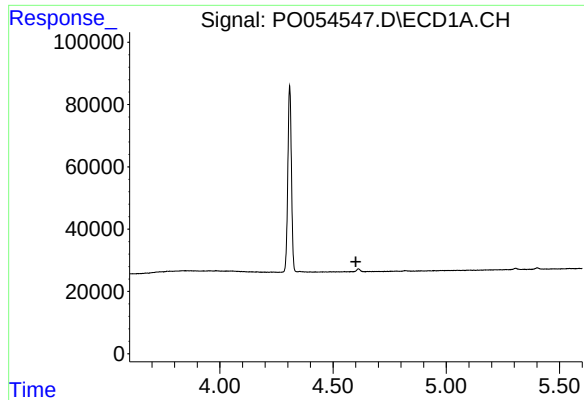

#9 AR-1221-2

R.T.: 0.000 min
Exp R.T.: 4.601 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

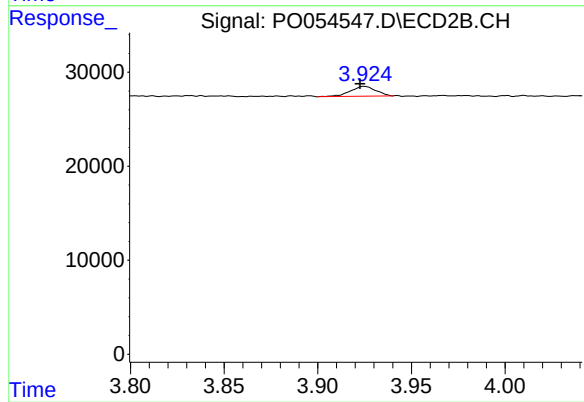

#9 AR-1221-2

R.T.: 3.925 min
Delta R.T.: 0.002 min
Response: 9903
Conc: 31.50 ng/ml