

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032419\
 Data File : P0054570.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Mar 2019 22:03
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 05:45:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 05:05:57 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.308	3.626	728792	687915	20.859	20.760
2)	SA Decachlor...	9.931	8.610	946560	658704	20.130	19.813
Target Compounds							
7)	L1 AR-1016-5	0.000	5.157	0	2623	N.D.	2.035 #
9)	L2 AR-1221-2	0.000	3.924	0	11012	N.D.	35.024 #
15)	L3 AR-1232-5	0.000	5.157	0	2623	N.D.	5.600 #
20)	L4 AR-1242-5	6.320	5.532	26364	10711	24.056	8.987 #
24)	L5 AR-1248-4	6.320	5.157	26364	2623	10.471	1.286 #
25)	L5 AR-1248-5	6.320	5.532	26364	10711	10.952	5.375 #
26)	L6 AR-1254-1	6.320	5.532	26364	10711	14.372	4.884 #
32)	L7 AR-1260-2	0.000	6.358	0	12420	N.D.	4.354 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO032419\
Data File : PO054570.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Mar 2019 22:03
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 05:45:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032319.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 05:05:57 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

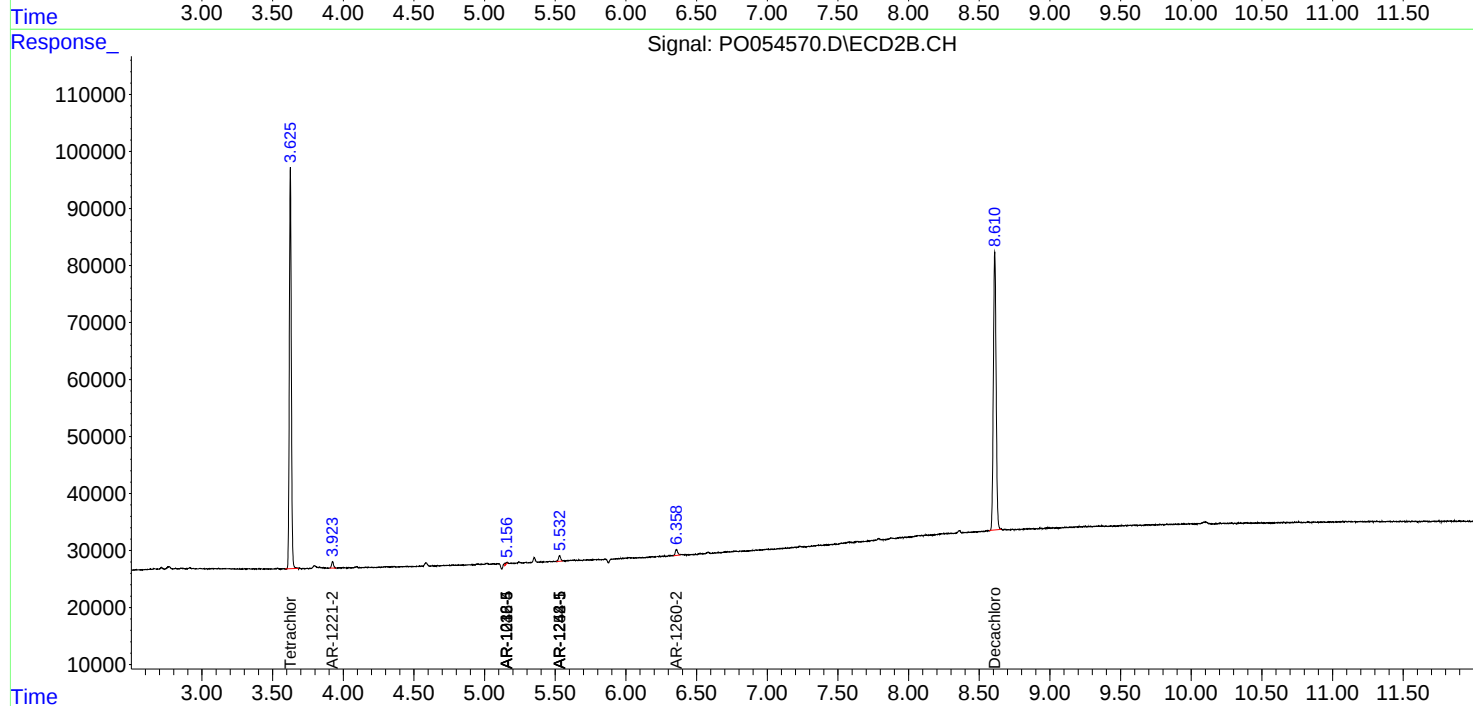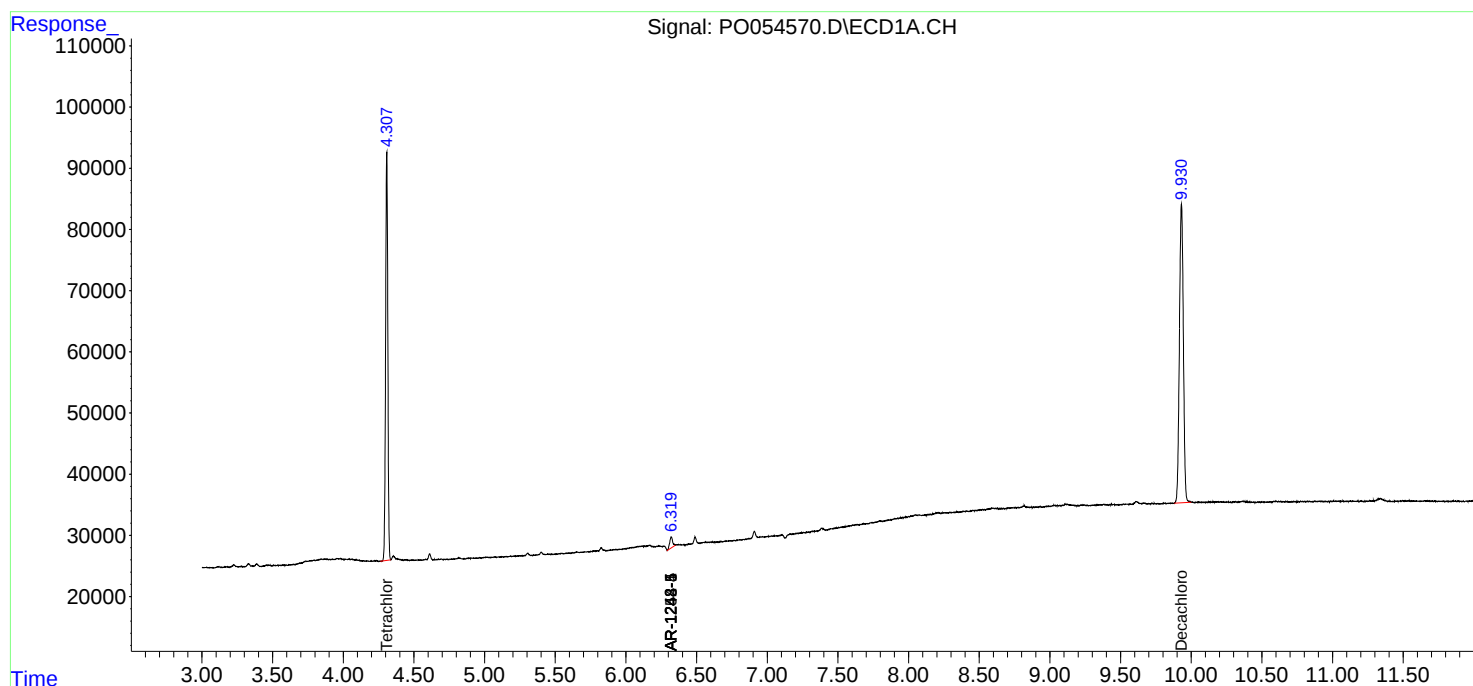


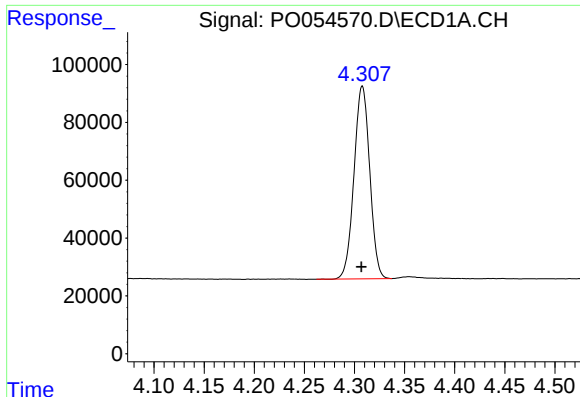

#1 Tetrachloro-m-xylene


R.T.: 4.308 min
Delta R.T.: 0.000 min
Response: 728792
Conc: 20.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

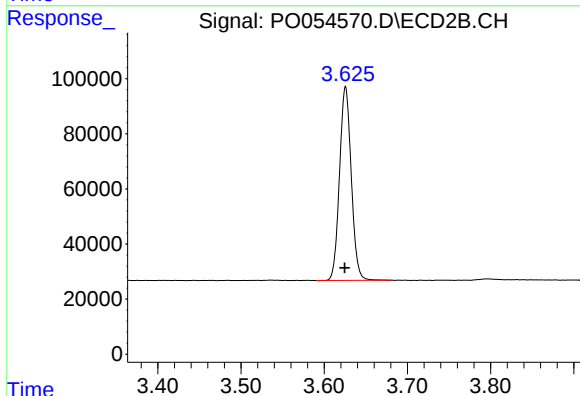


#1 Tetrachloro-m-xylene

R.T.: 3.626 min
Delta R.T.: 0.001 min
Response: 687915
Conc: 20.76 ng/ml

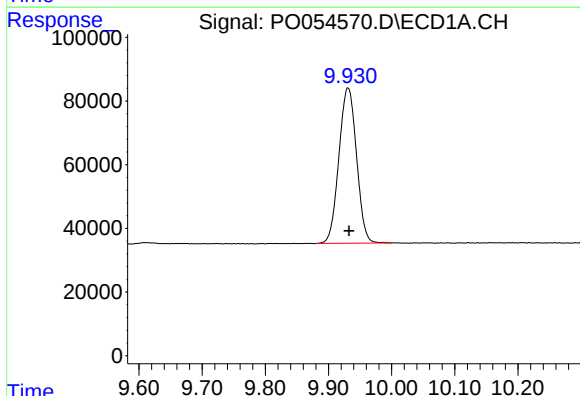


#2 Decachlorobiphenyl

R.T.: 9.931 min
Delta R.T.: -0.002 min
Response: 946560
Conc: 20.13 ng/ml

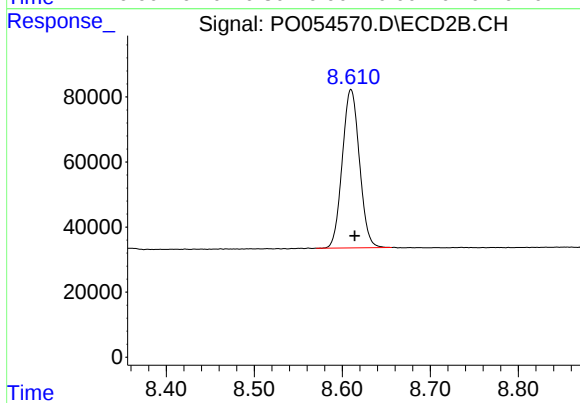

#2 Decachlorobiphenyl


R.T.: 8.610 min
Delta R.T.: -0.004 min
Response: 658704
Conc: 19.81 ng/ml

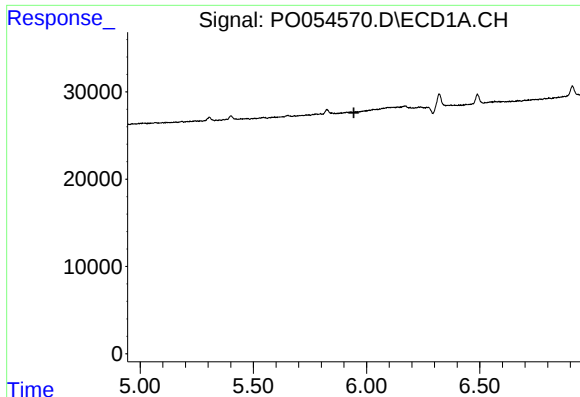

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 5.944 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

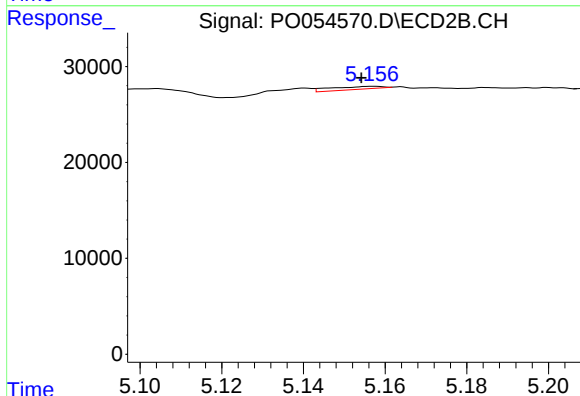


#7 AR-1016-5

R.T.: 5.157 min
Delta R.T.: 0.003 min
Response: 2623
Conc: 2.03 ng/ml

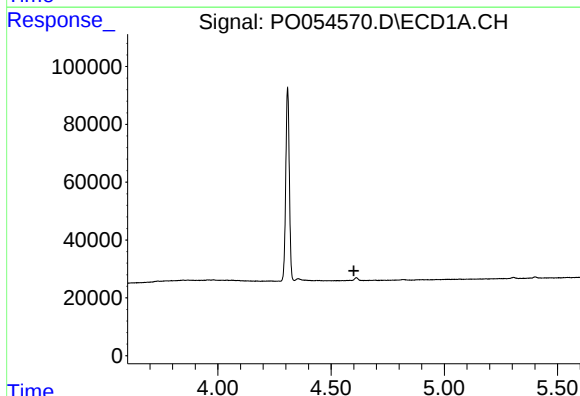


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T.: 4.601 min
Response: 0
Conc: N.D.

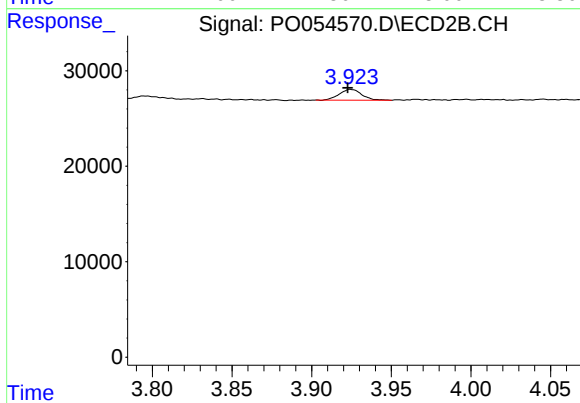

#9 AR-1221-2


R.T.: 3.924 min
Delta R.T.: 0.001 min
Response: 11012
Conc: 35.02 ng/ml

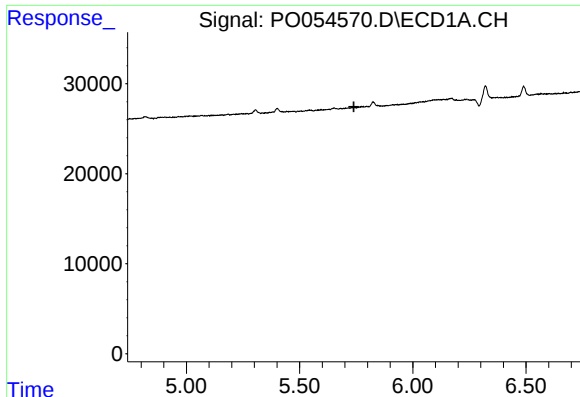

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T.: 5.740 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

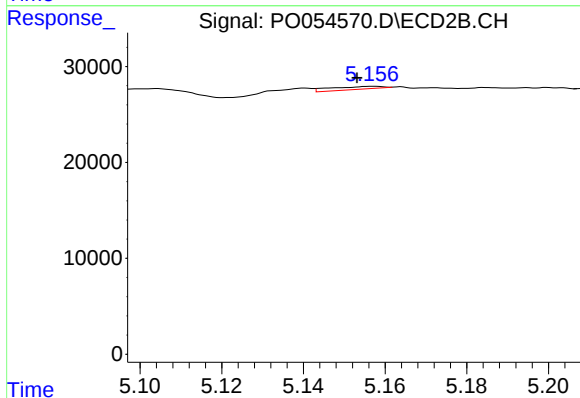


#15 AR-1232-5

R.T.: 5.157 min
Delta R.T.: 0.004 min
Response: 2623
Conc: 5.60 ng/ml

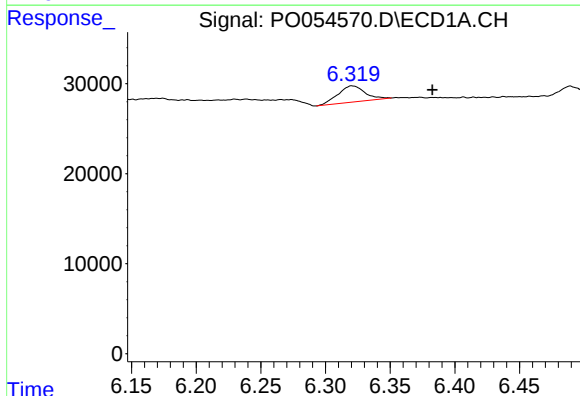


#20 AR-1242-5

R.T.: 6.320 min
Delta R.T.: -0.062 min
Response: 26364
Conc: 24.06 ng/ml

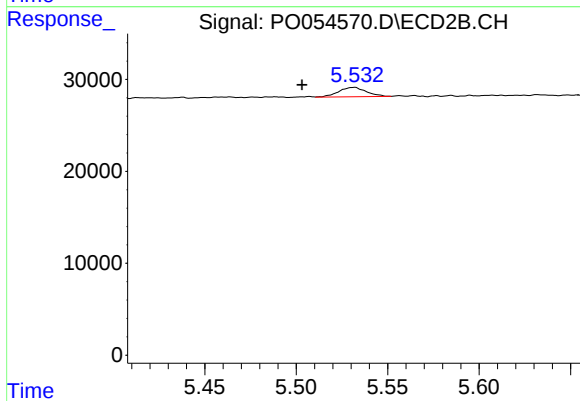

#20 AR-1242-5


R.T.: 5.532 min
Delta R.T.: 0.029 min
Response: 10711
Conc: 8.99 ng/ml

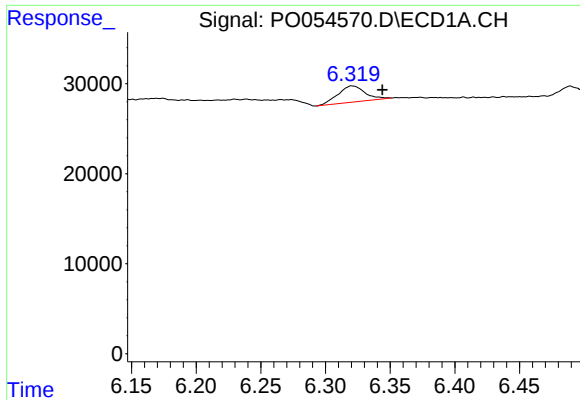

#24 AR-1248-4


R.T.: 6.320 min
Delta R.T.: -0.024 min
Response: 26364
Conc: 10.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

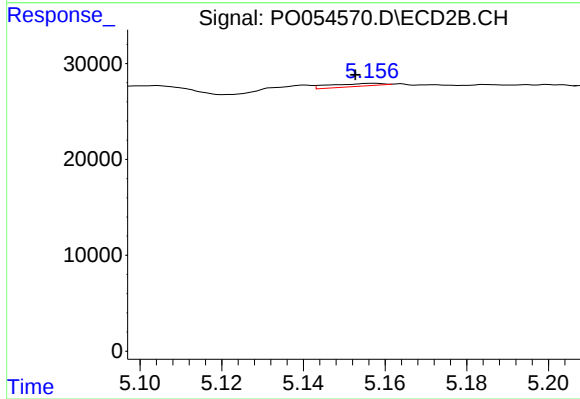


#24 AR-1248-4

R.T.: 5.157 min
Delta R.T.: 0.004 min
Response: 2623
Conc: 1.29 ng/ml

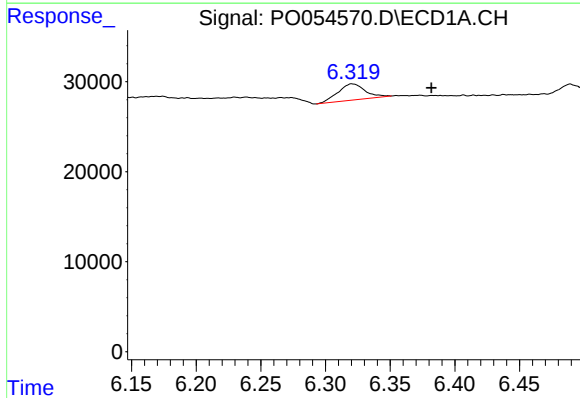


#25 AR-1248-5

R.T.: 6.320 min
Delta R.T.: -0.062 min
Response: 26364
Conc: 10.95 ng/ml

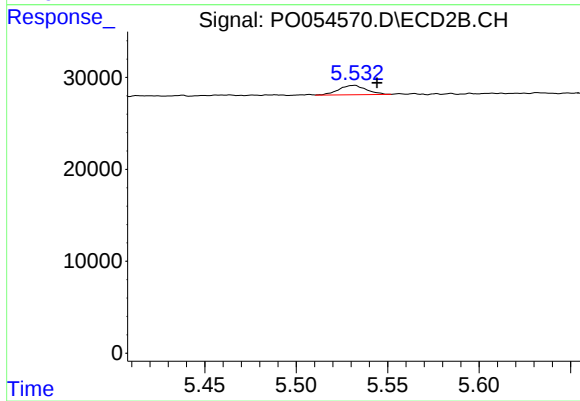

#25 AR-1248-5


R.T.: 5.532 min
Delta R.T.: -0.012 min
Response: 10711
Conc: 5.37 ng/ml

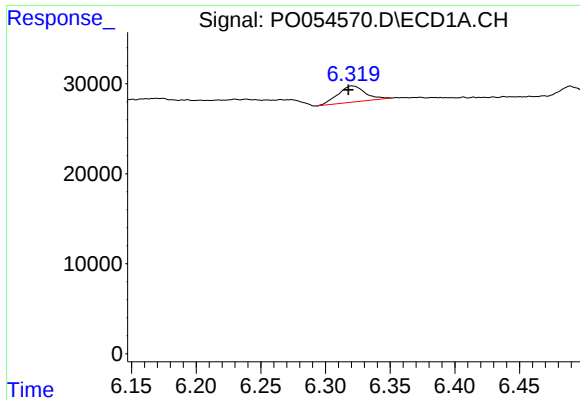

#26 AR-1254-1


R.T.: 6.320 min
Delta R.T.: 0.003 min
Response: 26364
Conc: 14.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

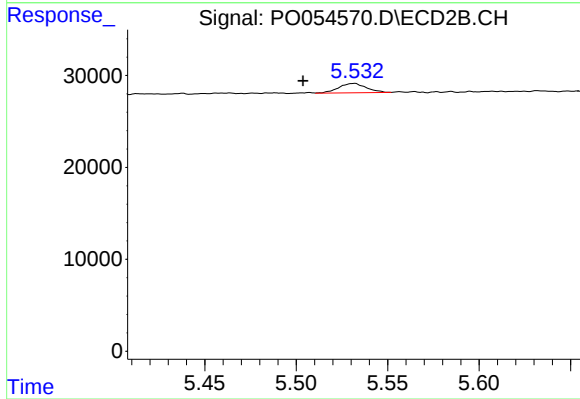


#26 AR-1254-1

R.T.: 5.532 min
Delta R.T.: 0.028 min
Response: 10711
Conc: 4.88 ng/ml

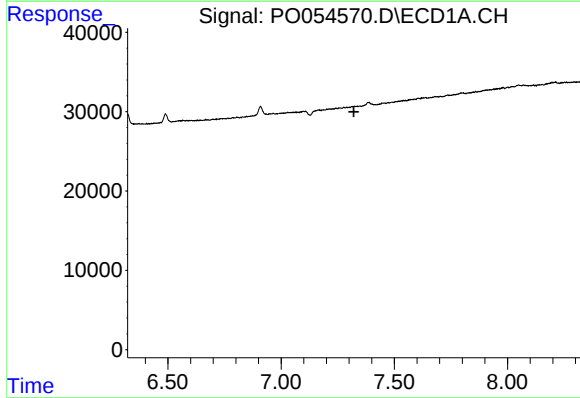

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.322 min
Response: 0
Conc: N.D.

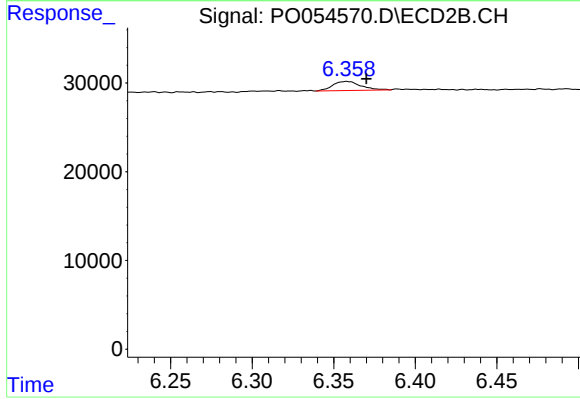

#32 AR-1260-2

R.T.: 6.358 min
Delta R.T.: -0.012 min
Response: 12420
Conc: 4.35 ng/ml